

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012838.D
 Acq On : 29 Nov 2022 03:54
 Operator : CG/JU
 Sample : N5666-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	33	rBV	118518	173987	1.12%	0.117%
2	3.399	33	36	39	rVV	117611	167694	1.08%	0.113%
3	3.434	39	42	51	rVB	205402	274521	1.77%	0.184%
4	3.822	105	108	125	rBV	508408	821958	5.30%	0.552%
5	4.064	144	149	154	rVB	66788	102593	0.66%	0.069%
6	4.158	161	165	171	rVB	46557	67641	0.44%	0.045%
7	5.105	321	326	334	rVB2	24343	41555	0.27%	0.028%
8	7.163	668	676	685	rVB	659674	1045894	6.74%	0.703%
9	7.334	698	705	715	rBV	2227259	3515644	22.66%	2.362%
10	7.540	732	740	750	rBV	2102070	3239249	20.88%	2.176%
11	7.628	750	755	761	rVB4	18938	40087	0.26%	0.027%
12	8.016	811	821	828	rBV	2158474	3488288	22.49%	2.344%
13	8.075	828	831	837	rVB2	17667	25747	0.17%	0.017%
14	8.716	933	940	952	rBV	1811153	2898721	18.69%	1.948%
15	9.093	998	1004	1011	rBV	45579	79948	0.52%	0.054%
16	9.181	1011	1019	1026	rBV	2481909	3986125	25.70%	2.678%
17	9.275	1031	1035	1044	rVV6	20543	54867	0.35%	0.037%
18	9.375	1047	1052	1061	rVB2	49311	94113	0.61%	0.063%
19	9.487	1066	1071	1078	rBV6	12504	32247	0.21%	0.022%
20	9.563	1078	1084	1087	rVV	21680	42252	0.27%	0.028%
21	9.599	1087	1090	1095	rVV3	32419	47552	0.31%	0.032%
22	9.728	1110	1112	1119	rVB8	10699	18323	0.12%	0.012%
23	9.904	1133	1142	1153	rVV	1896371	3121832	20.12%	2.098%
24	10.104	1172	1176	1182	rVB7	9965	17381	0.11%	0.012%
25	10.228	1192	1197	1209	rVB	28357	53993	0.35%	0.036%
26	10.440	1225	1233	1247	rBV	3102089	5044546	32.52%	3.389%
27	10.828	1291	1299	1306	rBV	3283820	5538120	35.70%	3.721%
28	10.887	1306	1309	1314	rVV3	44491	66365	0.43%	0.045%
29	10.963	1314	1322	1338	rVV	2143825	3650374	23.53%	2.453%
30	11.187	1355	1360	1368	rBV	11128	23979	0.15%	0.016%
31	11.481	1405	1410	1419	rVB	7924	19733	0.13%	0.013%
32	11.746	1446	1455	1458	rVB10	11855	19514	0.13%	0.013%
33	11.940	1482	1488	1499	rBV	160416	325427	2.10%	0.219%
34	12.093	1506	1514	1520	rBV	11518	24069	0.16%	0.016%
35	12.240	1534	1539	1544	rVB2	38443	55082	0.36%	0.037%
36	12.404	1559	1567	1572	rVV2	61778	128483	0.83%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012838.D
 Acq On : 29 Nov 2022 03:54
 Operator : CG/JU
 Sample : N5666-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	12.446	1572	1574	1582	rVB9	13365	23420	0.15%	0.016%
38	12.687	1609	1615	1618	rBV7	9076	16174	0.10%	0.011%
39	12.869	1640	1646	1650	rBV8	14241	27389	0.18%	0.018%
40	13.045	1672	1676	1683	rVB9	13440	31638	0.20%	0.021%
41	13.134	1686	1691	1697	rVV9	11793	22104	0.14%	0.015%
42	13.187	1697	1700	1705	rVB3	14214	20317	0.13%	0.014%
43	13.387	1728	1734	1739	rBV8	14854	25381	0.16%	0.017%
44	13.469	1743	1748	1753	rVV	60396	91008	0.59%	0.061%
45	13.540	1755	1760	1767	rVB	72461	129154	0.83%	0.087%
46	13.622	1768	1774	1778	rVV5	15254	29243	0.19%	0.020%
47	13.987	1831	1836	1838	rBV6	9076	16021	0.10%	0.011%
48	14.051	1840	1847	1858	rBV	5898475	8404716	54.18%	5.647%
49	14.169	1864	1867	1873	rVB8	18693	31157	0.20%	0.021%
50	14.345	1884	1897	1909	rBV	7105667	10563252	68.10%	7.097%
51	14.540	1924	1930	1936	rVB4	15527	35682	0.23%	0.024%
52	14.651	1939	1949	1957	rBV	5294771	7941576	51.20%	5.336%
53	14.828	1971	1979	1987	rBV	469600	732887	4.72%	0.492%
54	15.051	2012	2017	2023	rVB3	66078	107261	0.69%	0.072%
55	15.398	2069	2076	2079	rBV9	9518	15969	0.10%	0.011%
56	15.463	2085	2087	2096	rVB7	18004	32804	0.21%	0.022%
57	15.575	2103	2106	2110	rBV2	16292	25374	0.16%	0.017%
58	15.639	2111	2117	2129	rVV	9341800	13377388	86.24%	8.988%
59	15.751	2129	2136	2143	rVV	2375120	3235528	20.86%	2.174%
60	15.804	2143	2145	2148	rVV2	40307	57133	0.37%	0.038%
61	15.845	2149	2152	2155	rVV4	43101	76421	0.49%	0.051%
62	15.881	2155	2158	2165	rVB5	40120	66292	0.43%	0.045%
63	16.004	2172	2179	2185	rVB2	144622	230027	1.48%	0.155%
64	16.092	2190	2194	2198	rVV	76357	116812	0.75%	0.078%
65	16.134	2198	2201	2211	rVB3	69461	157238	1.01%	0.106%
66	16.339	2231	2236	2237	rBV4	14303	24996	0.16%	0.017%
67	16.492	2259	2262	2266	rVB5	18981	21241	0.14%	0.014%
68	16.557	2266	2273	2278	rBV2	500478	765310	4.93%	0.514%
69	16.675	2288	2293	2297	rBV	119062	158491	1.02%	0.106%
70	16.881	2324	2328	2331	rBV5	18061	22475	0.14%	0.015%
71	16.928	2332	2336	2340	rVV	43134	58667	0.38%	0.039%
72	17.198	2376	2382	2389	rBV3	150720	281372	1.81%	0.189%
73	17.269	2389	2394	2405	rVV	342746	544345	3.51%	0.366%
74	17.404	2411	2417	2424	rVB	6445371	9135670	58.89%	6.138%
75	17.504	2427	2434	2445	rBV	10115368	14396836	92.81%	9.673%
76	17.586	2445	2448	2450	rBV4	25935	30359	0.20%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012838.D
 Acq On : 29 Nov 2022 03:54
 Operator : CG/JU
 Sample : N5666-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

77	17.716	2466	2470	2475	rVB4	22167	34143	0.22%	0.023%
78	17.775	2477	2480	2483	rBV2	13997	21788	0.14%	0.015%
79	18.269	2560	2564	2575	rBV	268457	389782	2.51%	0.262%
80	18.457	2592	2596	2604	rVB2	27414	51581	0.33%	0.035%
81	18.686	2631	2635	2639	rBV6	36539	45726	0.29%	0.031%
82	19.304	2737	2740	2746	rVB	111141	148811	0.96%	0.100%
83	19.375	2747	2752	2753	rVV	112301	153465	0.99%	0.103%
84	19.404	2753	2757	2763	rVB	299982	428017	2.76%	0.288%
85	19.498	2770	2773	2780	rBV4	109625	145806	0.94%	0.098%
86	19.645	2795	2798	2803	rVB4	50162	61101	0.39%	0.041%
87	19.727	2806	2812	2825	rBV	11952976	15512312	100.00%	10.423%
88	21.180	3056	3059	3065	rBV3	170455	206657	1.33%	0.139%
89	21.486	3106	3111	3121	rBV	5396309	7049697	45.45%	4.737%
90	23.833	3503	3510	3528	rVB2	4563290	9434508	60.82%	6.339%
91	23.998	3531	3538	3553	rVB2	2751753	5721348	36.88%	3.844%




Sum of corrected areas: 148831774

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012838.D
Acq On : 29 Nov 2022 03:54
Operator : CG/JU
Sample : N5666-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

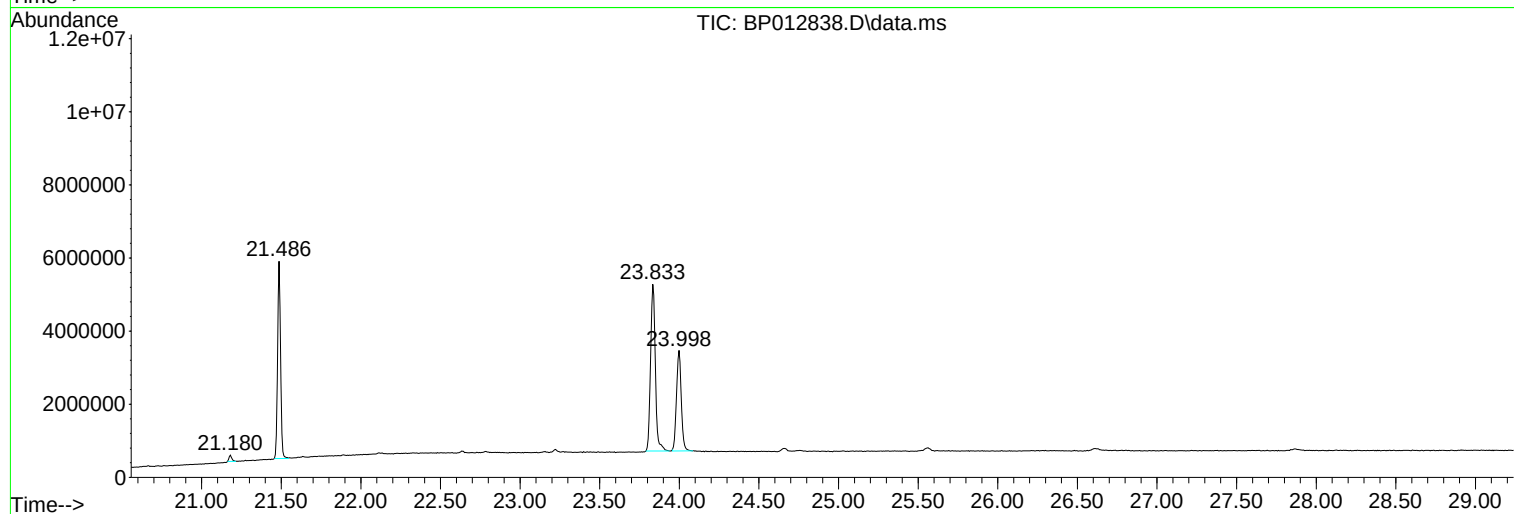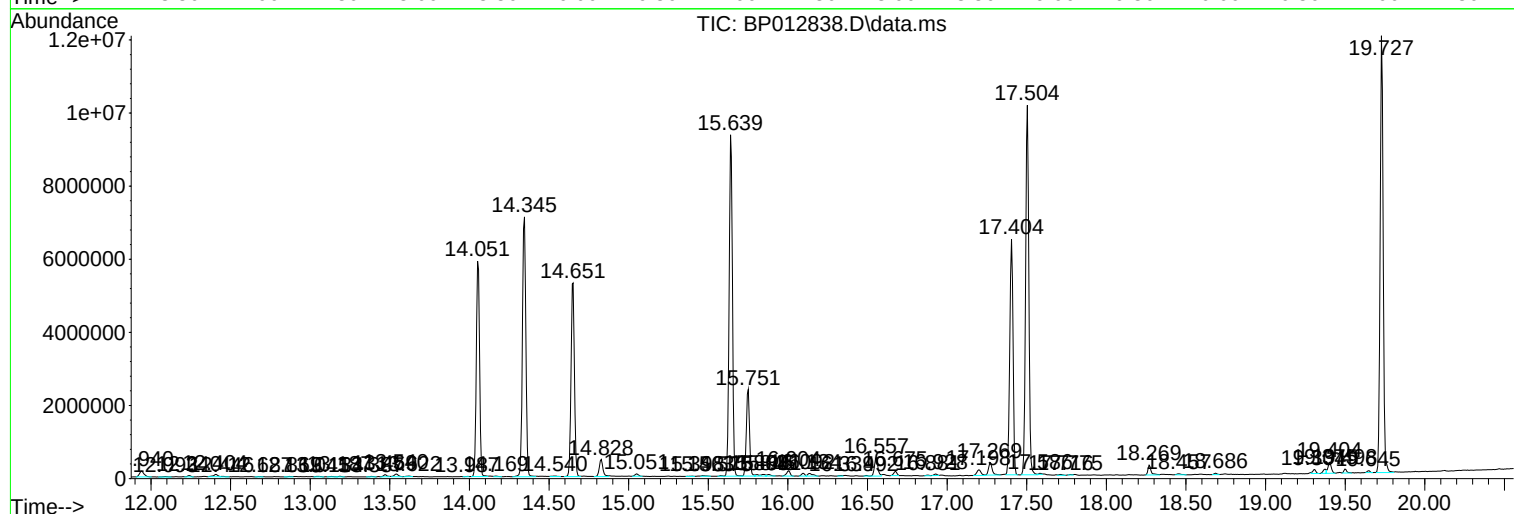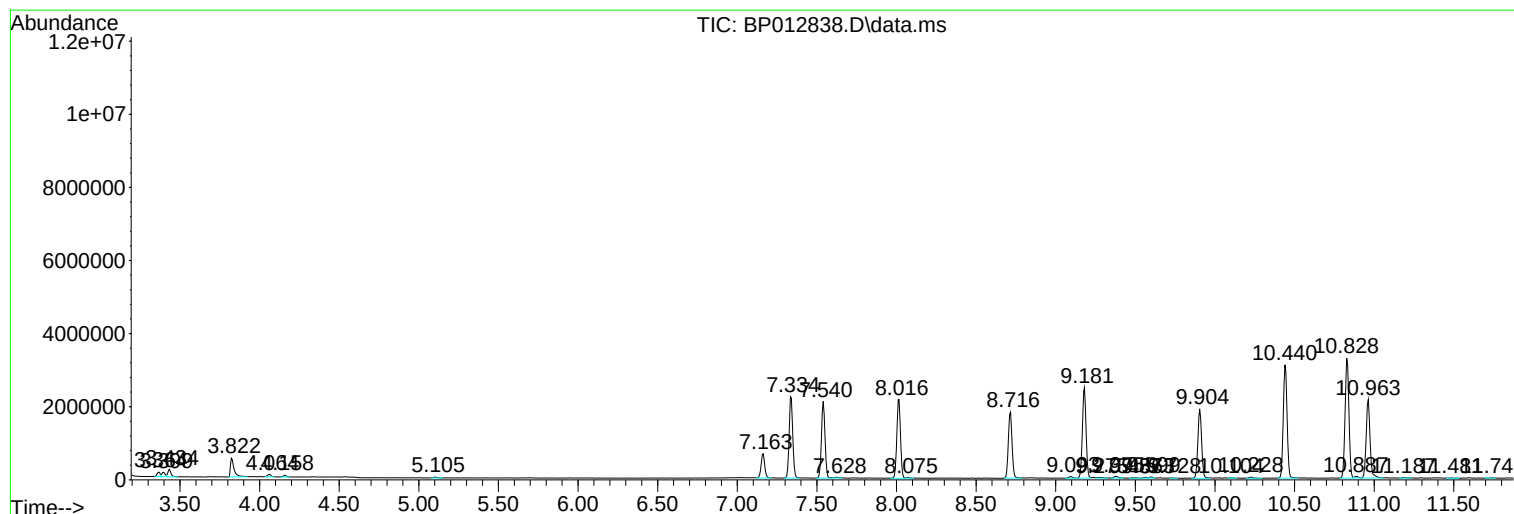

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012838.D
Acq On : 29 Nov 2022 03:54
Operator : CG/JU
Sample : N5666-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012838.D
Acq On : 29 Nov 2022 03:54
Operator : CG/JU
Sample : N5666-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc