

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012877.D
 Acq On : 30 Nov 2022 13:48
 Operator : CG/JU
 Sample : N5811-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCE0

Quant Time: Nov 30 21:54:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	568326	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	2673228	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	1875481	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	4173163	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	3782070	20.000	ng/ul	0.00
88) Perylene-d12	23.998	264	3304251	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	50679	3.821	ng/uL	0.00
4) Pyridine-d5	3.822	84	240786	6.067	ng/ul	0.00
7) Phenol-d5	7.158	99	213526	4.572	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	694191	24.123	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	653754	18.371	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	433805	11.529	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	419874	25.662	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	440944	25.381	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	828002	20.426	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	1100261	19.821	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3532180	27.362	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	3638306	24.155	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	73727	3.203	ng/ul	0.00
60) Fluorene-d10	15.640	176	3218648	28.470	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	457239	22.924	ng/ul	0.00
73) Anthracene-d10	17.498	188	5757783	31.344	ng/ul	0.00
81) Pyrene-d10	19.728	212	6582158	29.952	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.833	264	5046872	31.096	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.380	149	680987	6.731	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012877.D
Acq On : 30 Nov 2022 13:48
Operator : CG/JU
Sample : N5811-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCE0

Quant Time: Nov 30 21:54:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

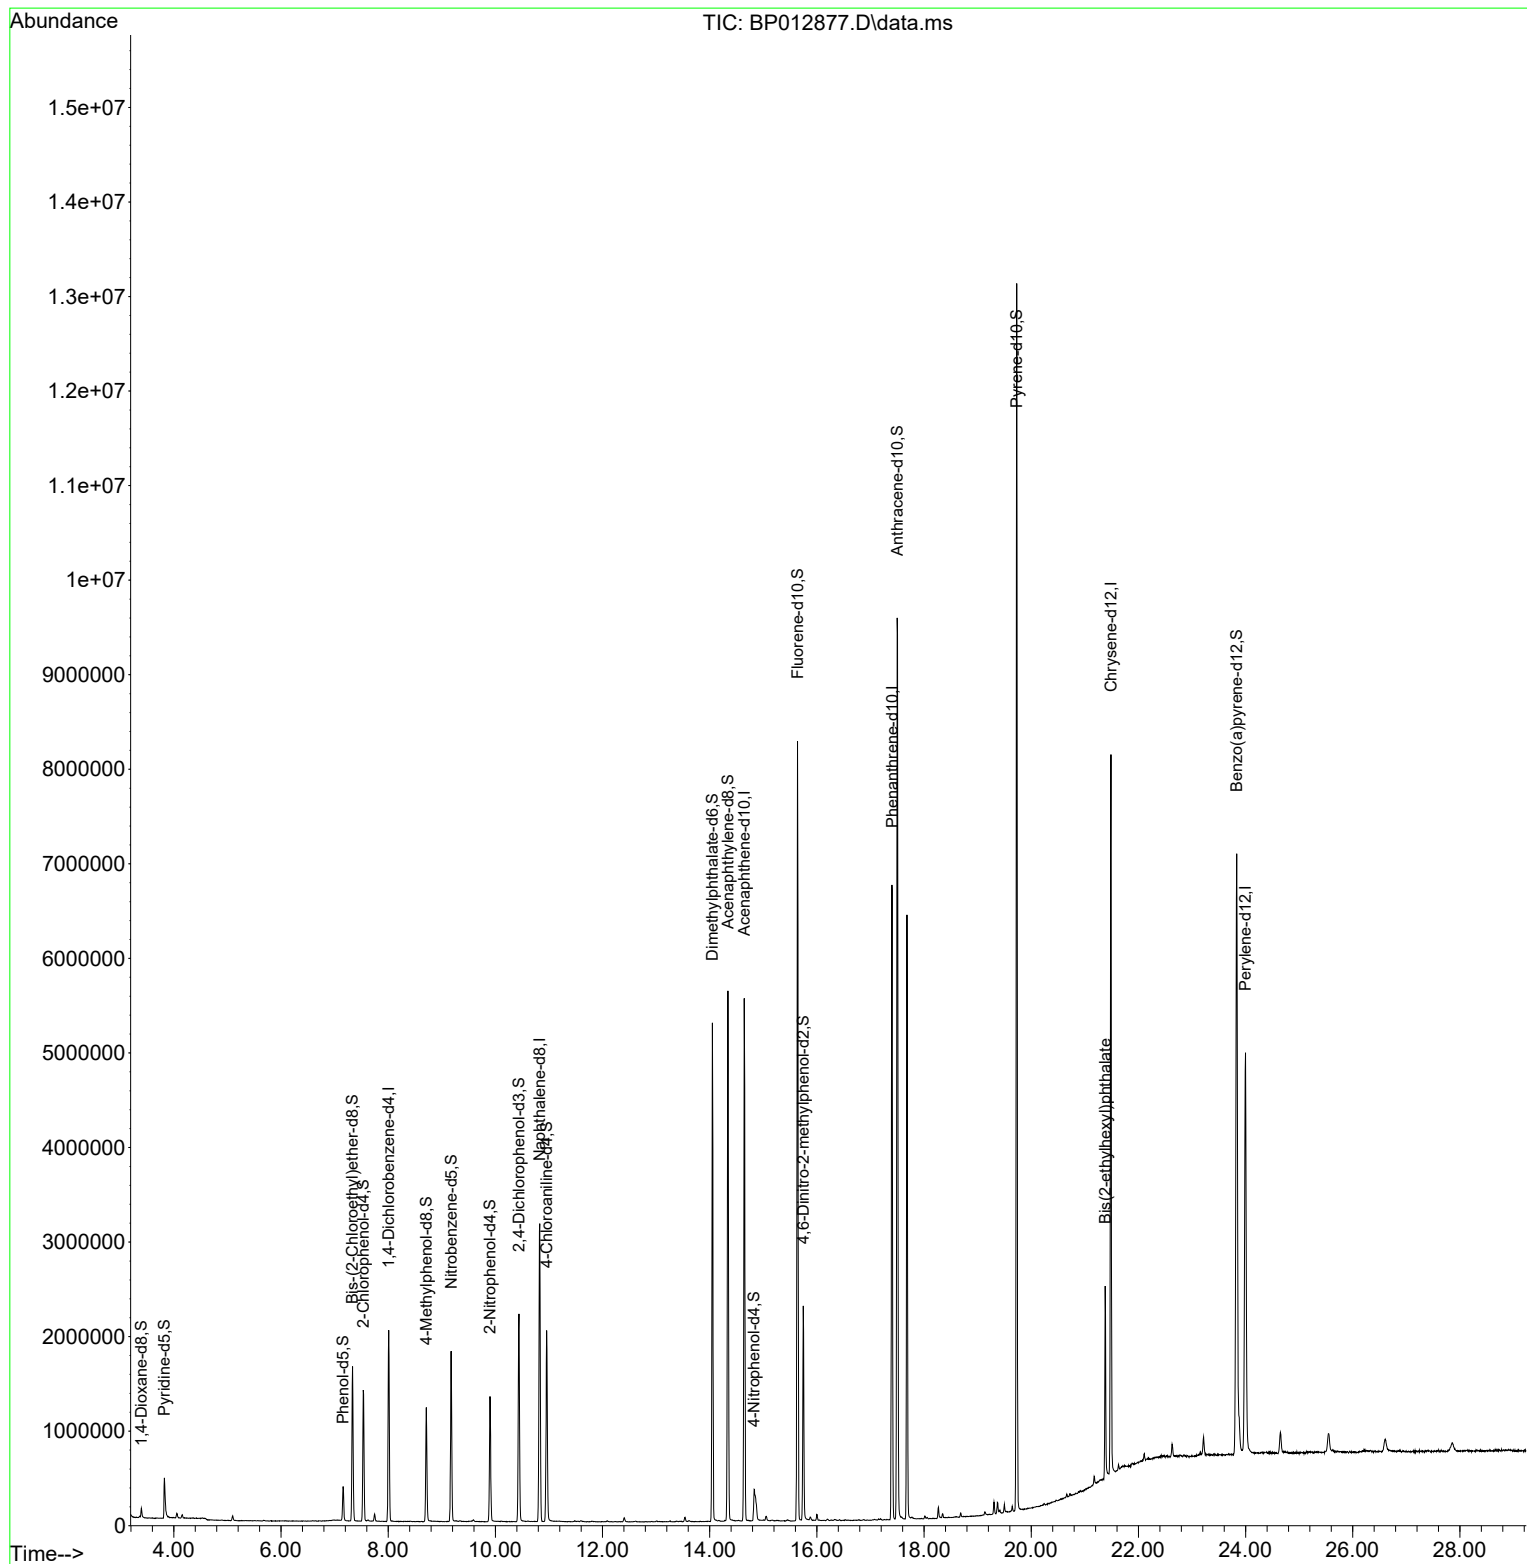

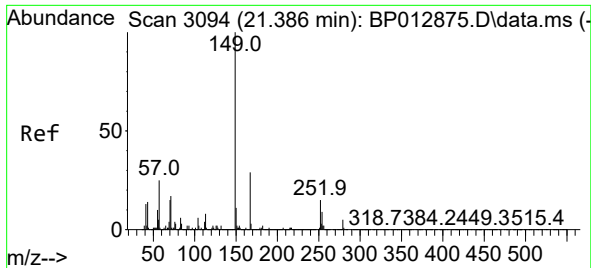

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 6.731 ng/ul
 RT: 21.380 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP012877.D
 Acq: 30 Nov 2022 13:48

Instrument :
 BNA_P
 ClientSampleId :
 BGCE0

Tgt Ion:149 Resp: 680987
 Ion Ratio Lower Upper
 149 100
 167 27.1 22.7 34.1
 279 3.9 3.8 5.6

