

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012888.D
 Acq On : 30 Nov 2022 20:39
 Operator : CG/JU
 Sample : N5759-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB76

Quant Time: Nov 30 21:57:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	517522	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2390788	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.646	164	1624919	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3413476	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	2425477	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	1972431	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	65865	5.454	ng/uL	0.00
4) Pyridine-d5	3.823	84	322481	8.923	ng/u1	0.00
7) Phenol-d5	7.158	99	376514	8.854	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	998716	38.112	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	954204	29.447	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	693267	20.233	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	611022	41.756	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	623196	40.109	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	1173078	32.358	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	738050	14.867	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	4327938	38.695	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	4905443	37.589	ng/u1	0.00
54) 4-Nitrophenol-d4	14.822	143	91405	4.584	ng/u1	0.00
60) Fluorene-d10	15.640	176	3849508	39.300	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.746	200	487183	29.862	ng/u1	0.00
73) Anthracene-d10	17.498	188	5968864	39.724	ng/u1	0.00
81) Pyrene-d10	19.728	212	6306386	44.747	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	3866794	39.912	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.429	88	120200	9.267	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012888.D
Acq On : 30 Nov 2022 20:39
Operator : CG/JU
Sample : N5759-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB76

Quant Time: Nov 30 21:57:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

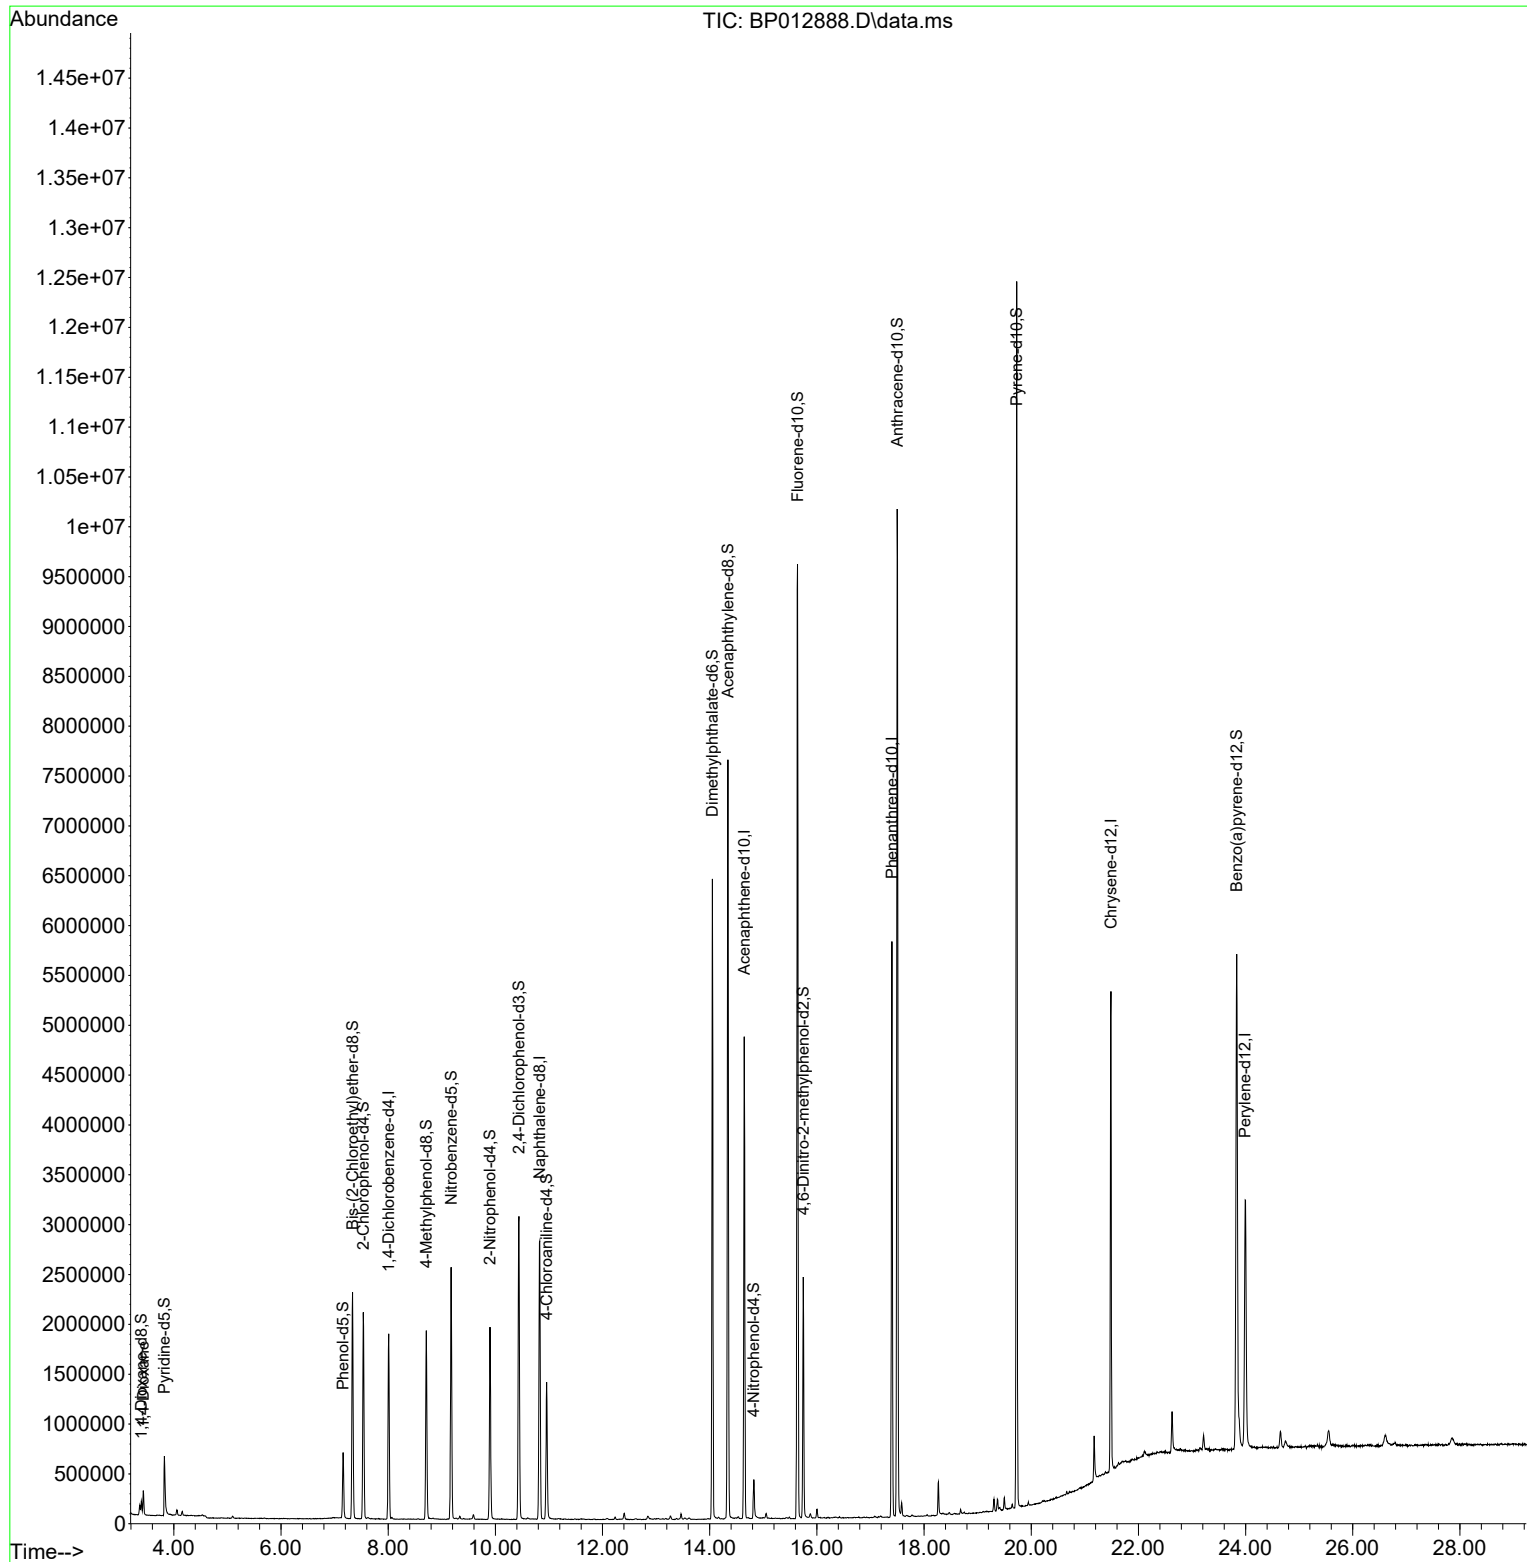

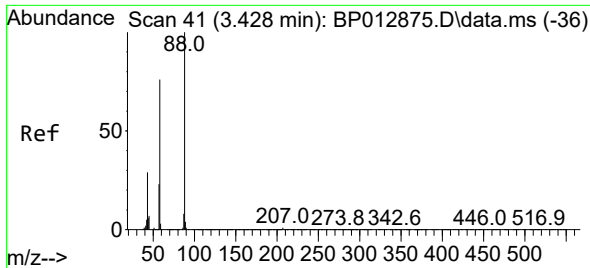

#2
 1,4-Dioxane
 Concen: 9.267 ng/uL
 RT: 3.429 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012888.D
 Acq: 30 Nov 2022 20:39

Instrument :
 BNA_P
 ClientSampleId :
 BHB76

Tgt Ion: 88 Resp: 120200
 Ion Ratio Lower Upper
 88 100
 43 27.9 22.6 34.0
 58 73.9 59.6 89.4

