

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012915.D
 Acq On : 01 Dec 2022 13:09
 Operator : CG/JU
 Sample : N5737-01DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4345DL

Quant Time: Dec 01 21:37:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	551031	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	2447938	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	1547418	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2824860	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	2224060	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	2290176	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	5474	0.426	ng/uL	0.00
4) Pyridine-d5	3.828	84	62574	1.626	ng/u1	0.01
7) Phenol-d5	7.158	99	45741	1.010	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	158861	5.694	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	139736	4.050	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	90085	2.469	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	84900	5.667	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	79281	4.983	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	168365	4.536	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	189306	3.724	ng/u1	0.00
46) Dimethylphthalate-d6	14.046	166	642899	6.036	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	667534	5.371	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	5730	0.302	ng/u1	0.00
60) Fluorene-d10	15.634	176	558684	5.989	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	33607	2.489	ng/u1	0.00
73) Anthracene-d10	17.492	188	739370	5.946	ng/u1	-0.01
81) Pyrene-d10	19.722	212	780536	6.040	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.822	264	650880	5.786	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.428	88	163407	11.832	ng/uL 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012915.D
Acq On : 01 Dec 2022 13:09
Operator : CG/JU
Sample : N5737-01DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4345DL

Quant Time: Dec 01 21:37:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

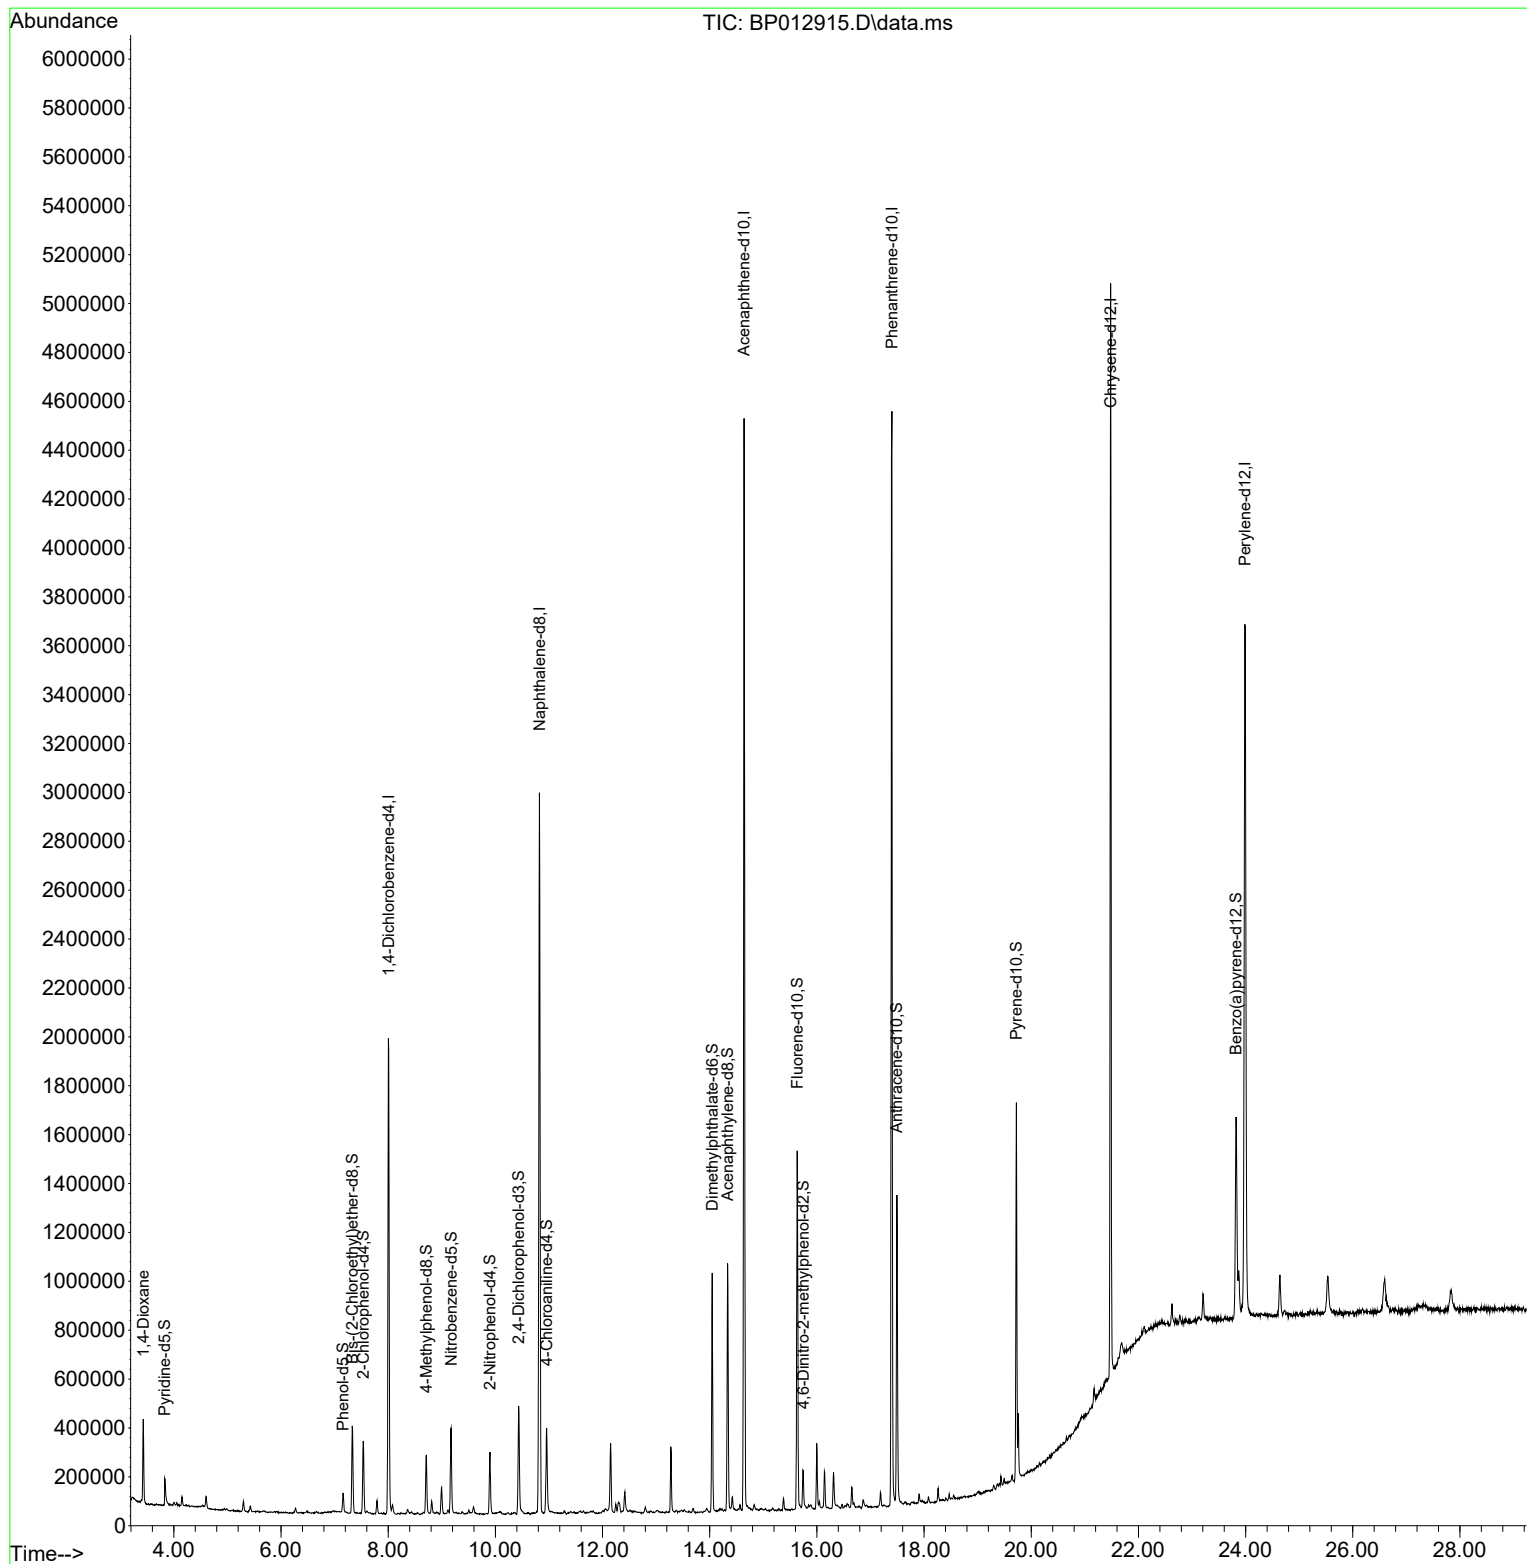

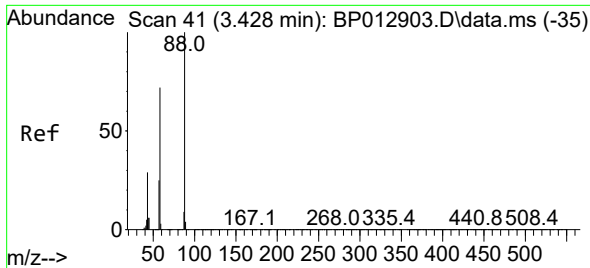

#2
 1,4-Dioxane
 Concen: 11.832 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012915.D
 Acq: 01 Dec 2022 13:09

Instrument :
 BNA_P
 ClientSampleId :
 A4345DL

Tgt Ion: 88 Resp: 163407
 Ion Ratio Lower Upper
 88 100
 43 27.9 22.6 34.0
 58 74.5 59.6 89.4

