

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012916.D
 Acq On : 01 Dec 2022 13:43
 Operator : CG/JU
 Sample : N5737-04DL 2X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4346DL

Quant Time: Dec 01 21:38:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	513815	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	2181270	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	1375349	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2896957	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	2870019	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	2936137	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	15211	1.269	ng/uL	0.00
4) Pyridine-d5	3.823	84	174436	4.861	ng/u1	0.00
7) Phenol-d5	7.158	99	152985	3.623	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	374951	14.412	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	388594	12.079	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	265766	7.812	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	213925	16.024	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	219425	15.479	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	456359	13.797	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	476426	10.519	ng/u1	0.00
46) Dimethylphthalate-d6	14.046	166	1516093	16.015	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	1661598	15.043	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	35903	2.127	ng/u1	0.00
60) Fluorene-d10	15.634	176	1354298	16.335	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	145288	10.493	ng/u1	0.00
73) Anthracene-d10	17.492	188	2105964	16.515	ng/u1	-0.01
81) Pyrene-d10	19.722	212	2515063	15.082	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.822	264	2339090	16.219	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.428	88	338685	26.301	ng/uL	100
67) N-Nitrosodiphenylamine	15.893	169	339518	4.124	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012916.D
Acq On : 01 Dec 2022 13:43
Operator : CG/JU
Sample : N5737-04DL 2X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4346DL

Quant Time: Dec 01 21:38:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration




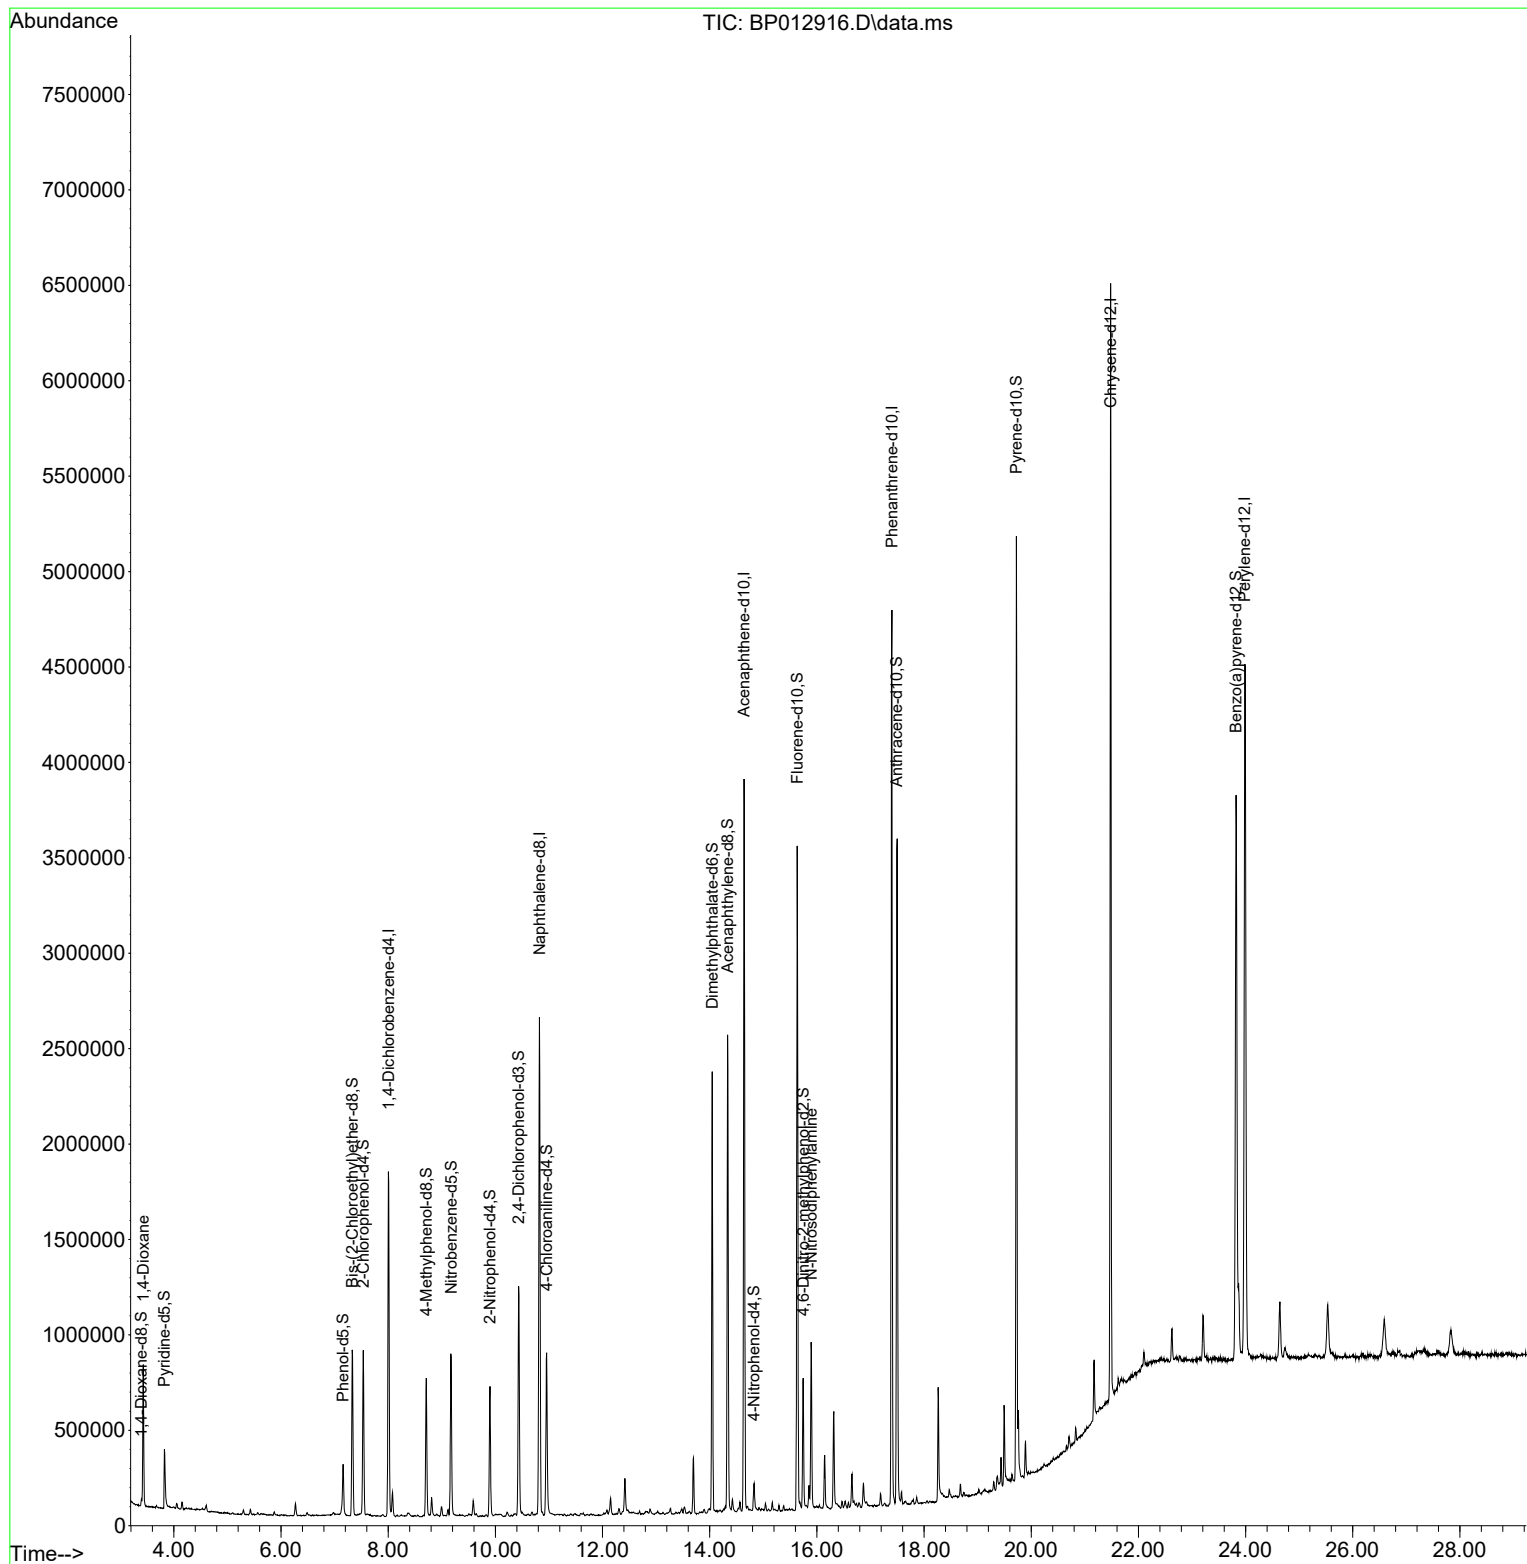


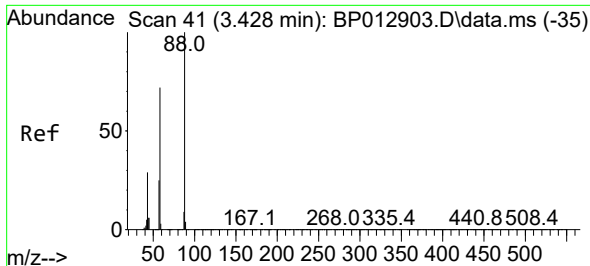

#2
 1,4-Dioxane
 Concen: 26.301 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012916.D
 Acq: 01 Dec 2022 13:43

Instrument :
 BNA_P
 ClientSampleId :
 A4346DL

Tgt Ion: 88 Resp: 338685
 Ion Ratio Lower Upper
 88 100
 43 28.0 22.6 34.0
 58 74.8 59.6 89.4

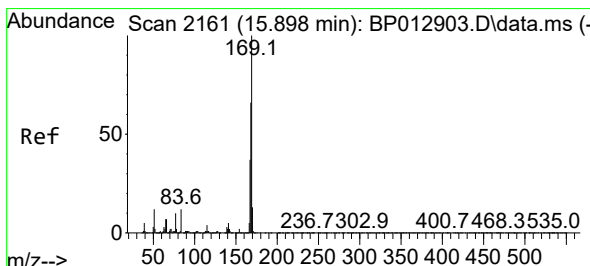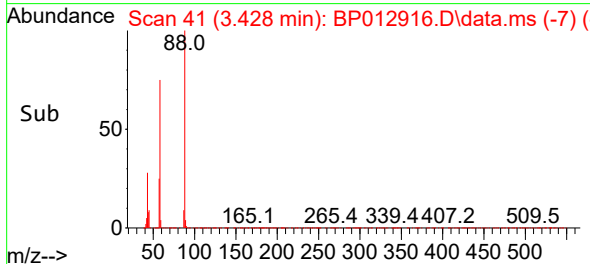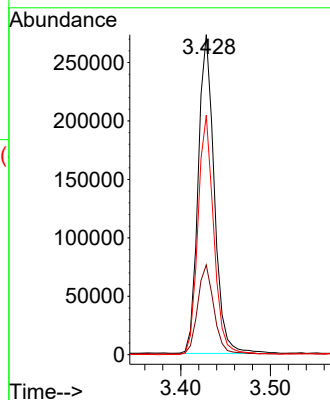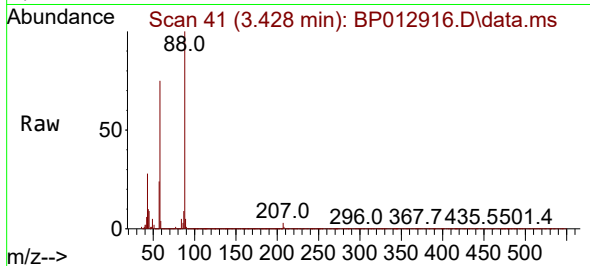

#67
 N-Nitrosodiphenylamine
 Concen: 4.124 ng/uL
 RT: 15.893 min Scan# 2160
 Delta R.T. -0.012 min
 Lab File: BP012916.D
 Acq: 01 Dec 2022 13:43

Tgt Ion: 169 Resp: 339518
 Ion Ratio Lower Upper
 169 100
 168 67.2 53.2 79.8
 167 35.6 29.6 44.4

