

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012917.D
 Acq On : 01 Dec 2022 14:17
 Operator : CG/JU
 Sample : N5737-05DL 2X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4347DL

Quant Time: Dec 01 21:38:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	473716	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1947399	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	1230814	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2617060	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	2617443	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	2638972	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	15100	1.366	ng/uL	0.00
4) Pyridine-d5	3.823	84	182888	5.528	ng/u1	0.00
7) Phenol-d5	7.158	99	122854	3.156	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	344063	14.344	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	334301	11.271	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	216015	6.887	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	190049	15.945	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	187363	14.804	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	379944	12.866	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	465443	11.510	ng/u1	0.00
46) Dimethylphthalate-d6	14.046	166	1326333	15.656	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	1443360	14.602	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	25965	1.719	ng/u1	0.00
60) Fluorene-d10	15.634	176	1188284	16.016	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	115892	9.265	ng/u1	0.00
73) Anthracene-d10	17.498	188	1890927	16.414	ng/u1	0.00
81) Pyrene-d10	19.722	212	2220930	14.603	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.821	264	2048629	15.804	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.428	88	289198	24.359	ng/uL	98
67) N-Nitrosodiphenylamine	15.893	169	529279	7.116	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012917.D
Acq On : 01 Dec 2022 14:17
Operator : CG/JU
Sample : N5737-05DL 2X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4347DL

Quant Time: Dec 01 21:38:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration




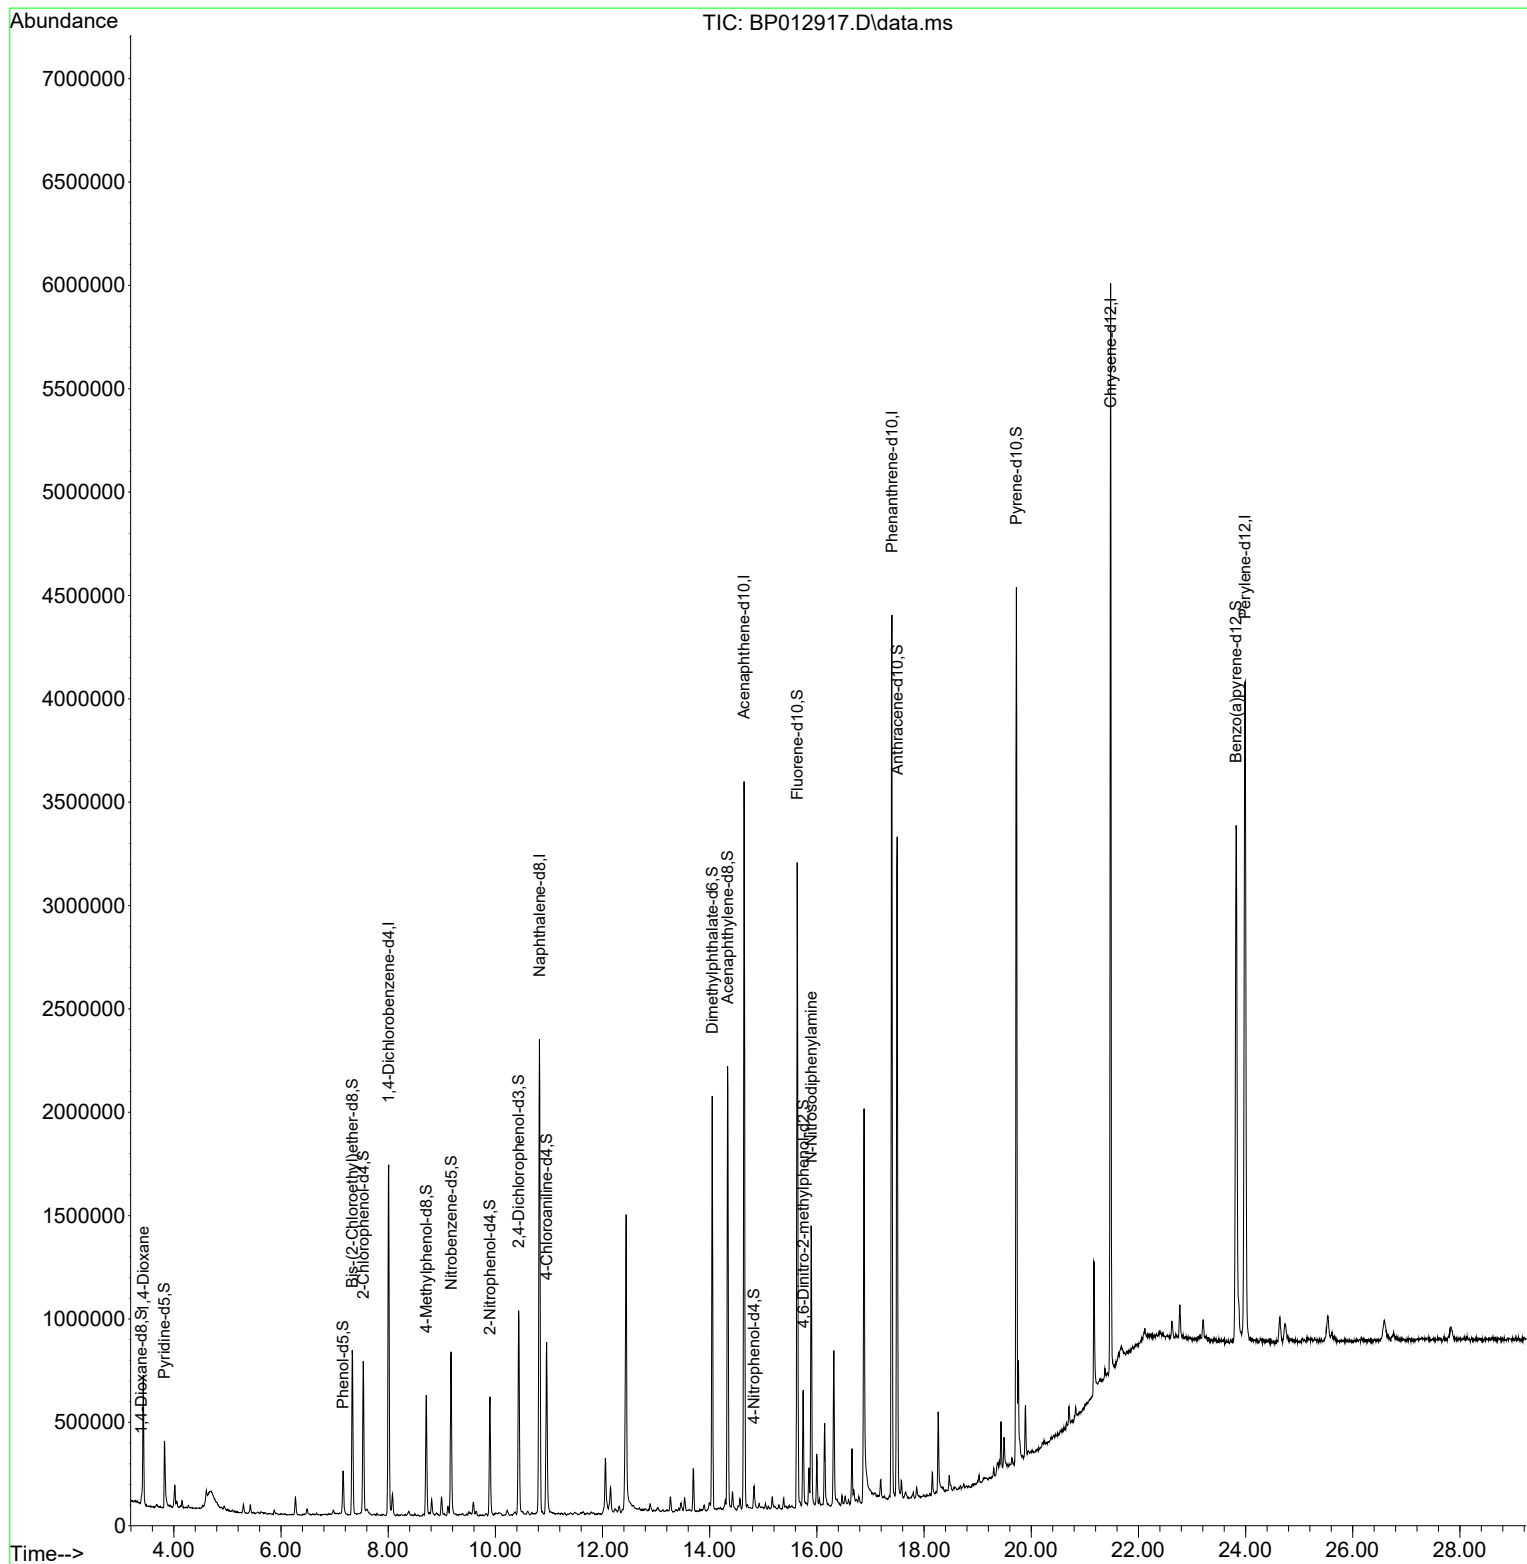


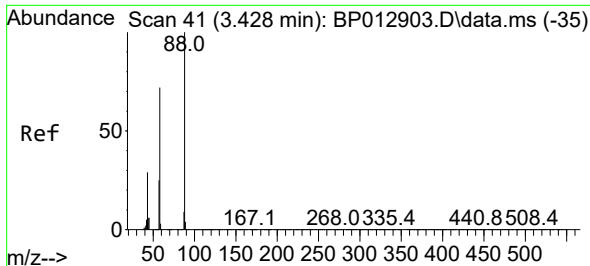

#2
1,4-Dioxane
Concen: 24.359 ng/uL
RT: 3.428 min Scan# 41
Delta R.T. 0.000 min
Lab File: BP012917.D
Acq: 01 Dec 2022 14:17

Instrument :
BNA_P
ClientSampleId :
A4347DL

Tgt Ion: 88 Resp: 289198
Ion Ratio Lower Upper
88 100
43 28.5 22.6 34.0
58 72.5 59.6 89.4

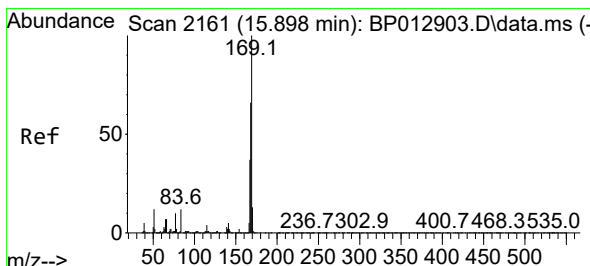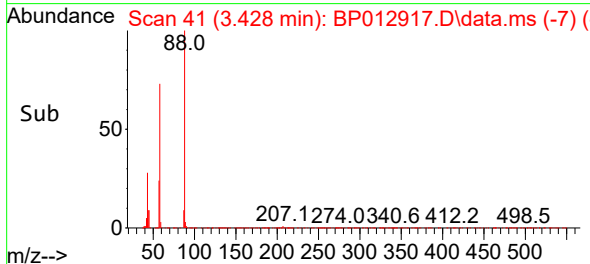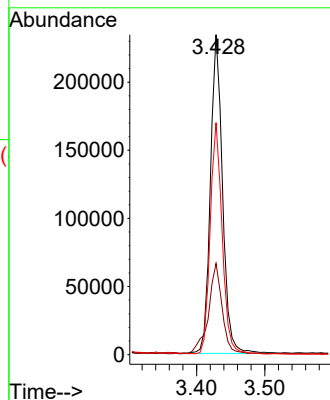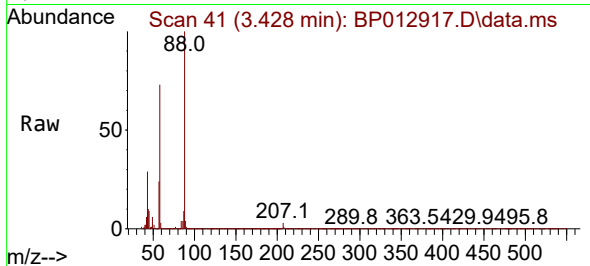

#67
N-Nitrosodiphenylamine
Concen: 7.116 ng/uL
RT: 15.893 min Scan# 2160
Delta R.T. -0.012 min
Lab File: BP012917.D
Acq: 01 Dec 2022 14:17

Tgt Ion: 169 Resp: 529279
Ion Ratio Lower Upper
169 100
168 66.2 53.2 79.8
167 36.2 29.6 44.4

