




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012899.D
 Acq On : 01 Dec 2022 02:55
 Operator : CG/JU
 Sample : N5770-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1F9

Manual IntegrationsAPPROVED

Quant Time: Dec 01 03:54:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/01/2022
 Supervised By :mohammad ahmed 12/02/2022

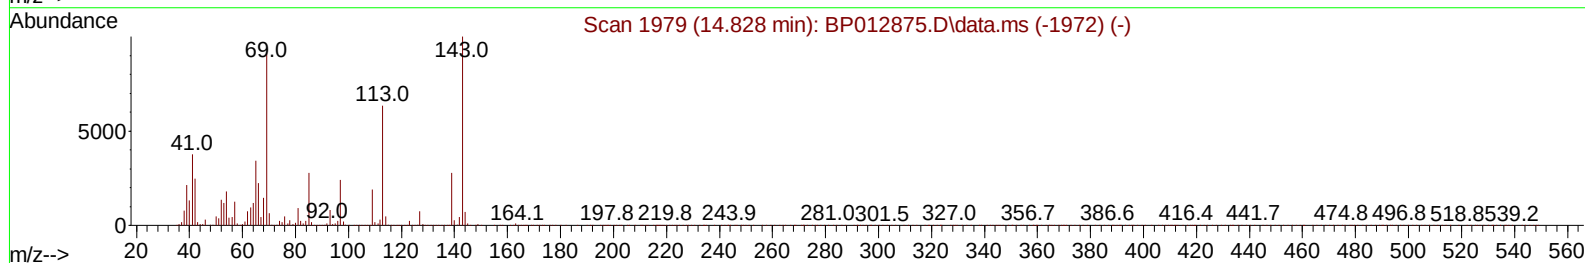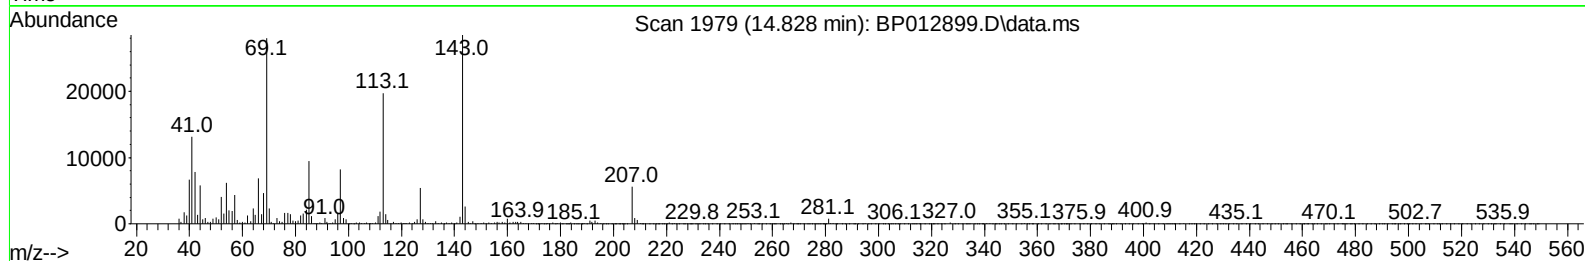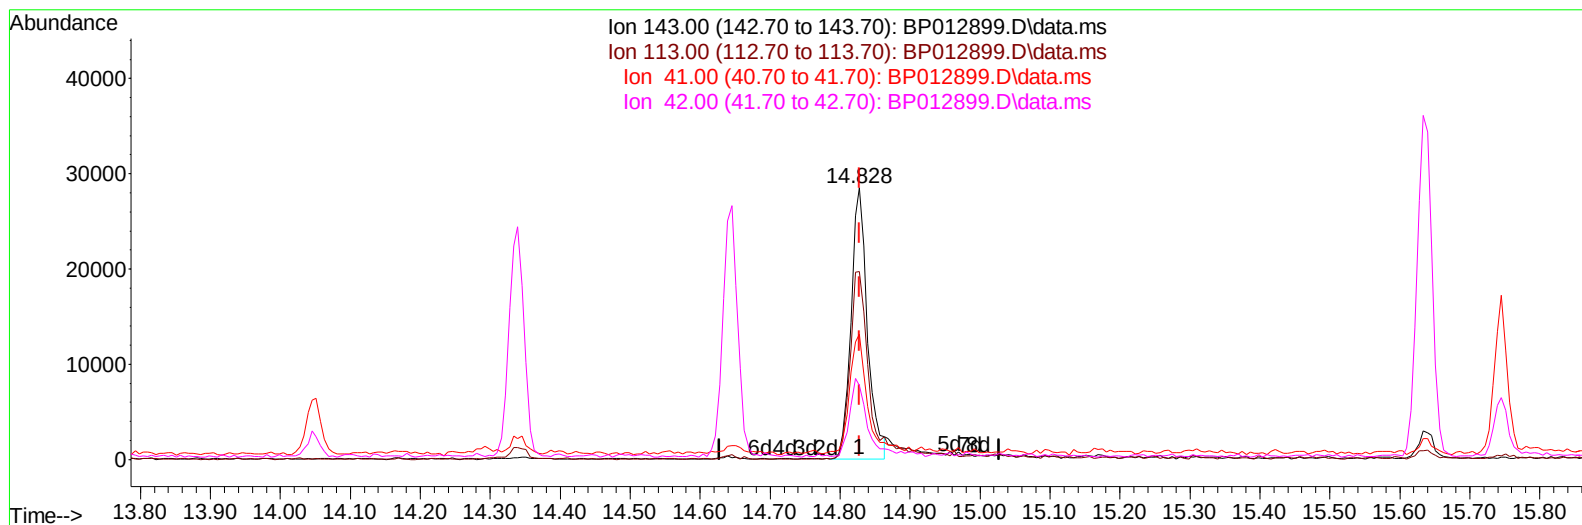

TIC: BP012899.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.828min (-0.000) 2.40 ng/ul

response 45711

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.70	69.16
41.00	37.00	46.09#
42.00	24.70	27.31




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012899.D
 Acq On : 01 Dec 2022 02:55
 Operator : CG/JU
 Sample : N5770-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1F9

Manual IntegrationsAPPROVED

Quant Time: Dec 01 03:54:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/01/2022
 Supervised By :mohammad ahmed 12/02/2022

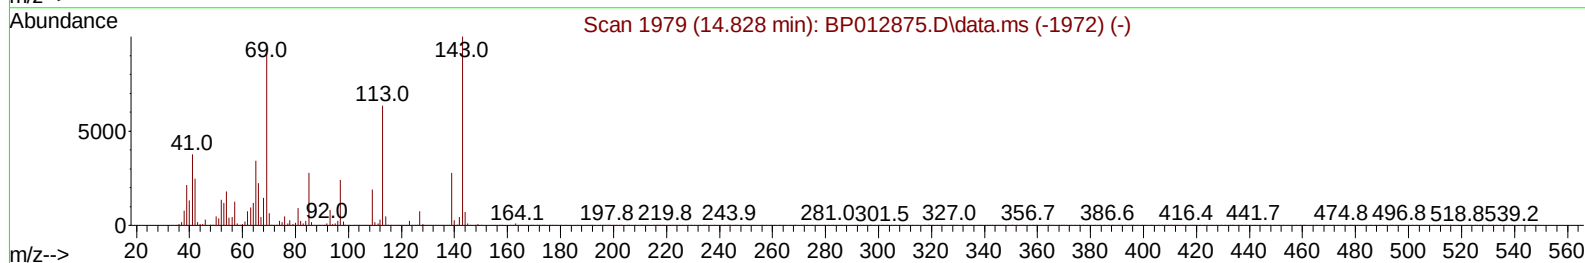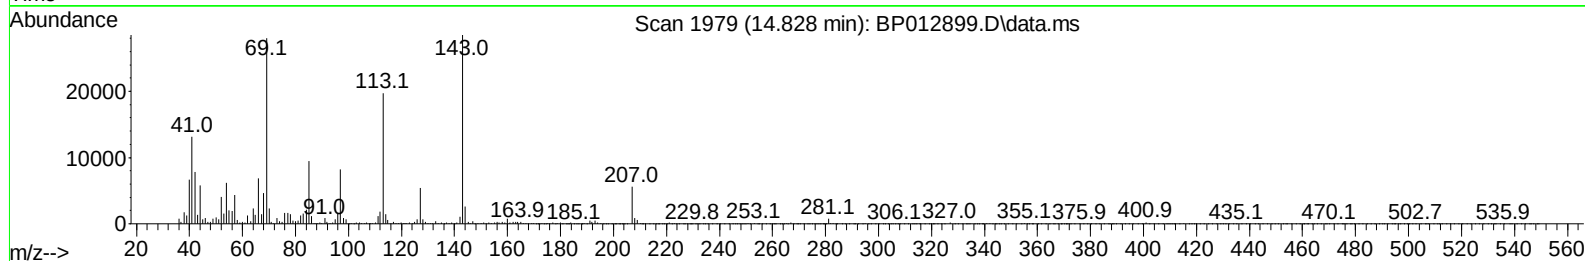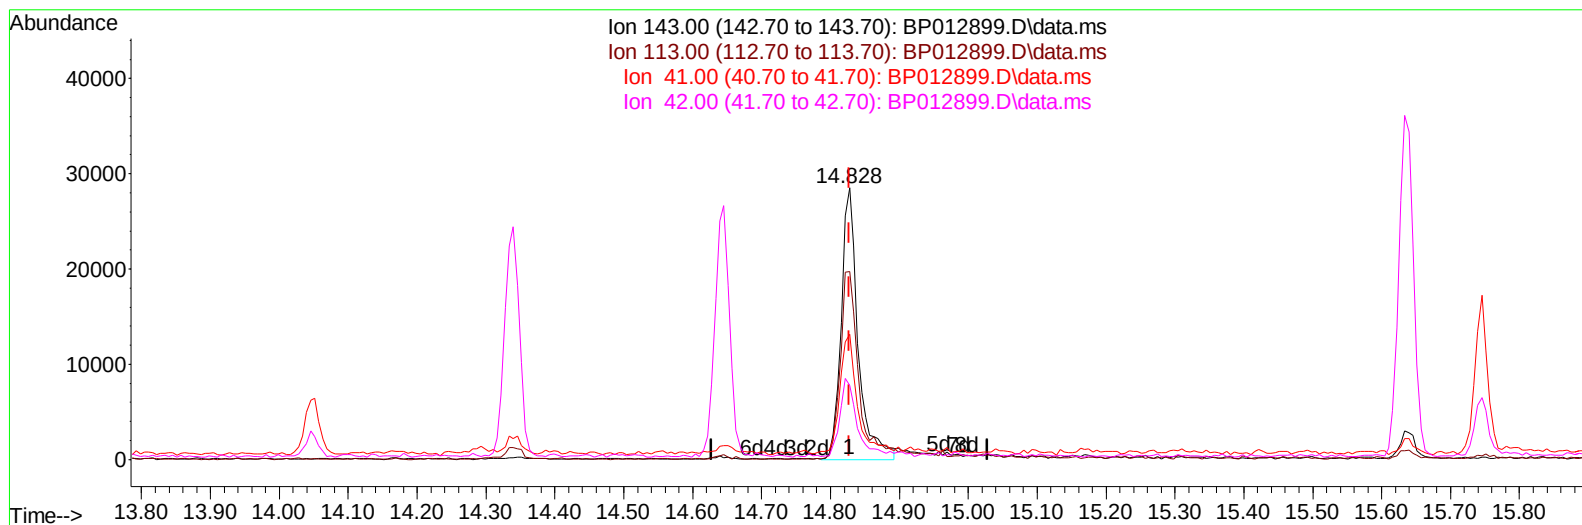

TIC: BP012899.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.828min (-0.000) 2.55 ng/ul m

response 48628

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.70	69.16
41.00	37.00	46.09#
42.00	24.70	27.31

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012899.D
 Acq On : 01 Dec 2022 02:55
 Operator : CG/JU
 Sample : N5770-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/01/2022
 Supervised By :mohammad ahmed 12/02/2022

Quant Time: Dec 01 03:54:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	586288	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	2548429	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	1552044	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	2734316	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1931301	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	2080499	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	63535	4.644	ng/uL	0.00
4) Pyridine-d5	3.822	84	183556	4.483	ng/ul	0.00
7) Phenol-d5	7.157	99	338638	7.029	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	828386	27.905	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	851654	23.200	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	586455	15.108	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	512173	32.836	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	537433	32.450	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	967351	25.033	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	382115	7.221	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3057047	28.616	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	3539914	28.399	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	48628m	2.553	ng/ul	0.00
60) Fluorene-d10	15.639	176	2646542	28.288	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	255964	19.586	ng/ul	0.00
73) Anthracene-d10	17.498	188	3556094	29.545	ng/ul	0.00
81) Pyrene-d10	19.727	212	3444867	30.698	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	3037367	29.722	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012899.D
Acq On : 01 Dec 2022 02:55
Operator : CG/JU
Sample : N5770-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/01/2022
Supervised By :mohammad ahmed 12/02/2022

Quant Time: Dec 01 03:54:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

