

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012883.D
 Acq On : 30 Nov 2022 17:13
 Operator : CG/JU
 Sample : N5725-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB69

Quant Time: Nov 30 21:56:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	557991	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2516036	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1663126	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3217177	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1946604	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	1860229	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	52334	4.019	ng/uL	0.00
4) Pyridine-d5	3.822	84	249792	6.410	ng/u1	0.00
7) Phenol-d5	7.158	99	241999	5.278	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	758333	26.840	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	725114	20.754	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	476308	12.893	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	456996	29.676	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	466977	28.559	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	874335	22.917	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1153444	22.077	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	3280199	28.654	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	3620515	27.106	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	49385	2.420	ng/u1	0.00
60) Fluorene-d10	15.639	176	2904803	28.974	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	308997	20.095	ng/u1	0.00
73) Anthracene-d10	17.498	188	4420384	31.214	ng/u1	0.00
81) Pyrene-d10	19.727	212	4193289	37.073	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	2865202	31.357	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.093	107	68618	1.714	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012883.D
Acq On : 30 Nov 2022 17:13
Operator : CG/JU
Sample : N5725-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB69

Quant Time: Nov 30 21:56:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

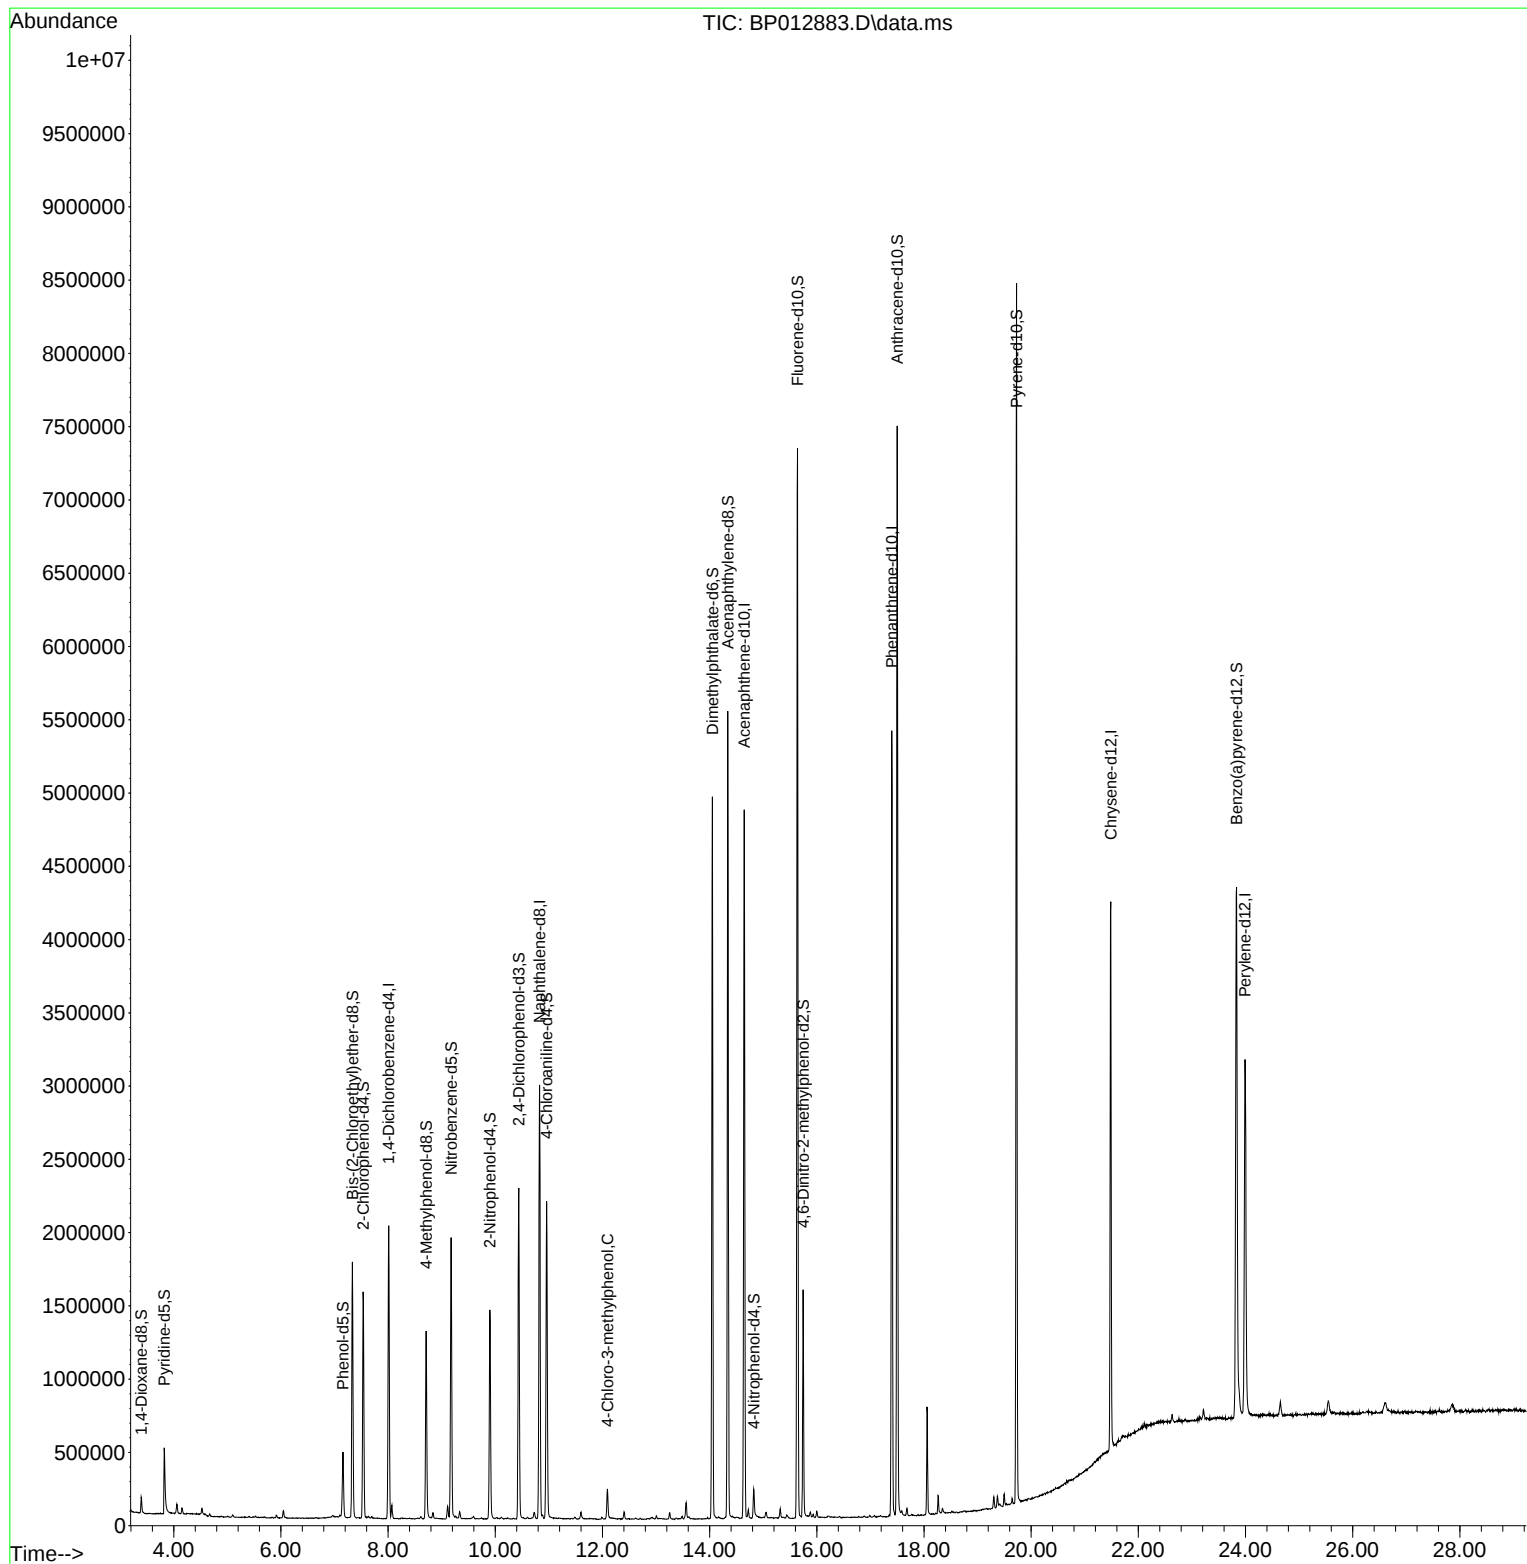

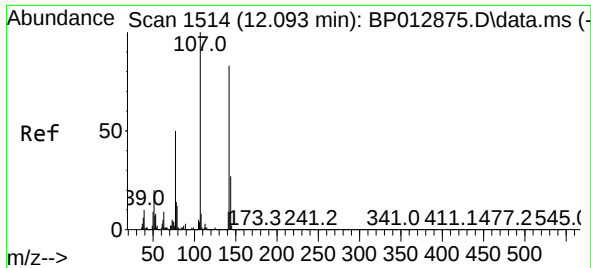

#35
 4-Chloro-3-methylphenol
 Concen: 1.714 ng/ul
 RT: 12.093 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP012883.D
 Acq: 30 Nov 2022 17:13

Instrument :
 BNA_P
 ClientSampleId :
 BHB69

Tgt Ion:107 Resp: 68618
 Ion Ratio Lower Upper
 107 100
 144 25.4 21.4 32.2
 142 78.3 66.6 100.0

