

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012894.D
 Acq On : 01 Dec 2022 00:05
 Operator : CG/JU
 Sample : N5737-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4345

Quant Time: Dec 01 00:42:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	588728	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2437611	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1501631	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3179876	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	3279751	20.000	ng/u1	0.00
88) Perylene-d12	23.998	264	3472329	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	52498	3.821	ng/uL	0.00
4) Pyridine-d5	3.822	84	370007	8.999	ng/u1	0.00
7) Phenol-d5	7.158	99	243822	5.040	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	761020	25.529	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	714573	19.385	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	460910	11.825	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	432455	28.986	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	420933	26.571	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	855068	23.133	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	967787	19.120	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	2904767	28.103	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	3298898	27.354	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	65806	3.571	ng/u1	0.00
60) Fluorene-d10	15.634	176	2612033	28.856	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	325621	21.425	ng/u1	0.00
73) Anthracene-d10	17.498	188	4037631	28.845	ng/u1	0.00
81) Pyrene-d10	19.727	212	4909109	25.760	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	4913262	28.807	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	822774	55.763	ng/uL	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012894.D
Acq On : 01 Dec 2022 00:05
Operator : CG/JU
Sample : N5737-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4345

Quant Time: Dec 01 00:42:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

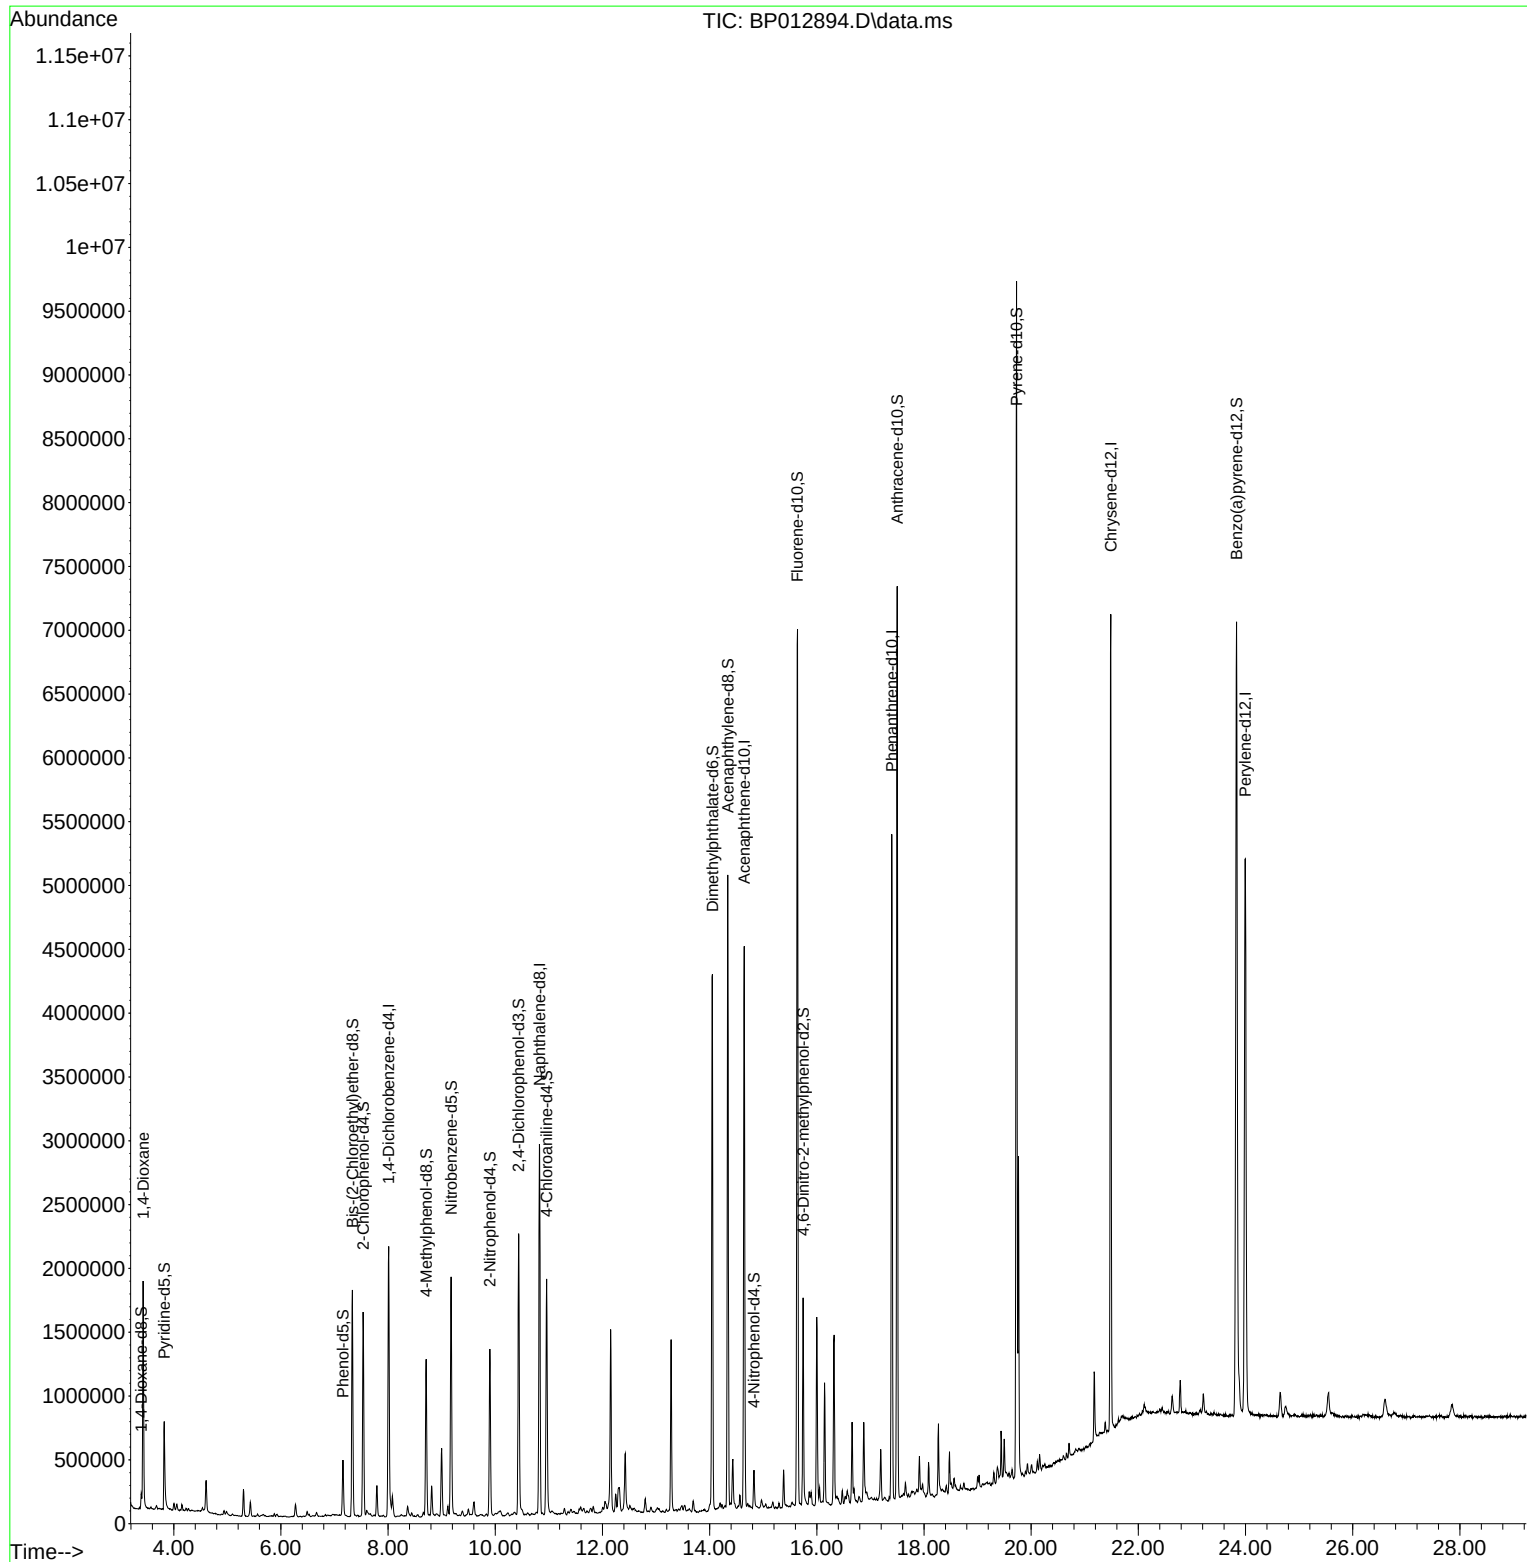

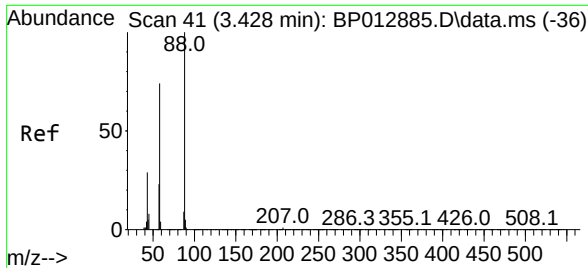

#2
 1,4-Dioxane
 Concen: 55.763 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012894.D
 Acq: 01 Dec 2022 00:05

Instrument :
 BNA_P
 ClientSampleId :
 A4345

Tgt Ion: 88 Resp: 822774

Ion	Ratio	Lower	Upper
88	100		
43	27.6	22.6	34.0
58	74.5	59.6	89.4

