

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012897.D
 Acq On : 01 Dec 2022 01:47
 Operator : CG/JU
 Sample : N5737-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4346

Quant Time: Dec 01 02:58:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	519922	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	2196258	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1400776	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3023929	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	3091945	20.000	ng/u1	0.00
88) Perylene-d12	23.998	264	3215893	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	52694	4.343	ng/uL	0.00
4) Pyridine-d5	3.822	84	352421	9.706	ng/u1	0.00
7) Phenol-d5	7.157	99	326092	7.633	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	736459	27.975	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	798526	24.529	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	562395	16.338	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	451999	33.625	ng/u1	0.00
24) 2-Nitrophenol-d4	9.898	143	487257	34.138	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	952690	28.606	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	984978	21.598	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	3090256	32.051	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	3471525	30.858	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	105126	6.116	ng/u1	0.00
60) Fluorene-d10	15.633	176	2772092	32.829	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	406186	28.104	ng/u1	0.00
73) Anthracene-d10	17.498	188	4369194	32.824	ng/u1	0.00
81) Pyrene-d10	19.727	212	5261300	29.285	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	5207036	32.964	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	655645	50.316	ng/uL	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012897.D
Acq On : 01 Dec 2022 01:47
Operator : CG/JU
Sample : N5737-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4346


Quant Time: Dec 01 02:58:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

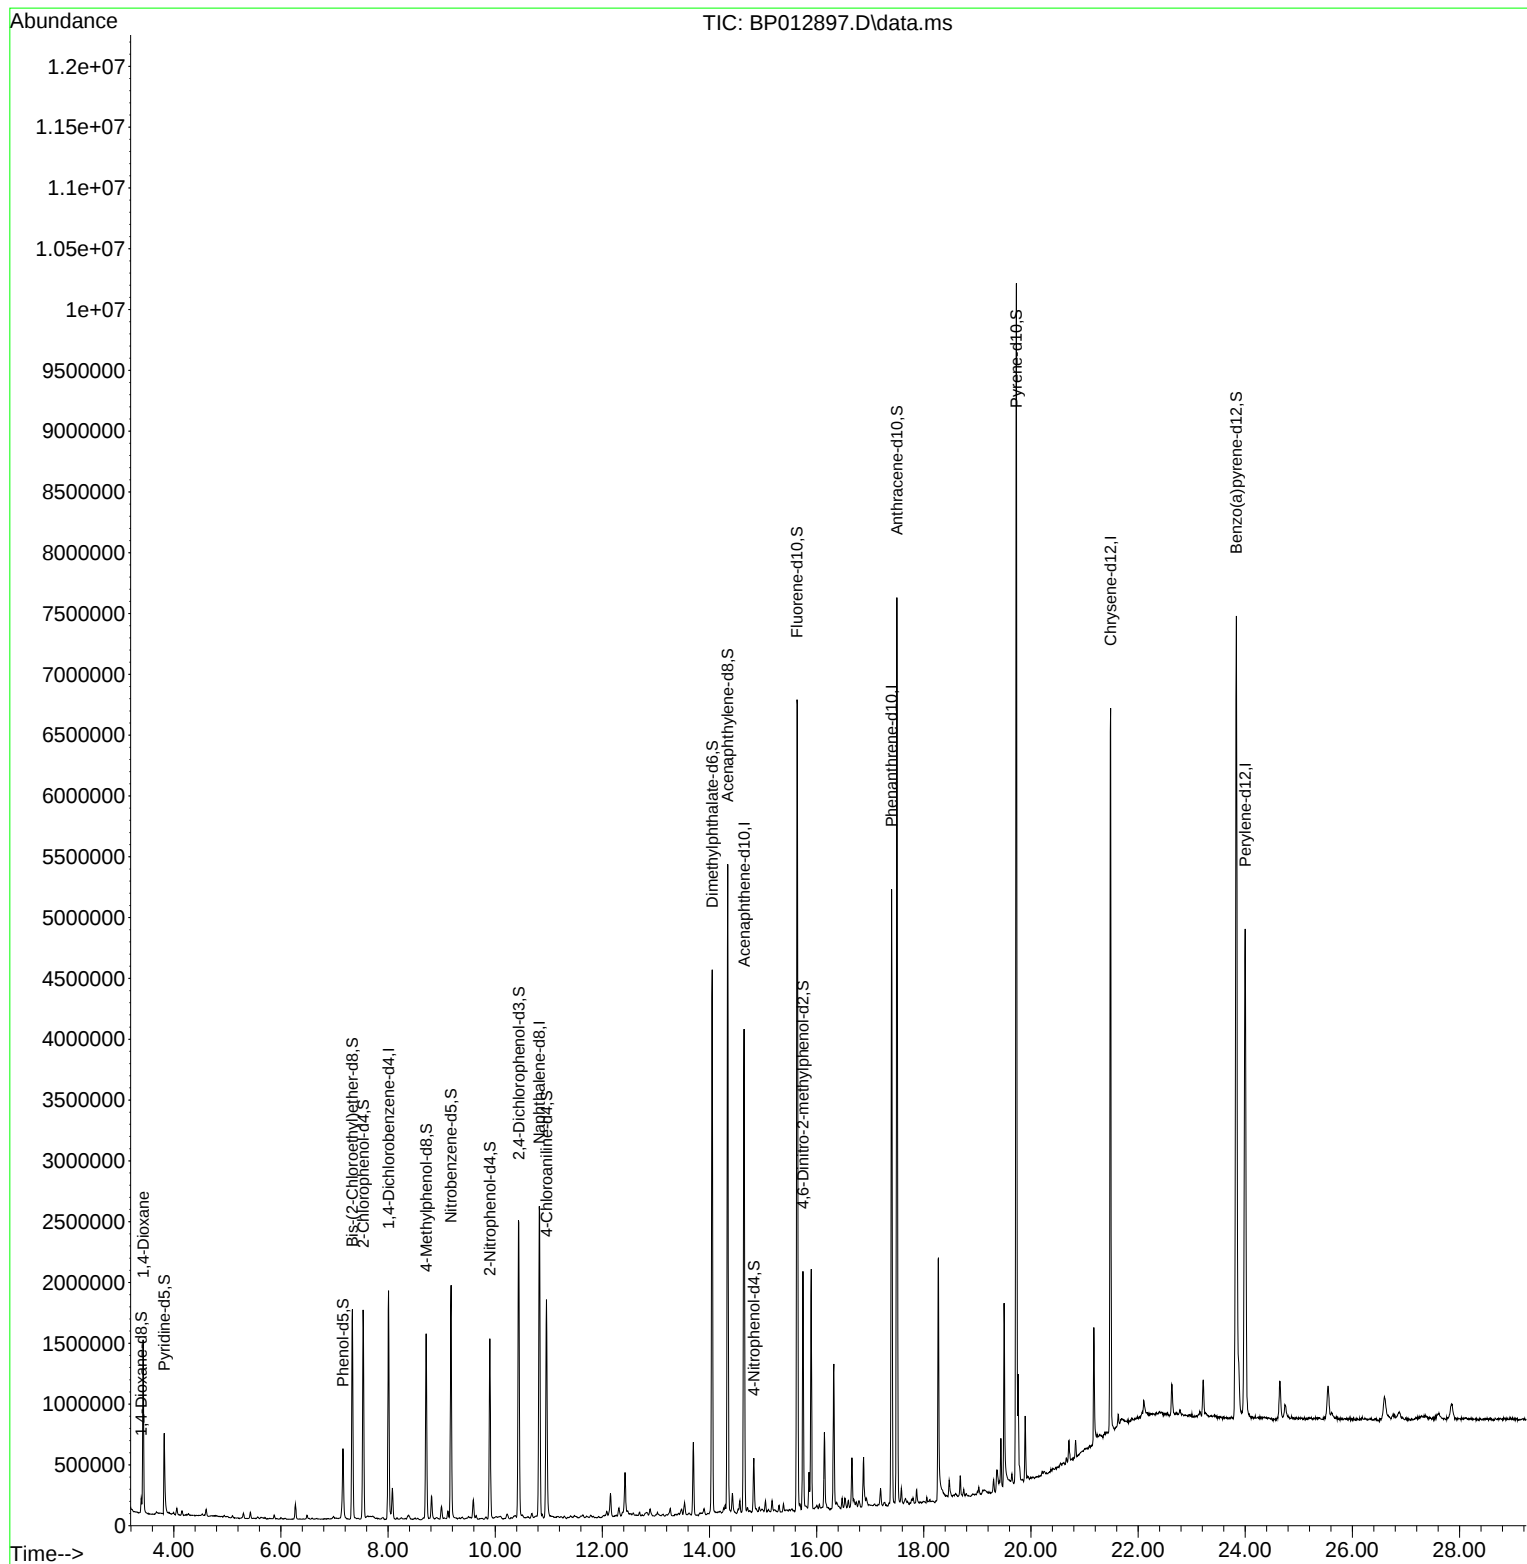

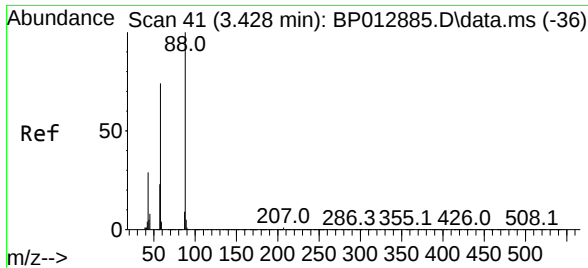

#2
 1,4-Dioxane
 Concen: 50.316 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012897.D
 Acq: 01 Dec 2022 01:47

Instrument :
 BNA_P
 ClientSampleId :
 A4346

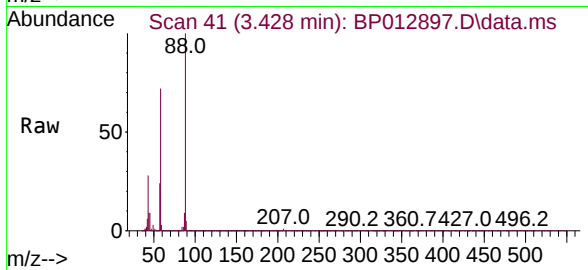

Tgt Ion: 88 Resp: 655645

Ion	Ratio	Lower	Upper
88	100		
43	27.5	22.6	34.0
58	72.0	59.6	89.4

