

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012876.D
 Acq On : 30 Nov 2022 13:14
 Operator : CG/JU
 Sample : PB149338BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK338

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	44	rVB	182461	245492	1.16%	0.130%
2	3.816	104	107	128	rBV	2231456	3443076	16.20%	1.822%
3	4.152	160	164	170	rBV2	33086	51441	0.24%	0.027%
4	7.157	668	675	685	rBV	2750839	4337508	20.41%	2.296%
5	7.334	698	705	714	rVB	2479118	3782768	17.80%	2.002%
6	7.534	732	739	749	rBV	2750554	4415474	20.77%	2.337%
7	8.010	812	820	828	rBV	1852938	2897258	13.63%	1.533%
8	8.710	931	939	957	rBV	3608018	5803086	27.30%	3.071%
9	9.175	1009	1018	1029	rBV	2754359	4403847	20.72%	2.331%
10	9.898	1131	1141	1154	rBV	2216418	3654861	17.20%	1.934%
11	10.440	1224	1233	1248	rBV	3594590	6125759	28.82%	3.242%
12	10.828	1290	1299	1311	rVB	2773315	4750341	22.35%	2.514%
13	10.957	1313	1321	1336	rBV	3607263	6179576	29.07%	3.271%
14	12.404	1562	1567	1574	rVB2	68726	112643	0.53%	0.060%
15	13.534	1754	1759	1764	rBV3	16320	26266	0.12%	0.014%
16	13.622	1767	1774	1778	rBV4	13847	25751	0.12%	0.014%
17	14.051	1840	1847	1858	rBV	7464048	10236455	48.16%	5.418%
18	14.339	1889	1896	1911	rBV	8455444	12177088	57.29%	6.445%
19	14.645	1941	1948	1957	rBV	4863835	7104584	33.43%	3.760%
20	14.828	1971	1979	1998	rBV	3288828	4772446	22.45%	2.526%
21	15.057	2015	2018	2024	rVB6	16611	23550	0.11%	0.012%
22	15.639	2108	2117	2128	rBV	11125625	15823611	74.45%	8.375%
23	15.745	2129	2135	2150	rVV	3188198	4490019	21.13%	2.377%
24	15.881	2154	2158	2163	rVB2	50213	82165	0.39%	0.043%
25	17.080	2357	2362	2366	rVB8	14572	22494	0.11%	0.012%
26	17.398	2409	2416	2426	rBV	6081193	8800579	41.41%	4.658%
27	17.504	2427	2434	2456	rVV	12027310	18171206	85.50%	9.618%
28	17.780	2477	2481	2490	rVB5	12430	26671	0.13%	0.014%
29	19.304	2736	2740	2746	rBV2	147031	196769	0.93%	0.104%
30	19.369	2747	2751	2756	rBV	142199	200972	0.95%	0.106%
31	19.645	2796	2798	2801	rVB4	27527	23759	0.11%	0.013%
32	19.727	2806	2812	2823	rBV	15873821	21253928	100.00%	11.249%
33	21.486	3105	3111	3121	rBV	6765694	9066003	42.66%	4.799%
34	23.833	3502	3510	3527	rBV	8581592	18198436	85.62%	9.632%
35	23.998	3531	3538	3552	rVB2	3783643	8007752	37.68%	4.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012876.D
Acq On : 30 Nov 2022 13:14
Operator : CG/JU
Sample : PB149338BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 188933634

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012876.D
Acq On : 30 Nov 2022 13:14
Operator : CG/JU
Sample : PB149338BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

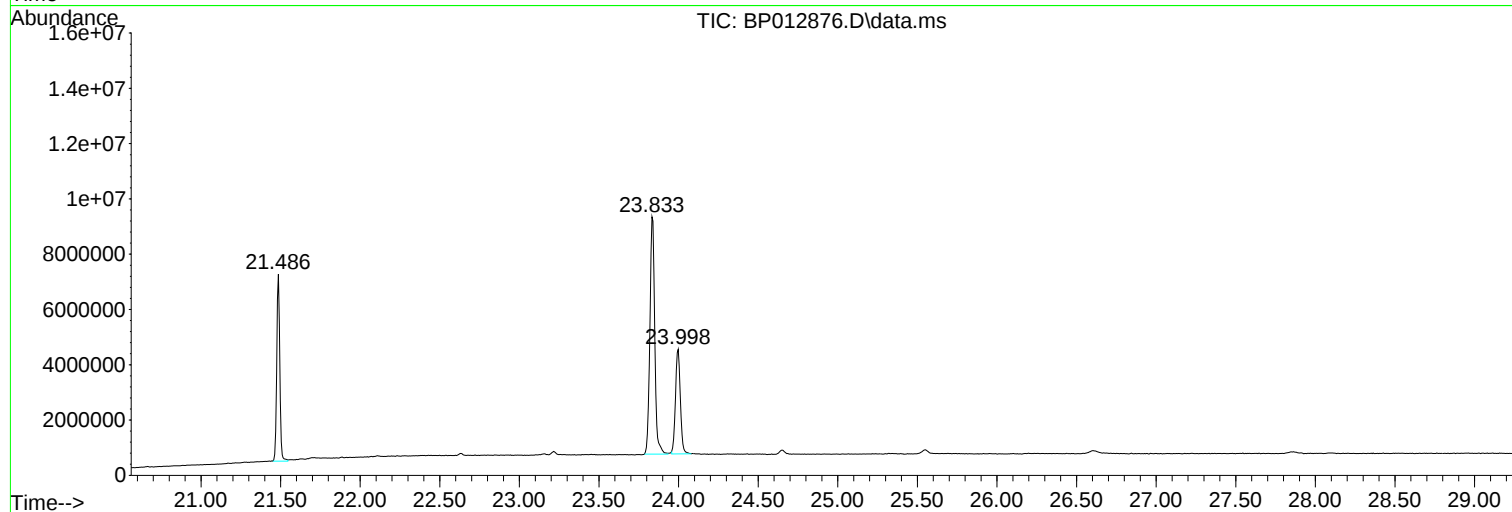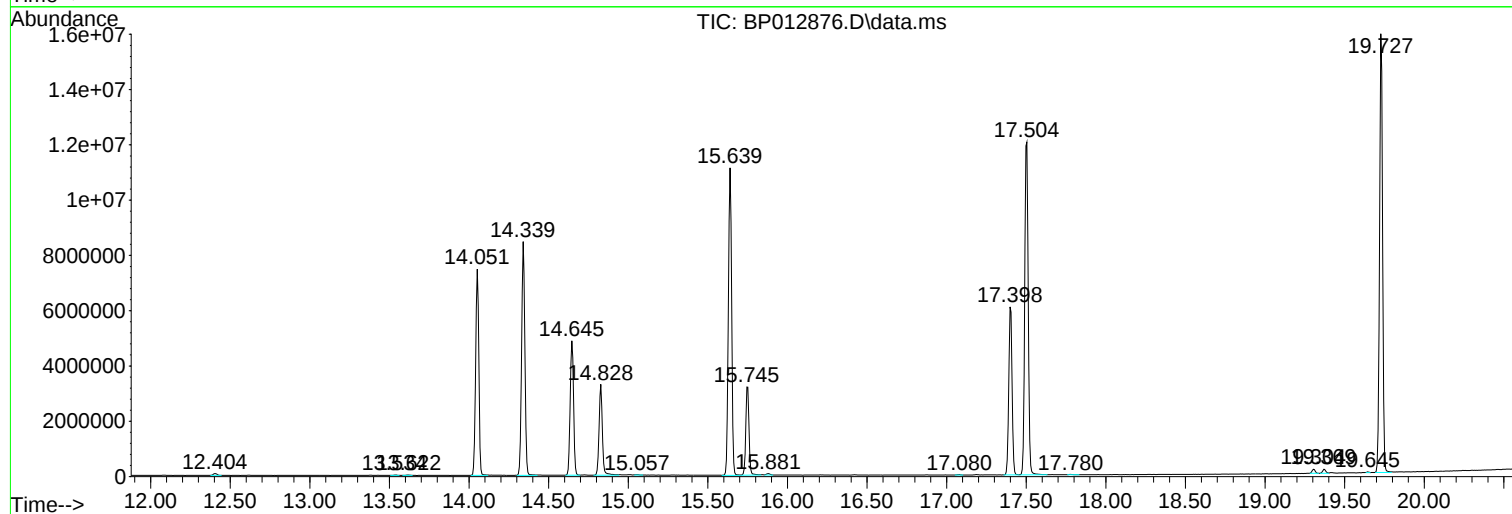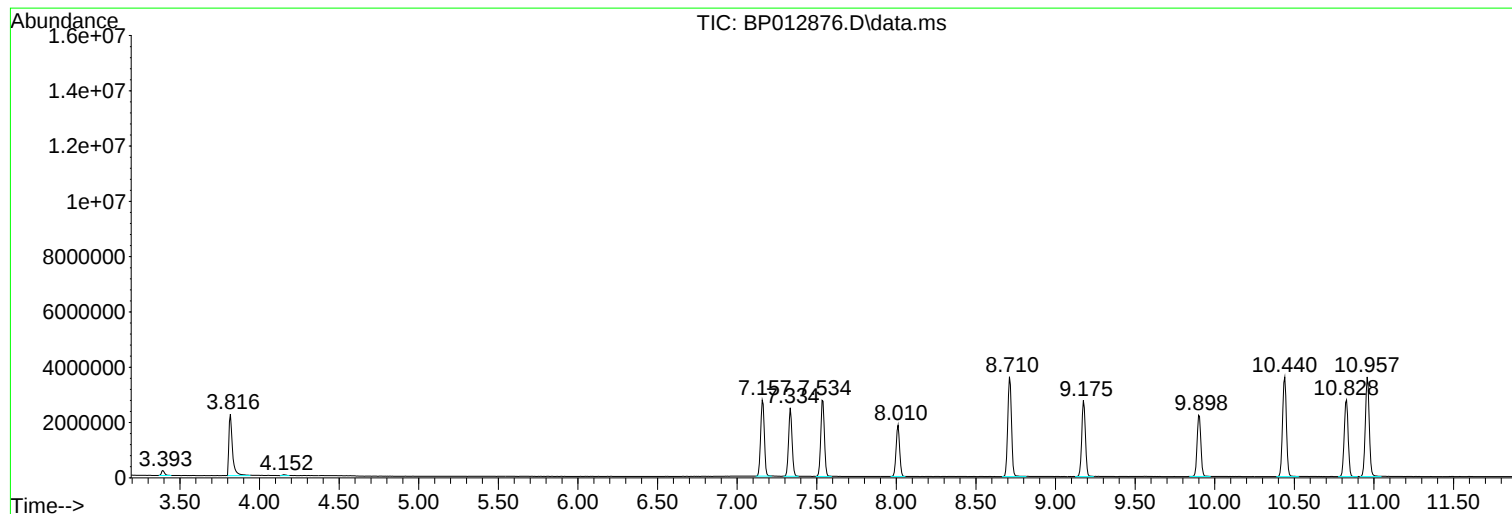

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012876.D
Acq On : 30 Nov 2022 13:14
Operator : CG/JU
Sample : PB149338BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012876.D
Acq On : 30 Nov 2022 13:14
Operator : CG/JU
Sample : PB149338BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc