

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012878.D
 Acq On : 30 Nov 2022 14:22
 Operator : CG/JU
 Sample : N5811-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	42	rBV	109824	137527	0.81%	0.094%
2	3.822	105	108	124	rBV	296372	514598	3.02%	0.351%
3	4.058	144	148	153	rVB	50258	77638	0.46%	0.053%
4	4.158	161	165	170	rBV	37629	53962	0.32%	0.037%
5	5.093	320	324	332	rBV	199332	297215	1.74%	0.203%
6	7.158	669	675	683	rVB	515162	795585	4.66%	0.542%
7	7.334	698	705	718	rBV	1942616	2988508	17.52%	2.037%
8	7.534	732	739	751	rBV	1719563	2741580	16.07%	1.869%
9	8.010	812	820	827	rBV	1902864	2985806	17.50%	2.035%
10	8.710	931	939	951	rBV	1468414	2357983	13.82%	1.607%
11	9.175	1011	1018	1028	rBV	2155298	3405142	19.96%	2.321%
12	9.593	1084	1089	1095	rVB5	12393	22102	0.13%	0.015%
13	9.899	1134	1141	1151	rBV	1634608	2637179	15.46%	1.798%
14	10.440	1224	1233	1248	rBV	2599439	4312066	25.28%	2.939%
15	10.828	1288	1299	1307	rBV	2849063	4851418	28.44%	3.307%
16	10.957	1313	1321	1337	rBV	2129335	3712778	21.76%	2.531%
17	11.598	1423	1430	1434	rBV9	10167	19696	0.12%	0.013%
18	12.345	1553	1557	1562	rVB6	12573	21189	0.12%	0.014%
19	12.404	1562	1567	1573	rBV2	53058	83000	0.49%	0.057%
20	13.540	1755	1760	1766	rBV	59930	94300	0.55%	0.064%
21	13.616	1766	1773	1779	rVB6	15213	31109	0.18%	0.021%
22	14.051	1840	1847	1857	rBV	5777822	7723393	45.27%	5.265%
23	14.339	1888	1896	1910	rBV	6648846	9482813	55.59%	6.464%
24	14.539	1927	1930	1937	rVB8	9045	17266	0.10%	0.012%
25	14.645	1937	1948	1958	rBV	4995238	7313572	42.87%	4.986%
26	14.822	1973	1978	1984	rBV	366100	594829	3.49%	0.405%
27	14.869	1984	1986	1992	rVB	46581	64144	0.38%	0.044%
28	15.051	2011	2017	2023	rBV5	57042	93212	0.55%	0.064%
29	15.639	2110	2117	2126	rBV	8521516	12444312	72.94%	8.483%
30	15.745	2129	2135	2153	rVV	2314439	3125293	18.32%	2.130%
31	15.881	2153	2158	2164	rVB	39860	66742	0.39%	0.045%
32	16.333	2229	2235	2244	rBV	31042	62131	0.36%	0.042%
33	17.186	2377	2380	2386	rVB3	15114	23915	0.14%	0.016%
34	17.398	2409	2416	2425	rBV	6311027	9084420	53.25%	6.193%
35	17.498	2426	2433	2446	rBV	10287851	14467588	84.80%	9.862%
36	18.263	2559	2563	2570	rBV	191351	268277	1.57%	0.183%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012878.D
 Acq On : 30 Nov 2022 14:22
 Operator : CG/JU
 Sample : N5811-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	18.345	2574	2577	2581	rVB2	20161	29272	0.17%	0.020%
38	18.680	2631	2634	2638	rVB3	25081	26700	0.16%	0.018%
39	19.304	2735	2740	2745	rBV2	127064	174519	1.02%	0.119%
40	19.369	2747	2751	2756	rBV	119592	175827	1.03%	0.120%
41	19.498	2769	2773	2779	rBV2	142687	198446	1.16%	0.135%
42	19.645	2795	2798	2802	rVB3	56028	59726	0.35%	0.041%
43	19.727	2806	2812	2823	rBV	13233985	17059941	100.00%	11.630%
44	21.486	3105	3111	3120	rBV	6862835	9364758	54.89%	6.384%
45	23.833	3502	3510	3527	rBV2	6642086	14344590	84.08%	9.779%
46	23.998	3530	3538	3552	rVB	3966368	8288044	48.58%	5.650%




Sum of corrected areas: 146694111

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012878.D
Acq On : 30 Nov 2022 14:22
Operator : CG/JU
Sample : N5811-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

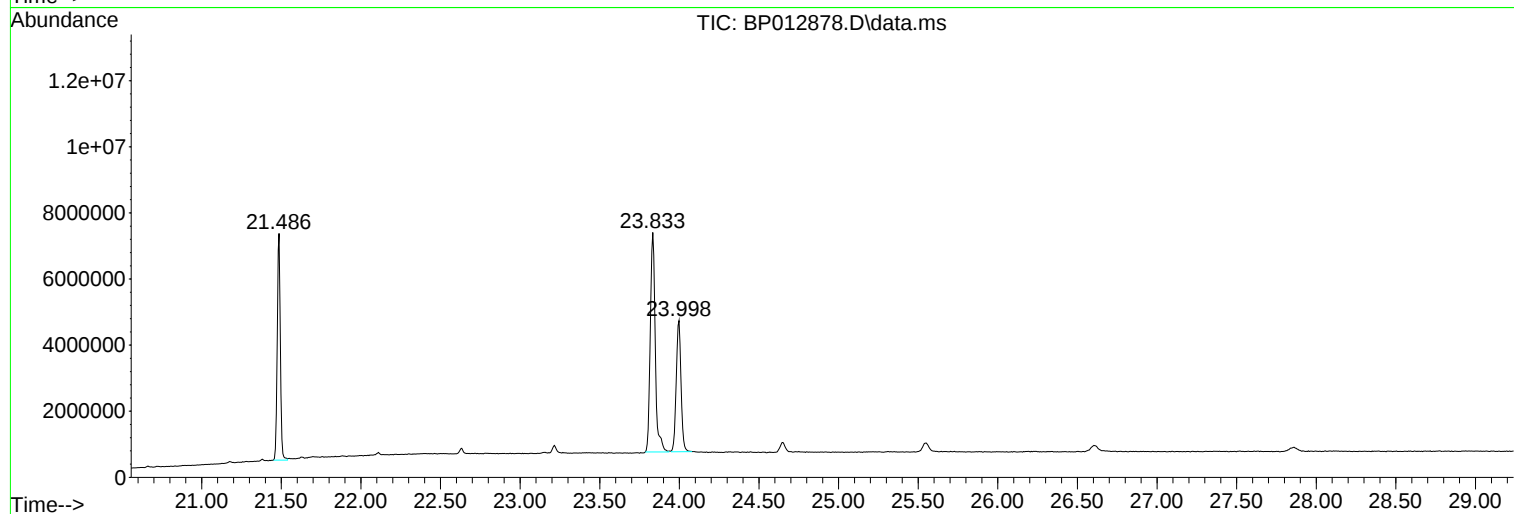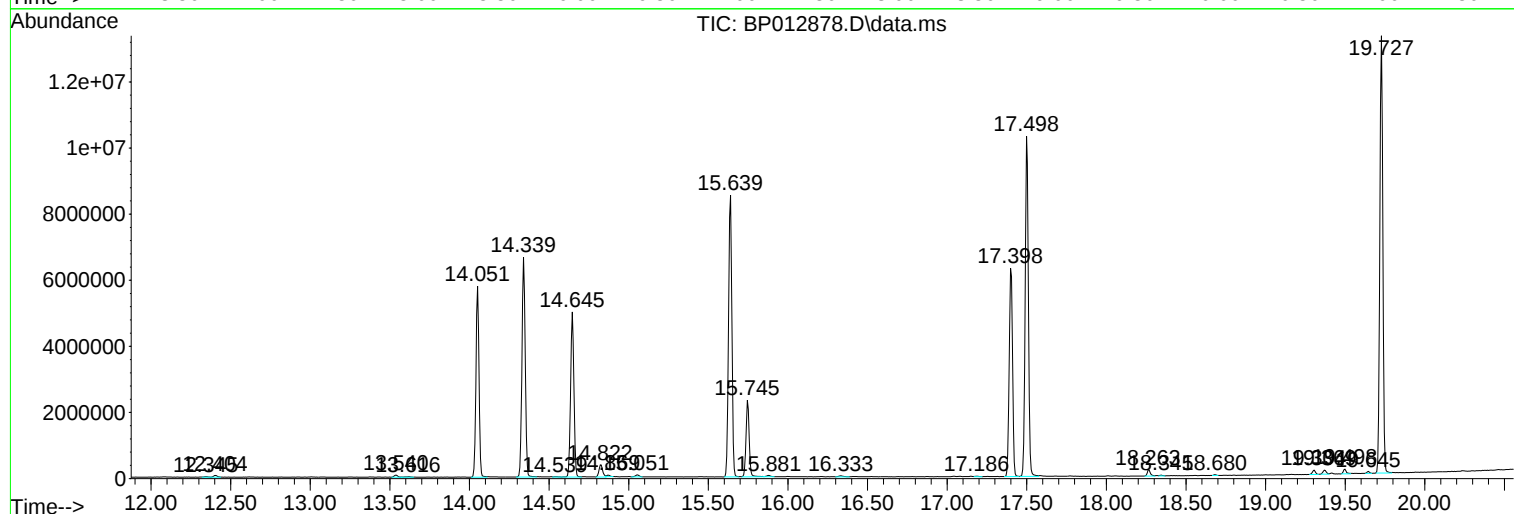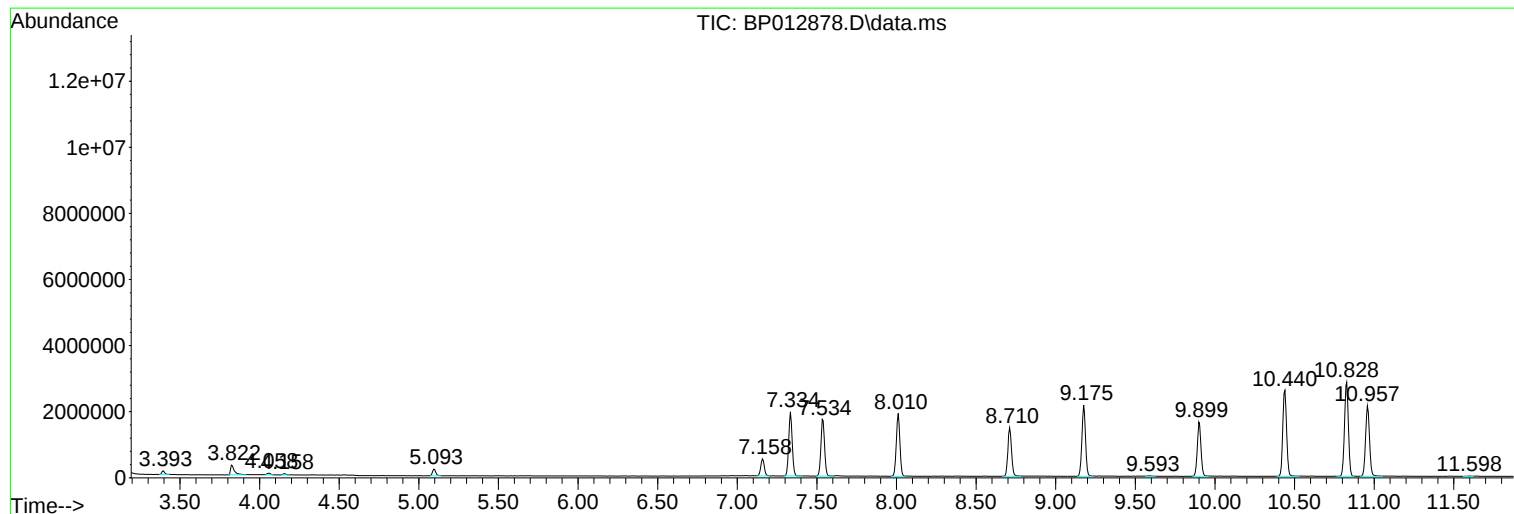

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012878.D
Acq On : 30 Nov 2022 14:22
Operator : CG/JU
Sample : N5811-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012878.D
Acq On : 30 Nov 2022 14:22
Operator : CG/JU
Sample : N5811-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc