

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012880.D
 Acq On : 30 Nov 2022 15:31
 Operator : CG/JU
 Sample : N5811-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	40	rBV	116819	142156	1.35%	0.122%
2	3.822	106	108	122	rBV	388923	603357	5.73%	0.519%
3	4.058	144	148	154	rVB	54432	80568	0.76%	0.069%
4	4.158	161	165	171	rVB	42302	59565	0.57%	0.051%
5	5.099	320	325	337	rVB	148797	223162	2.12%	0.192%
6	7.158	669	675	684	rVB	485762	739004	7.01%	0.636%
7	7.334	698	705	716	rBV	1937152	2960681	28.10%	2.549%
8	7.534	732	739	750	rBV	1701883	2704256	25.66%	2.328%
9	7.622	750	754	762	rVB6	17791	32445	0.31%	0.028%
10	8.010	812	820	828	rBV	2101562	3306604	31.38%	2.847%
11	8.710	931	939	949	rBV	1378904	2152650	20.43%	1.853%
12	9.175	1011	1018	1030	rBV	2055201	3281002	31.14%	2.825%
13	9.275	1030	1035	1040	rVV8	16295	34383	0.33%	0.030%
14	9.340	1042	1046	1051	rVB8	7472	12560	0.12%	0.011%
15	9.593	1082	1089	1095	rVB6	15741	32204	0.31%	0.028%
16	9.899	1134	1141	1155	rBV	1526272	2497229	23.70%	2.150%
17	10.440	1224	1233	1244	rBV	2440612	4008418	38.04%	3.451%
18	10.828	1290	1299	1310	rVB	3053213	5098412	48.39%	4.389%
19	10.957	1313	1321	1341	rBV	2031403	3499242	33.21%	3.013%
20	11.593	1426	1429	1432	rBV5	7943	11540	0.11%	0.010%
21	12.087	1507	1513	1516	rBV6	7551	12734	0.12%	0.011%
22	12.345	1551	1557	1561	rBV3	18622	33995	0.32%	0.029%
23	12.404	1562	1567	1576	rVB	49487	81962	0.78%	0.071%
24	12.616	1599	1603	1611	rVB10	7342	16561	0.16%	0.014%
25	13.381	1726	1733	1738	rBV9	7998	18266	0.17%	0.016%
26	13.469	1743	1748	1752	rVV8	8056	14107	0.13%	0.012%
27	13.540	1755	1760	1766	rVV2	41253	67270	0.64%	0.058%
28	13.616	1766	1773	1778	rVB4	13064	21769	0.21%	0.019%
29	14.051	1838	1847	1861	rBV	4525614	6251314	59.33%	5.382%
30	14.340	1889	1896	1904	rBV	5517342	7915203	75.12%	6.814%
31	14.645	1941	1948	1958	rBV	4614300	6777944	64.33%	5.835%
32	14.822	1972	1978	1991	rBV	184048	354661	3.37%	0.305%
33	15.051	2012	2017	2024	rVB8	23310	40022	0.38%	0.034%
34	15.639	2110	2117	2127	rBV	7168707	9861312	93.59%	8.490%
35	15.745	2129	2135	2148	rVV	1481719	2075082	19.69%	1.786%
36	15.881	2152	2158	2165	rVB2	33075	61087	0.58%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012880.D
 Acq On : 30 Nov 2022 15:31
 Operator : CG/JU
 Sample : N5811-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.398	2409	2416	2426	rBV	4976402	7049008	66.90%	6.069%
38	17.498	2426	2433	2451	rVV	7064384	10179215	96.60%	8.763%
39	17.769	2477	2479	2485	rVB5	9036	14077	0.13%	0.012%
40	18.016	2518	2521	2525	rBV6	8777	13817	0.13%	0.012%
41	18.063	2525	2529	2533	rVV6	11501	17584	0.17%	0.015%
42	18.269	2560	2564	2568	rBV2	60746	83105	0.79%	0.072%
43	18.686	2631	2635	2639	rBV5	27478	35749	0.34%	0.031%
44	19.304	2736	2740	2745	rBV2	76372	106740	1.01%	0.092%
45	19.369	2747	2751	2756	rBV	73581	119769	1.14%	0.103%
46	19.498	2770	2773	2777	rBV5	33831	41108	0.39%	0.035%
47	19.645	2796	2798	2801	rVB4	27607	28905	0.27%	0.025%
48	19.727	2806	2812	2824	rBV	8142330	10536991	100.00%	9.071%
49	21.486	3106	3111	3121	rBV	4687410	6230782	59.13%	5.364%
50	23.833	3503	3510	3527	rVB2	4729872	9950108	94.43%	8.566%
51	23.998	3531	3538	3553	rVB2	3124384	6666226	63.26%	5.739%




Sum of corrected areas: 116155911

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012880.D
Acq On : 30 Nov 2022 15:31
Operator : CG/JU
Sample : N5811-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

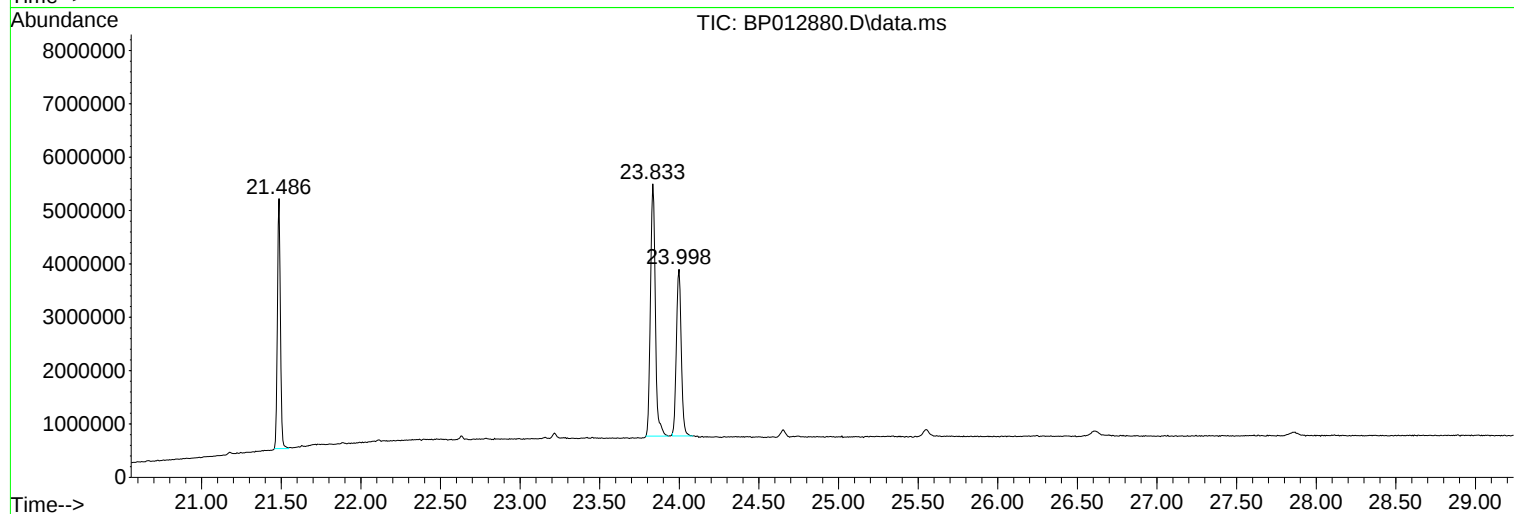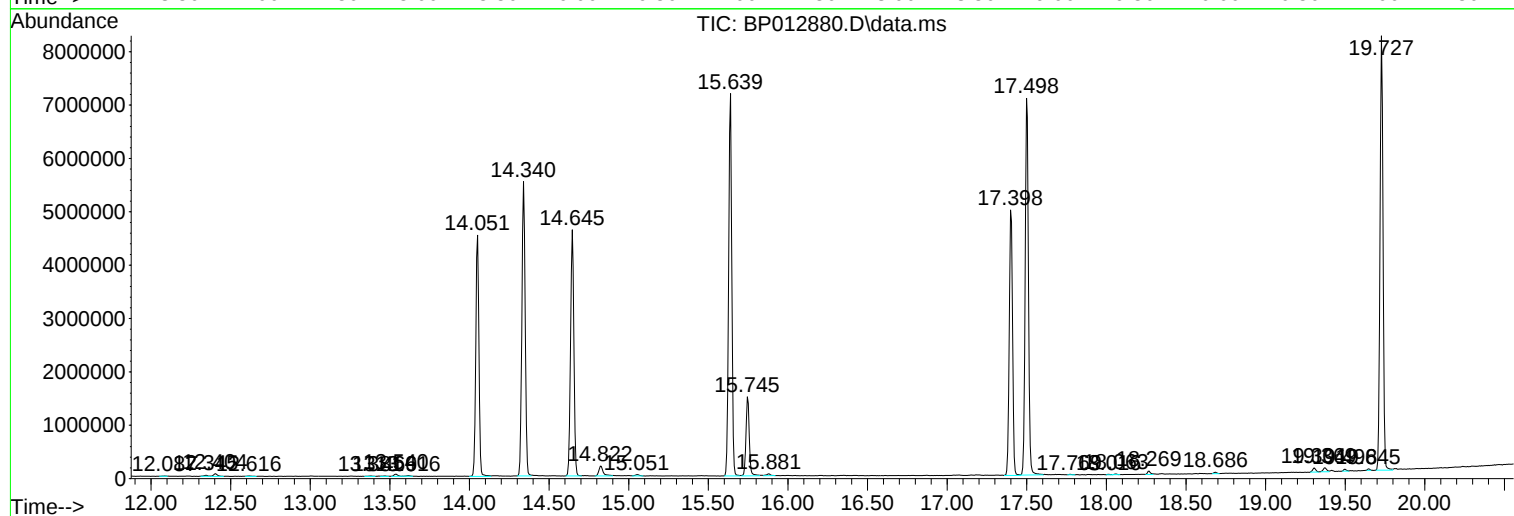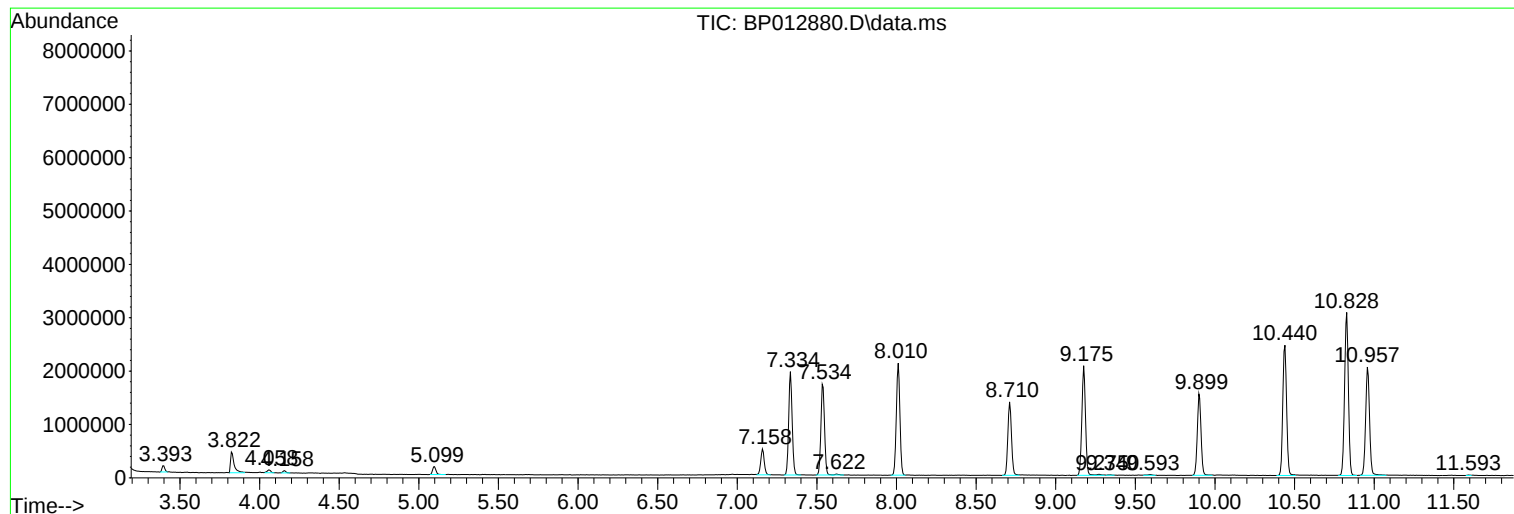

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012880.D
Acq On : 30 Nov 2022 15:31
Operator : CG/JU
Sample : N5811-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012880.D
Acq On : 30 Nov 2022 15:31
Operator : CG/JU
Sample : N5811-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
