

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012887.D
 Acq On : 30 Nov 2022 20:05
 Operator : CG/JU
 Sample : PB149276BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	47	rVB	193826	267427	1.86%	0.165%
2	3.816	103	107	128	rBV	2252098	3396334	23.58%	2.097%
3	4.158	161	165	169	rBV	39107	47841	0.33%	0.030%
4	7.157	668	675	692	rVB	2814009	4399007	30.54%	2.716%
5	7.334	698	705	715	rVB	2497110	3802363	26.40%	2.348%
6	7.534	732	739	749	rBV	2789896	4438645	30.81%	2.740%
7	8.010	811	820	831	rBV	2194596	3427372	23.79%	2.116%
8	8.710	931	939	953	rBV	3566895	5658780	39.29%	3.494%
9	9.175	1009	1018	1031	rBV	2677746	4308144	29.91%	2.660%
10	9.899	1130	1141	1157	rBV	2155618	3581257	24.86%	2.211%
11	10.440	1224	1233	1245	rBV	3536945	5917012	41.08%	3.653%
12	10.828	1291	1299	1308	rBV	3257505	5461163	37.91%	3.372%
13	10.957	1313	1321	1340	rBV	3893717	6526739	45.31%	4.029%
14	11.598	1425	1430	1434	rBV8	8285	16856	0.12%	0.010%
15	12.404	1560	1567	1573	rBV2	62186	104888	0.73%	0.065%
16	13.375	1726	1732	1737	rBV7	8449	21819	0.15%	0.013%
17	13.534	1754	1759	1767	rBV2	64078	103705	0.72%	0.064%
18	13.616	1770	1773	1780	rVB3	14151	21940	0.15%	0.014%
19	14.051	1839	1847	1859	rBV	6679586	9031471	62.70%	5.576%
20	14.339	1888	1896	1909	rBV	7721752	11039324	76.64%	6.815%
21	14.645	1941	1948	1957	rBV	5359372	7785375	54.05%	4.807%
22	14.722	1959	1961	1967	rVB7	11392	14938	0.10%	0.009%
23	14.828	1972	1979	1997	rBV	2476006	3616065	25.10%	2.232%
24	15.051	2014	2017	2024	rVB7	16924	28376	0.20%	0.018%
25	15.639	2110	2117	2127	rBV	9767041	13862551	96.24%	8.558%
26	15.745	2129	2135	2151	rVV	2513859	3458904	24.01%	2.135%
27	15.881	2153	2158	2163	rVB	44443	70286	0.49%	0.043%
28	16.428	2247	2251	2256	rVB7	11554	18131	0.13%	0.011%
29	17.075	2356	2361	2365	rBV6	12604	18221	0.13%	0.011%
30	17.186	2377	2380	2387	rVB2	12392	20487	0.14%	0.013%
31	17.398	2410	2416	2425	rBV	5890894	8542488	59.30%	5.274%
32	17.498	2427	2433	2447	rVV	10002534	14362880	99.71%	8.867%
33	17.775	2476	2480	2486	rBV8	8788	19146	0.13%	0.012%
34	19.304	2736	2740	2745	rBV2	106318	145400	1.01%	0.090%
35	19.369	2747	2751	2757	rBV	96041	145247	1.01%	0.090%
36	19.727	2806	2812	2824	rBV	10994105	14404350	100.00%	8.893%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012887.D
Acq On : 30 Nov 2022 20:05
Operator : CG/JU
Sample : PB149276BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	21.486	3106	3111	3122	rBV	4776744	6361561	44.16%	3.927%
38	23.833	3503	3510	3528	rVB2	5380291	11257638	78.15%	6.950%
39	23.998	3531	3538	3550	rVB	3132325	6270694	43.53%	3.871%




Sum of corrected areas: 161974825

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012887.D
Acq On : 30 Nov 2022 20:05
Operator : CG/JU
Sample : PB149276BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

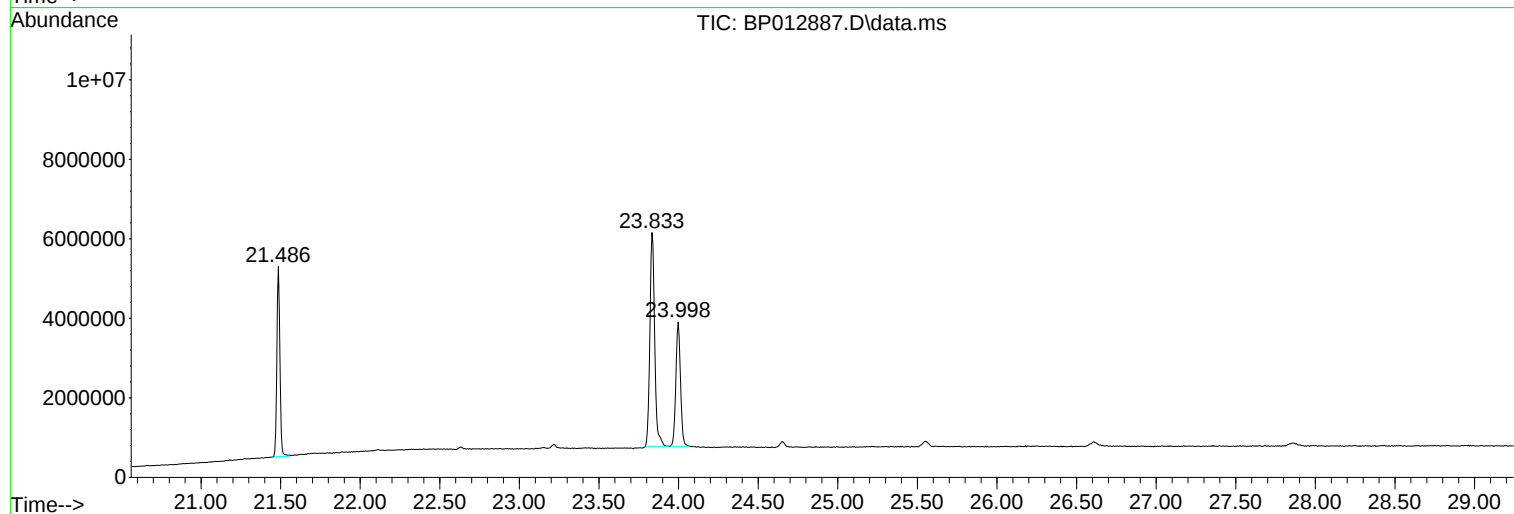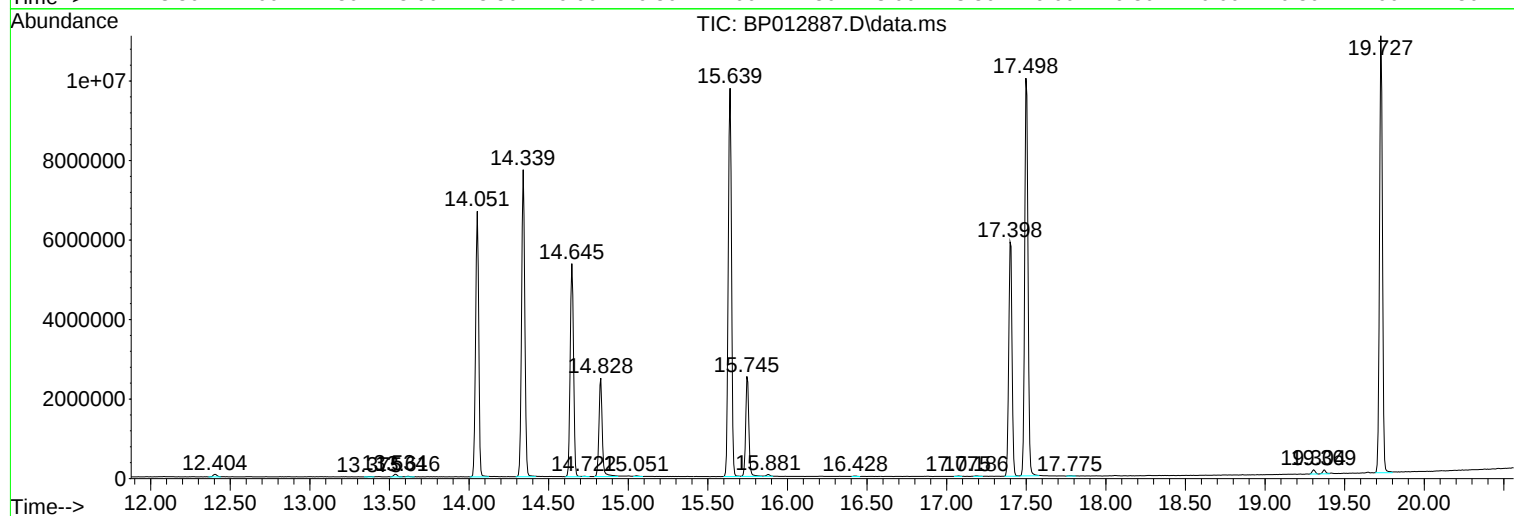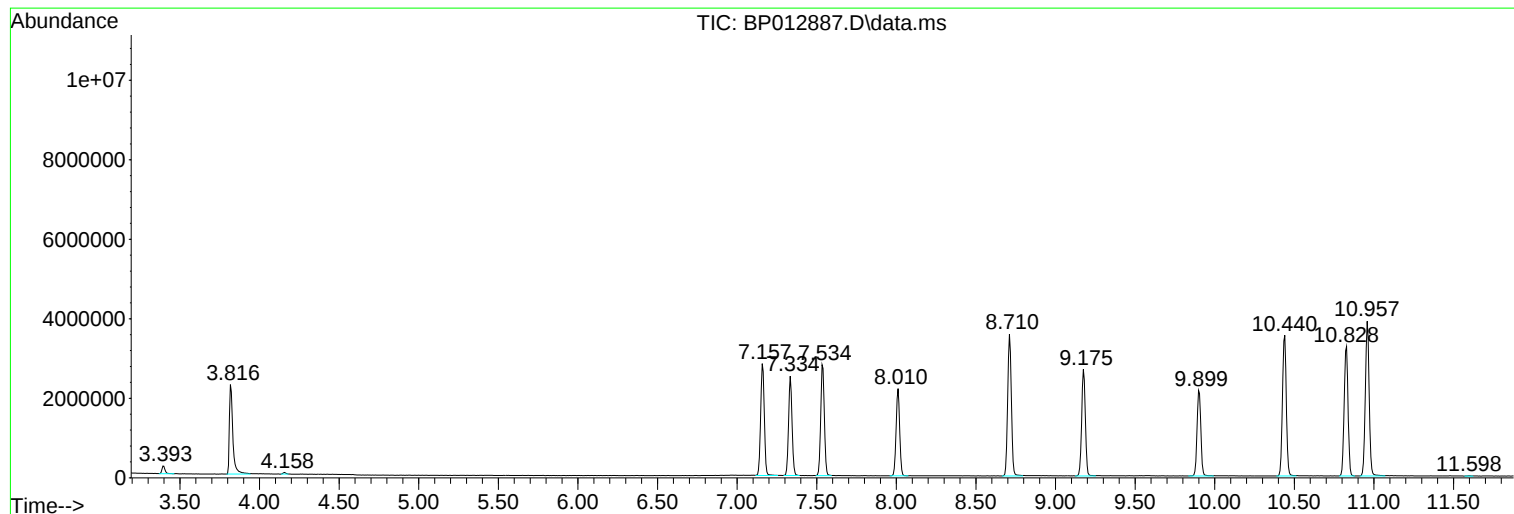

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012887.D
Acq On : 30 Nov 2022 20:05
Operator : CG/JU
Sample : PB149276BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012887.D
Acq On : 30 Nov 2022 20:05
Operator : CG/JU
Sample : PB149276BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc