

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012890.D
 Acq On : 30 Nov 2022 21:48
 Operator : CG/JU
 Sample : N5759-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	47	rVB	124382	177610	1.05%	0.117%
2	3.828	107	109	117	rBV	123512	199334	1.18%	0.131%
3	4.058	143	148	154	rVB	58446	88167	0.52%	0.058%
4	4.158	161	165	170	rVB	41517	61103	0.36%	0.040%
5	5.099	321	325	332	rVB4	11610	20614	0.12%	0.014%
6	7.157	669	675	682	rBV	617326	928753	5.51%	0.612%
7	7.334	698	705	716	rBV	2280575	3534321	20.97%	2.328%
8	7.534	731	739	751	rBV	2077267	3279394	19.46%	2.160%
9	8.010	812	820	828	rBV	2200609	3438727	20.41%	2.265%
10	8.710	931	939	951	rBV	1814745	2880410	17.09%	1.897%
11	9.175	1010	1018	1030	rBV	2606009	4146162	24.61%	2.731%
12	9.899	1131	1141	1157	rBV	2009508	3281346	19.47%	2.162%
13	10.440	1225	1233	1247	rBV	3063278	5252586	31.17%	3.460%
14	10.822	1290	1298	1309	rBV	3332864	5601856	33.24%	3.690%
15	10.957	1312	1321	1332	rBV	838142	1457979	8.65%	0.960%
16	11.593	1426	1429	1434	rBV5	13937	22244	0.13%	0.015%
17	12.404	1559	1567	1576	rBV2	63601	109496	0.65%	0.072%
18	12.616	1598	1603	1608	rBV8	9065	17193	0.10%	0.011%
19	13.269	1709	1714	1720	rBV	36248	55090	0.33%	0.036%
20	13.534	1753	1759	1766	rVB4	27534	44605	0.26%	0.029%
21	13.616	1768	1773	1780	rVB2	13642	24502	0.15%	0.016%
22	14.051	1840	1847	1861	rBV	6683794	9100693	54.01%	5.995%
23	14.157	1863	1865	1876	rVB10	8561	19228	0.11%	0.013%
24	14.339	1889	1896	1907	rBV2	7524615	11185277	66.38%	7.368%
25	14.645	1940	1948	1957	rBV	5811382	8253955	48.98%	5.437%
26	14.822	1969	1978	1999	rBV	401441	697101	4.14%	0.459%
27	14.998	2003	2008	2012	rVV7	11573	25085	0.15%	0.017%
28	15.051	2012	2017	2024	rVB8	24595	51317	0.30%	0.034%
29	15.298	2052	2059	2062	rBV4	36441	52851	0.31%	0.035%
30	15.639	2110	2117	2129	rBV	9736466	14347046	85.14%	9.451%
31	15.745	2129	2135	2148	rVV	2704690	3516420	20.87%	2.316%
32	15.875	2153	2157	2164	rVB3	42760	75008	0.45%	0.049%
33	16.422	2246	2250	2255	rVB5	10720	17265	0.10%	0.011%
34	17.069	2357	2360	2367	rVB8	10711	18083	0.11%	0.012%
35	17.186	2376	2380	2384	rBV2	15880	24833	0.15%	0.016%
36	17.398	2409	2416	2426	rBV	6892214	9795924	58.13%	6.453%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012890.D
 Acq On : 30 Nov 2022 21:48
 Operator : CG/JU
 Sample : N5759-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB78

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.498	2426	2433	2451	rVV	10688408	15335445	91.01%	10.102%
38	18.263	2559	2563	2571	rBV2	103278	144962	0.86%	0.095%
39	19.304	2736	2740	2746	rBV	125949	166493	0.99%	0.110%
40	19.369	2747	2751	2756	rVV	124887	179037	1.06%	0.118%
41	19.410	2756	2758	2762	rVB4	26988	31379	0.19%	0.021%
42	19.498	2769	2773	2779	rBV3	81169	110626	0.66%	0.073%
43	19.645	2795	2798	2802	rBV2	50849	56893	0.34%	0.037%
44	19.727	2806	2812	2825	rVV	12747944	16850310	100.00%	11.100%
45	21.486	3105	3111	3120	rBV	6507418	8621562	51.17%	5.679%
46	23.833	3503	3510	3526	rVB2	5556551	11483615	68.15%	7.565%
47	23.998	3531	3538	3552	rVB2	3340181	7025609	41.69%	4.628%




Sum of corrected areas: 151807509

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012890.D
Acq On : 30 Nov 2022 21:48
Operator : CG/JU
Sample : N5759-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

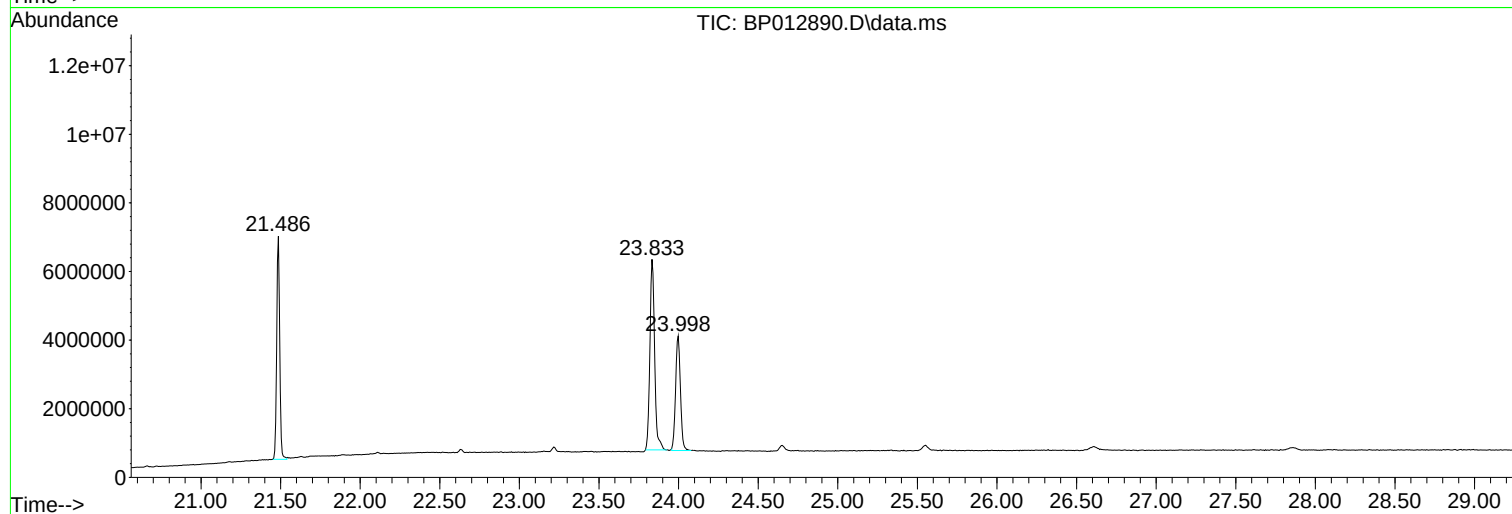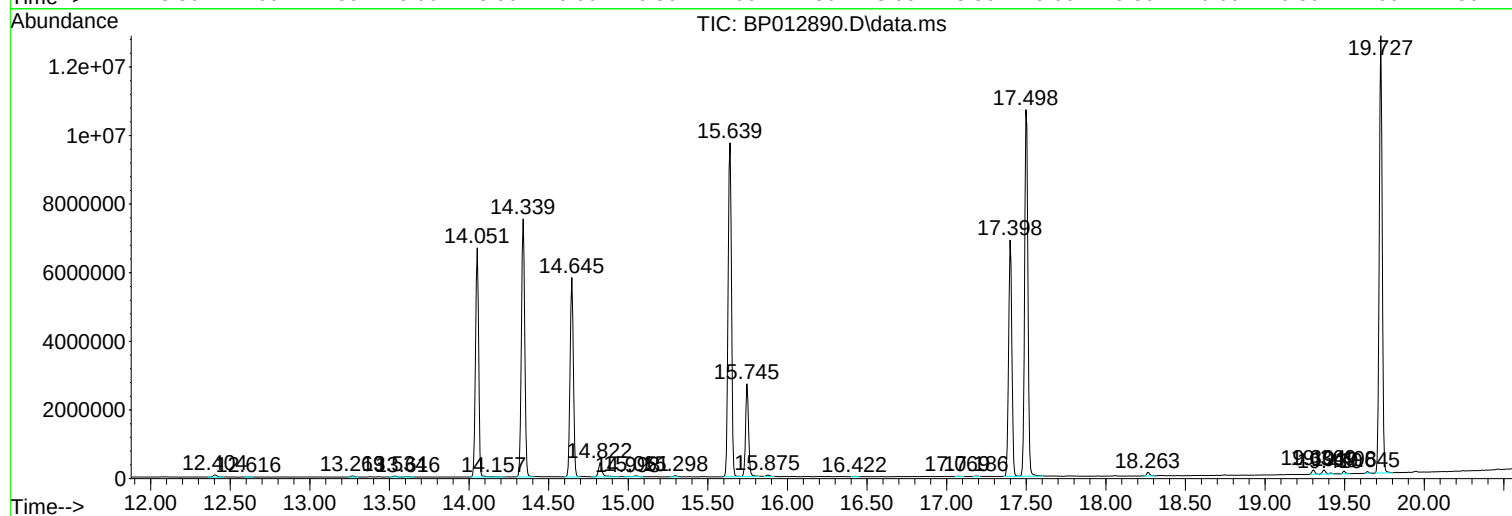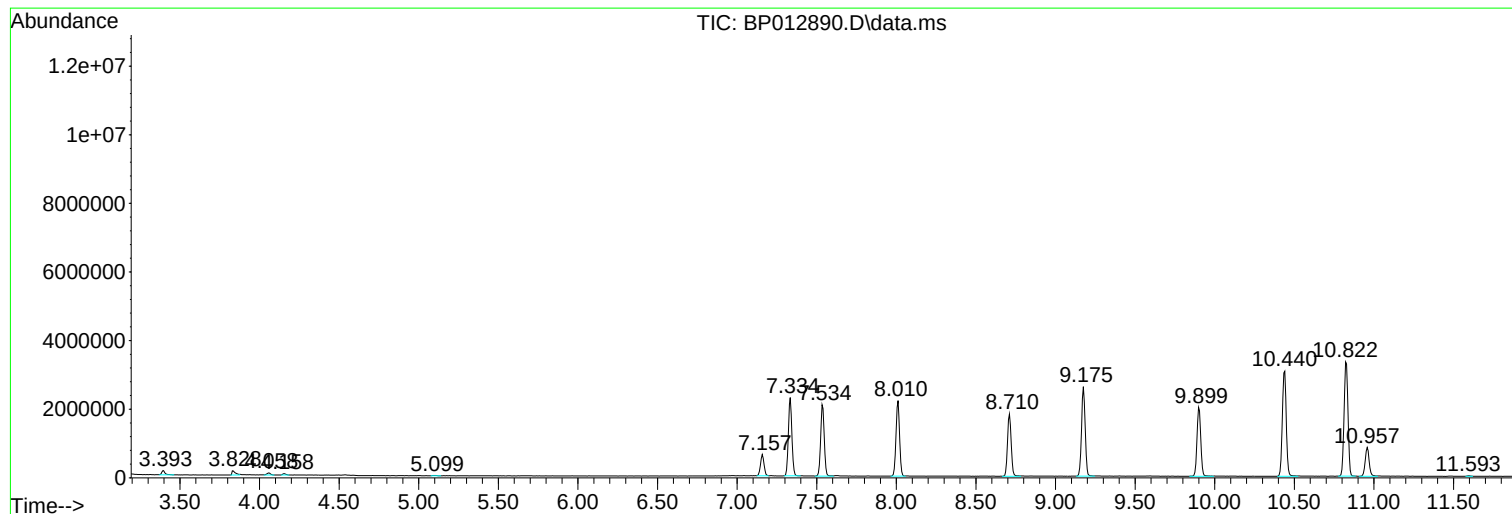

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012890.D
Acq On : 30 Nov 2022 21:48
Operator : CG/JU
Sample : N5759-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012890.D
Acq On : 30 Nov 2022 21:48
Operator : CG/JU
Sample : N5759-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
