

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012891.D
 Acq On : 30 Nov 2022 22:22
 Operator : CG/JU
 Sample : N5759-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	120518	157980	0.95%	0.107%
2	3.822	105	108	124	rBV	281780	482548	2.91%	0.327%
3	4.058	143	148	153	rVB	61299	87238	0.53%	0.059%
4	4.158	160	165	169	rBV	39045	54669	0.33%	0.037%
5	7.157	668	675	684	rVB	602464	901027	5.43%	0.611%
6	7.334	697	705	715	rBV	2268395	3536034	21.32%	2.397%
7	7.534	731	739	748	rBV	2001610	3154667	19.02%	2.139%
8	7.622	751	754	763	rVB7	13758	24630	0.15%	0.017%
9	8.010	812	820	828	rBV	2101855	3295638	19.87%	2.234%
10	8.710	932	939	952	rBV	1758845	2750656	16.58%	1.865%
11	9.175	1010	1018	1029	rBV	2568541	4078742	24.59%	2.765%
12	9.593	1085	1089	1094	rVB4	18144	29615	0.18%	0.020%
13	9.899	1133	1141	1155	rBV	1942649	3131228	18.88%	2.123%
14	10.434	1224	1232	1246	rBV	3016181	5064131	30.53%	3.433%
15	10.822	1289	1298	1307	rBV	3186981	5348628	32.25%	3.626%
16	10.957	1314	1321	1333	rBV	1125188	1889060	11.39%	1.281%
17	12.404	1560	1567	1574	rVB2	56491	99885	0.60%	0.068%
18	13.269	1708	1714	1719	rVB	45097	70827	0.43%	0.048%
19	13.381	1727	1733	1737	rBV6	12113	17488	0.11%	0.012%
20	13.463	1743	1747	1754	rVB3	16667	25377	0.15%	0.017%
21	13.534	1754	1759	1766	rVB4	22822	40915	0.25%	0.028%
22	13.610	1766	1772	1781	rVB5	14524	30708	0.19%	0.021%
23	14.051	1839	1847	1862	rBV	6717305	9211149	55.54%	6.245%
24	14.163	1862	1866	1871	rVB8	7906	17995	0.11%	0.012%
25	14.339	1889	1896	1912	rBV	7562266	11019298	66.44%	7.470%
26	14.645	1939	1948	1958	rBV	5288922	7802241	47.04%	5.289%
27	14.822	1972	1978	1990	rBV	379763	631554	3.81%	0.428%
28	15.045	2012	2016	2023	rVB8	27292	49543	0.30%	0.034%
29	15.292	2053	2058	2065	rBV8	14230	30613	0.18%	0.021%
30	15.639	2107	2117	2129	rBV	10059158	14585747	87.94%	9.888%
31	15.745	2129	2135	2151	rVV	2629860	3490520	21.05%	2.366%
32	15.875	2153	2157	2164	rVB2	47778	81770	0.49%	0.055%
33	15.998	2174	2178	2185	rVB	65769	89148	0.54%	0.060%
34	16.422	2244	2250	2256	rVB9	13245	29147	0.18%	0.020%
35	17.080	2357	2362	2366	rBV8	13142	21440	0.13%	0.015%
36	17.151	2369	2374	2376	rBV4	14879	19845	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012891.D
 Acq On : 30 Nov 2022 22:22
 Operator : CG/JU
 Sample : N5759-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.192	2376	2381	2386	rVB4	16046	30607	0.18%	0.021%
38	17.398	2410	2416	2426	rBV	6548117	8977851	54.13%	6.086%
39	17.498	2426	2433	2445	rBV	10851113	15712206	94.73%	10.652%
40	17.775	2476	2480	2484	rBV6	19330	31840	0.19%	0.022%
41	18.057	2524	2528	2532	rVB6	26338	32620	0.20%	0.022%
42	18.269	2559	2564	2573	rBV	295668	409271	2.47%	0.277%
43	18.680	2630	2634	2638	rBV	97690	115549	0.70%	0.078%
44	19.304	2736	2740	2745	rBV3	130308	179038	1.08%	0.121%
45	19.369	2746	2751	2756	rBV	128206	204530	1.23%	0.139%
46	19.498	2769	2773	2777	rBV	153774	187534	1.13%	0.127%
47	19.645	2795	2798	2803	rVB3	50667	59630	0.36%	0.040%
48	19.727	2806	2812	2826	rBV	12692794	16585759	100.00%	11.244%
49	19.945	2846	2849	2854	rBV	29199	44259	0.27%	0.030%
50	21.174	3055	3058	3063	rBV2	153264	205454	1.24%	0.139%
51	21.486	3105	3111	3124	rBV	5255830	6997542	42.19%	4.744%
52	23.833	3503	3510	3526	rVB2	5093398	10613369	63.99%	7.195%
53	23.992	3531	3537	3554	rVB2	2672704	5767911	34.78%	3.910%




Sum of corrected areas: 147506671

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012891.D
Acq On : 30 Nov 2022 22:22
Operator : CG/JU
Sample : N5759-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

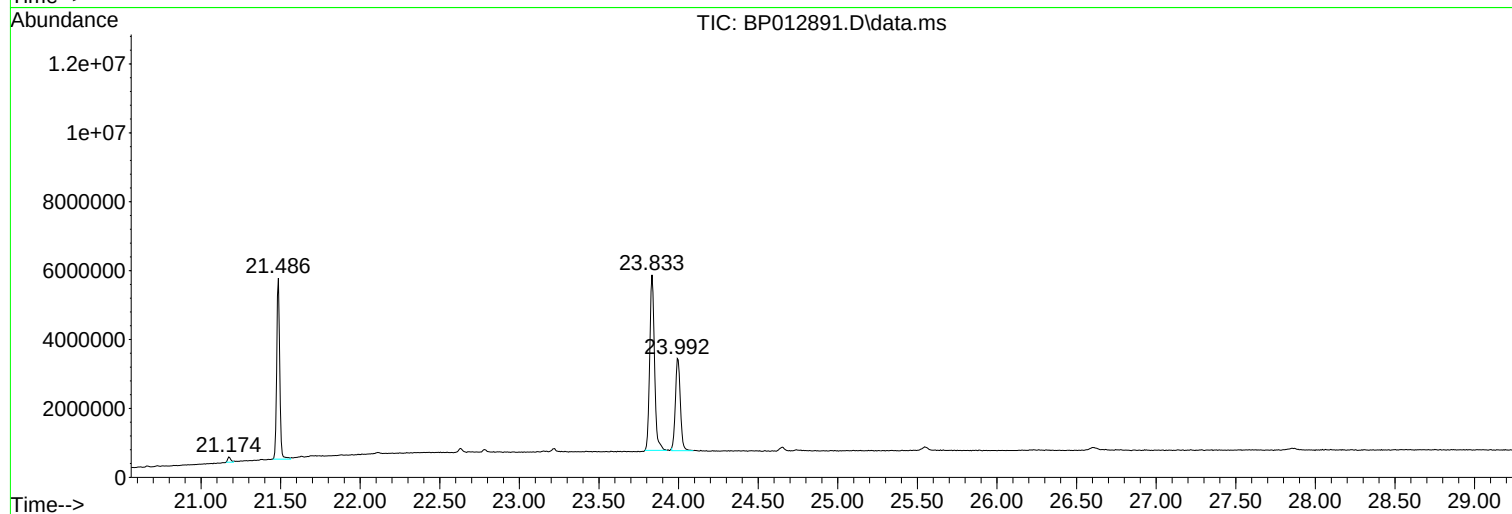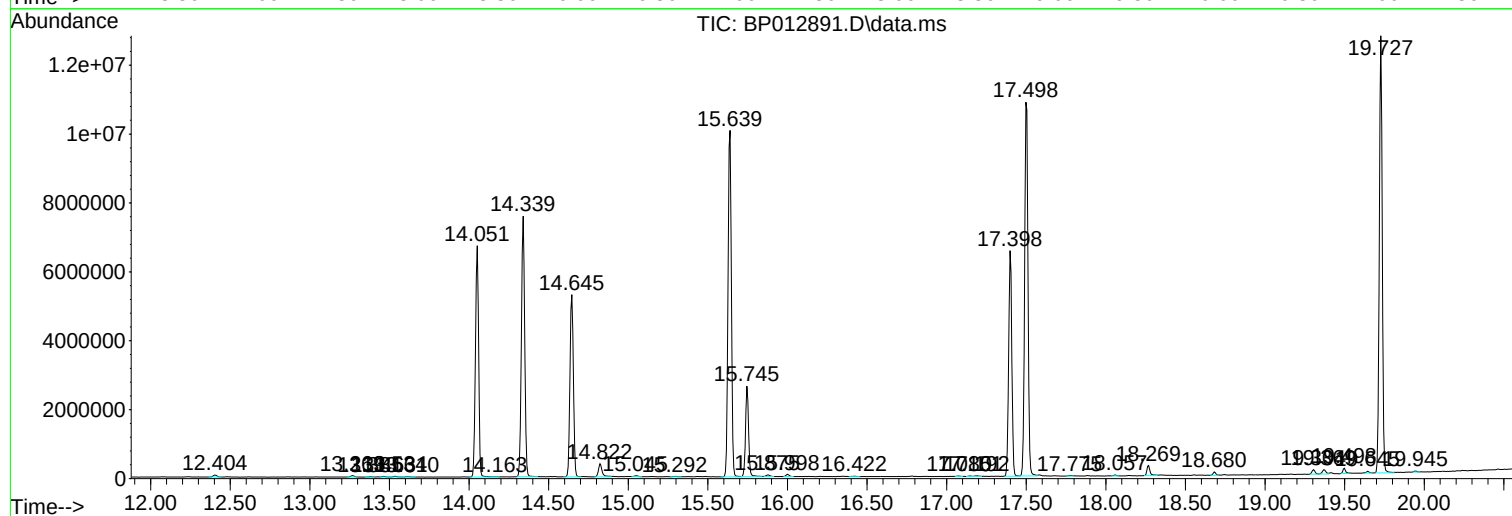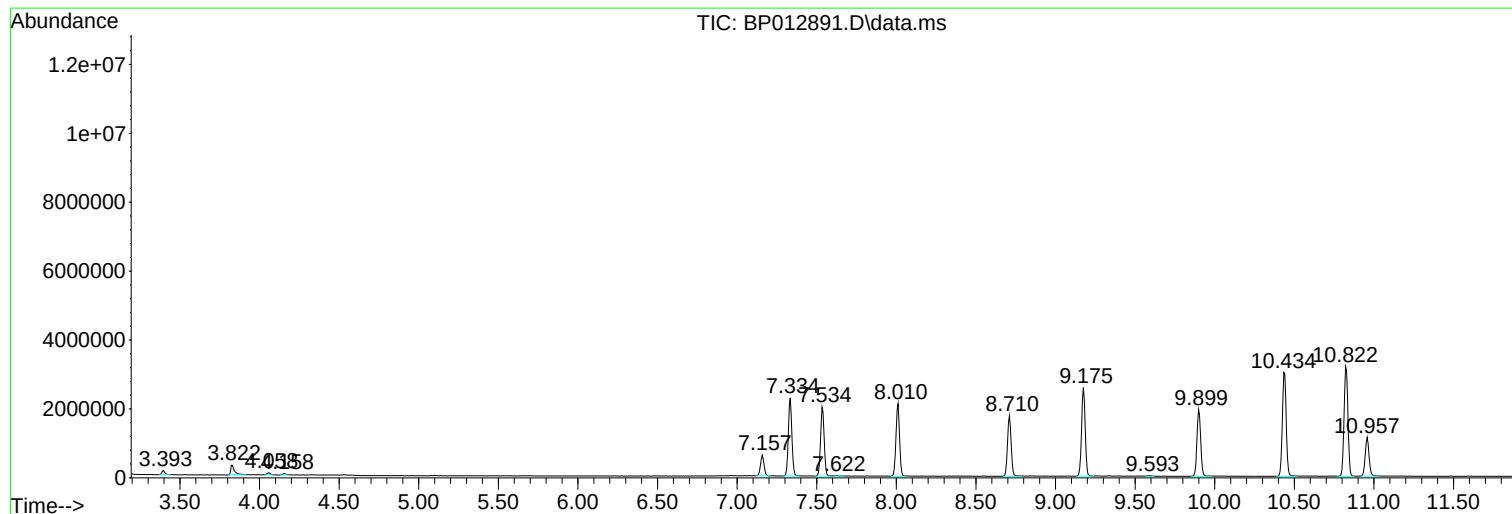

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012891.D
Acq On : 30 Nov 2022 22:22
Operator : CG/JU
Sample : N5759-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012891.D
Acq On : 30 Nov 2022 22:22
Operator : CG/JU
Sample : N5759-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc