

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012899.D
 Acq On : 01 Dec 2022 02:55
 Operator : CG/JU
 Sample : N5770-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	32	rBV2	32721	42166	0.44%	0.040%
2	3.393	32	35	43	rVB	139457	165668	1.74%	0.156%
3	3.822	105	108	120	rBV	321714	511874	5.36%	0.483%
4	4.058	143	148	154	rVB	60845	92299	0.97%	0.087%
5	4.152	160	164	171	rBV	46046	65534	0.69%	0.062%
6	4.693	251	256	264	rVB	128619	196271	2.06%	0.185%
7	4.799	270	274	281	rVB10	5392	10772	0.11%	0.010%
8	5.099	320	325	330	rVB3	19590	36227	0.38%	0.034%
9	5.493	388	392	398	rVB5	10211	18151	0.19%	0.017%
10	5.834	445	450	456	rVB	26975	37891	0.40%	0.036%
11	5.999	473	478	482	rBV4	16022	22364	0.23%	0.021%
12	6.969	639	643	645	rBV3	12200	16401	0.17%	0.015%
13	7.157	669	675	685	rVB	584904	915841	9.60%	0.864%
14	7.334	698	705	715	rBV	1933787	3002332	31.46%	2.832%
15	7.463	721	727	731	rVB4	15605	29139	0.31%	0.027%
16	7.534	732	739	749	rBV	1800447	2821162	29.56%	2.661%
17	7.622	751	754	758	rBV5	11056	17031	0.18%	0.016%
18	7.828	783	789	792	rBV6	6496	12441	0.13%	0.012%
19	8.010	812	820	826	rBV	2071468	3275592	34.32%	3.090%
20	8.069	826	830	834	rVB5	11384	17756	0.19%	0.017%
21	8.246	853	860	863	rBV8	4351	10174	0.11%	0.010%
22	8.710	929	939	953	rBV	1575743	2487004	26.06%	2.346%
23	9.110	1002	1007	1008	rBV5	6651	10028	0.11%	0.009%
24	9.175	1010	1018	1030	rVV	2110178	3387408	35.49%	3.195%
25	9.269	1030	1034	1039	rVB7	10440	18577	0.19%	0.018%
26	9.899	1132	1141	1154	rBV	1634566	2629827	27.55%	2.481%
27	10.434	1225	1232	1244	rBV	2449130	4142109	43.40%	3.907%
28	10.598	1256	1260	1269	rVB5	13822	26311	0.28%	0.025%
29	10.822	1289	1298	1306	rBV	3028887	5045685	52.87%	4.759%
30	10.957	1314	1321	1335	rBV	714408	1223330	12.82%	1.154%
31	11.057	1336	1338	1344	rVB7	7836	14884	0.16%	0.014%
32	11.216	1359	1365	1373	rVB7	11105	30896	0.32%	0.029%
33	11.481	1404	1410	1416	rVB7	9099	18126	0.19%	0.017%
34	11.598	1425	1430	1435	rBV9	7428	15990	0.17%	0.015%
35	12.081	1507	1512	1517	rBV7	6955	11849	0.12%	0.011%
36	12.404	1558	1567	1574	rBV	52135	93873	0.98%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012899.D
 Acq On : 01 Dec 2022 02:55
 Operator : CG/JU
 Sample : N5770-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	12.616	1601	1603	1607	rVB4	8671	9718	0.10%	0.009%
38	12.692	1612	1616	1621	rBV8	5943	10857	0.11%	0.010%
39	12.922	1646	1655	1661	rBV	179826	288688	3.02%	0.272%
40	13.269	1710	1714	1720	rVB	33556	53025	0.56%	0.050%
41	13.375	1727	1732	1737	rBV9	5594	11964	0.13%	0.011%
42	13.481	1746	1750	1755	rVB6	10165	13343	0.14%	0.013%
43	13.534	1755	1759	1767	rBV3	21839	40608	0.43%	0.038%
44	13.616	1767	1773	1777	rVV6	10595	15965	0.17%	0.015%
45	14.051	1838	1847	1860	rBV	4422828	6193979	64.90%	5.842%
46	14.169	1863	1867	1873	rVB8	13054	22755	0.24%	0.021%
47	14.292	1883	1888	1889	rBV5	12175	17377	0.18%	0.016%
48	14.339	1889	1896	1909	rVV	5496640	7784808	81.57%	7.343%
49	14.645	1941	1948	1958	rBV	4488320	6513233	68.24%	6.144%
50	14.828	1973	1979	1995	rBV	190016	359883	3.77%	0.339%
51	15.051	2013	2017	2022	rVB7	13700	24894	0.26%	0.023%
52	15.639	2109	2117	2129	rBV	6273925	9544254	100.00%	9.003%
53	15.745	2129	2135	2145	rBV	1245151	1655544	17.35%	1.562%
54	15.875	2151	2157	2164	rVB3	30578	59394	0.62%	0.056%
55	16.204	2208	2213	2221	rVB3	29673	49259	0.52%	0.046%
56	16.316	2230	2232	2238	rBV6	6352	13379	0.14%	0.013%
57	16.875	2322	2327	2332	rBV9	8660	16811	0.18%	0.016%
58	17.075	2357	2361	2367	rVB8	7816	15357	0.16%	0.014%
59	17.151	2370	2374	2376	rBV5	9853	13959	0.15%	0.013%
60	17.180	2376	2379	2387	rVB4	10998	21440	0.22%	0.020%
61	17.398	2410	2416	2426	rBV	4535093	6363563	66.67%	6.002%
62	17.498	2426	2433	2446	rBV	6070544	8713141	91.29%	8.219%
63	18.057	2526	2528	2535	rVB8	12131	12585	0.13%	0.012%
64	18.263	2559	2563	2569	rBV4	42890	65842	0.69%	0.062%
65	18.598	2616	2620	2622	rBV5	11601	18032	0.19%	0.017%
66	19.304	2736	2740	2745	rBV	63880	81817	0.86%	0.077%
67	19.369	2747	2751	2755	rBV2	60320	89865	0.94%	0.085%
68	19.492	2770	2772	2777	rVB3	29211	33723	0.35%	0.032%
69	19.639	2795	2797	2802	rVB4	27341	30683	0.32%	0.029%
70	19.727	2806	2812	2820	rBV	6437474	8647420	90.60%	8.157%
71	21.480	3105	3110	3117	rBV	3759934	5172166	54.19%	4.879%
72	23.827	3502	3509	3526	rVB2	3771556	8031355	84.15%	7.576%
73	23.992	3531	3537	3549	rVB2	2591010	5533199	57.97%	5.219%




Sum of corrected areas: 106016868

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012899.D
Acq On : 01 Dec 2022 02:55
Operator : CG/JU
Sample : N5770-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

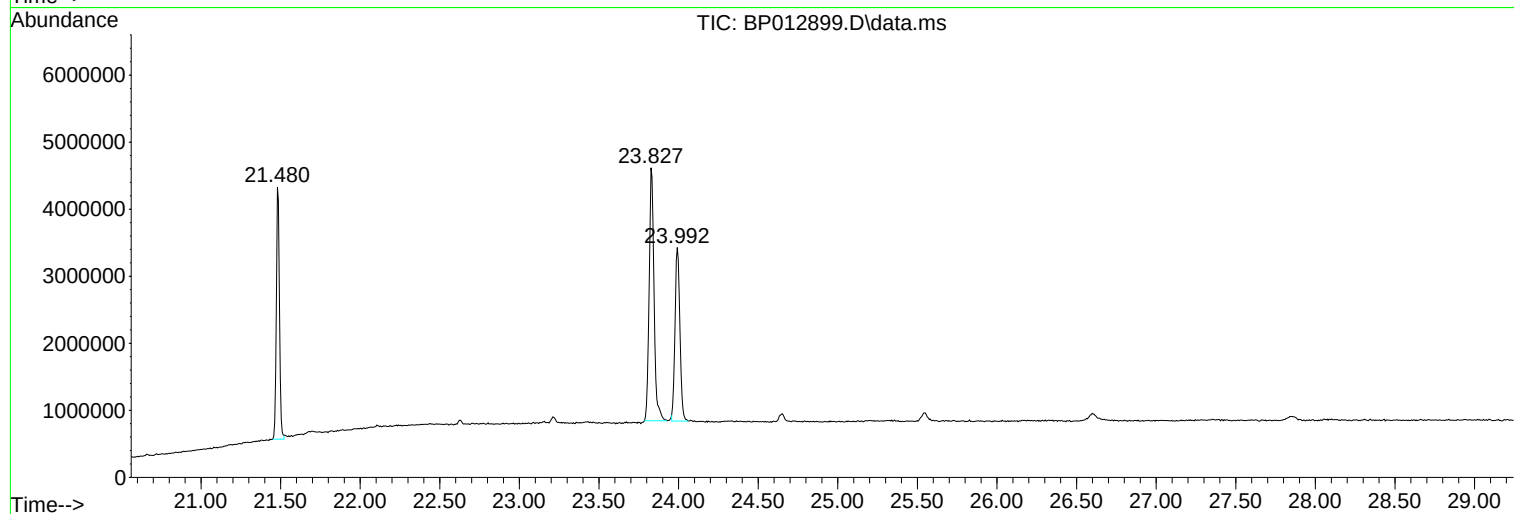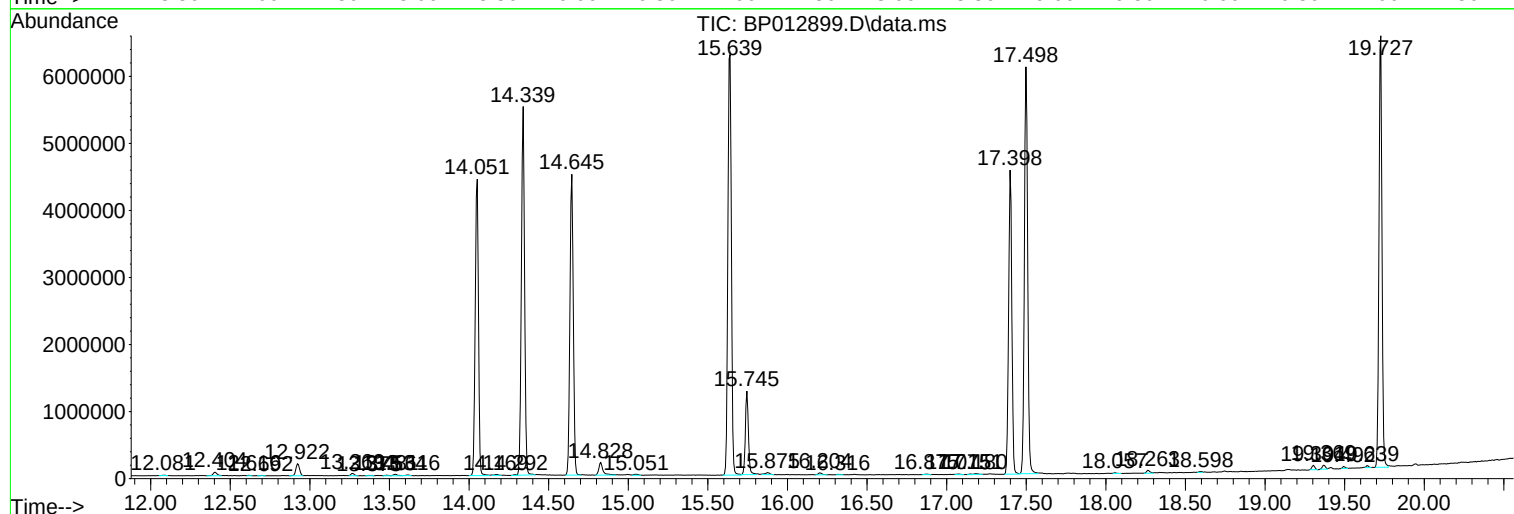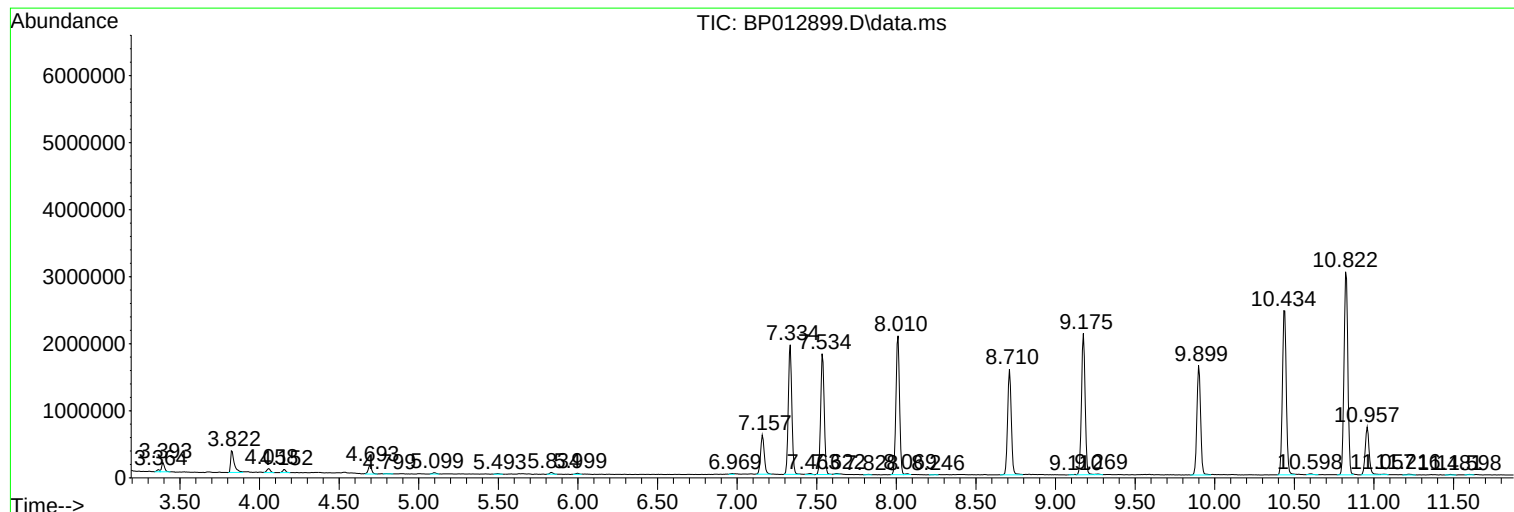

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012899.D
Acq On : 01 Dec 2022 02:55
Operator : CG/JU
Sample : N5770-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012899.D
Acq On : 01 Dec 2022 02:55
Operator : CG/JU
Sample : N5770-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1F9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc