

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012904.D
 Acq On : 01 Dec 2022 06:20
 Operator : CG/JU
 Sample : PB149319BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK319

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	179974	232176	1.82%	0.148%
2	3.816	103	107	123	rBV	2119765	3120228	24.39%	1.995%
3	4.152	161	164	170	rVB	48943	66700	0.52%	0.043%
4	7.157	668	675	686	rBV	2619380	4054748	31.70%	2.593%
5	7.334	698	705	716	rVB	2170917	3456792	27.03%	2.210%
6	7.534	732	739	748	rBV	2681705	4115069	32.17%	2.631%
7	8.010	811	820	827	rBV	2595085	4213755	32.94%	2.694%
8	8.710	931	939	949	rBV	3321433	5261288	41.13%	3.364%
9	9.175	1008	1018	1028	rBV	2501189	4021013	31.44%	2.571%
10	9.898	1134	1141	1152	rBV	2069211	3309801	25.88%	2.116%
11	10.434	1224	1232	1244	rBV	3365253	5540661	43.32%	3.543%
12	10.822	1288	1298	1307	rBV	4055304	6739160	52.69%	4.309%
13	10.957	1313	1321	1341	rBV	3370056	5794534	45.30%	3.705%
14	11.481	1404	1410	1416	rBV10	5807	15378	0.12%	0.010%
15	11.592	1424	1429	1436	rBV10	13967	31133	0.24%	0.020%
16	12.081	1506	1512	1514	rBV5	8696	15040	0.12%	0.010%
17	12.345	1551	1557	1561	rBV8	6042	13088	0.10%	0.008%
18	12.404	1561	1567	1573	rVB2	63953	104029	0.81%	0.067%
19	12.610	1595	1602	1607	rBV2	7050	16341	0.13%	0.010%
20	13.381	1728	1733	1737	rBV5	8565	14860	0.12%	0.010%
21	13.534	1751	1759	1767	rBV2	61575	105041	0.82%	0.067%
22	13.610	1770	1772	1780	rVB4	12975	22095	0.17%	0.014%
23	14.051	1839	1847	1859	rBV	5870191	8276215	64.71%	5.292%
24	14.339	1886	1896	1912	rBV	6993468	10137943	79.26%	6.482%
25	14.645	1941	1948	1957	rBV	6498525	9475597	74.08%	6.059%
26	14.822	1972	1978	1998	rBV	1972172	2995556	23.42%	1.915%
27	15.045	2013	2016	2023	rVB9	12152	20714	0.16%	0.013%
28	15.633	2106	2116	2126	rBV	8544175	12657123	98.96%	8.093%
29	15.745	2129	2135	2150	rVV	2013021	2799351	21.89%	1.790%
30	15.875	2152	2157	2165	rVB	41686	73696	0.58%	0.047%
31	16.422	2248	2250	2258	rVB9	14093	23045	0.18%	0.015%
32	17.075	2357	2361	2367	rVB8	10790	16074	0.13%	0.010%
33	17.186	2376	2380	2385	rVB	14259	22116	0.17%	0.014%
34	17.398	2409	2416	2426	rBV	7251580	10116496	79.09%	6.469%
35	17.498	2426	2433	2452	rVV	9098415	12790473	100.00%	8.178%
36	17.780	2475	2481	2483	rBV5	9815	15644	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012904.D
Acq On : 01 Dec 2022 06:20
Operator : CG/JU
Sample : PB149319BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	19.304	2736	2740	2744	rBV	92106	121384	0.95%	0.078%
38	19.369	2747	2751	2755	rBV	84945	110912	0.87%	0.071%
39	19.645	2795	2798	2803	rVB4	31388	35462	0.28%	0.023%
40	19.727	2806	2812	2823	rVV	9128520	12114394	94.71%	7.746%
41	21.486	3105	3111	3119	rBV	5159849	7113915	55.62%	4.549%
42	23.833	3502	3510	3524	rBV2	4622034	9725372	76.04%	6.219%
43	23.992	3530	3537	3550	rVB2	3497578	7487536	58.54%	4.788%




Sum of corrected areas: 156391948

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012904.D
Acq On : 01 Dec 2022 06:20
Operator : CG/JU
Sample : PB149319BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

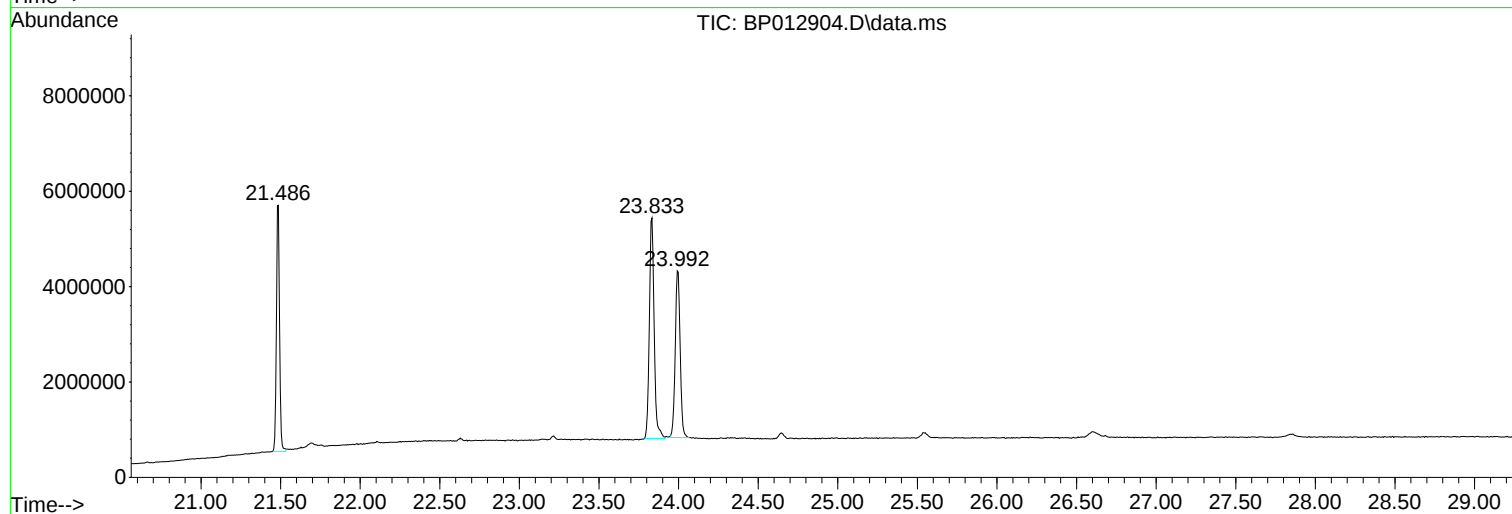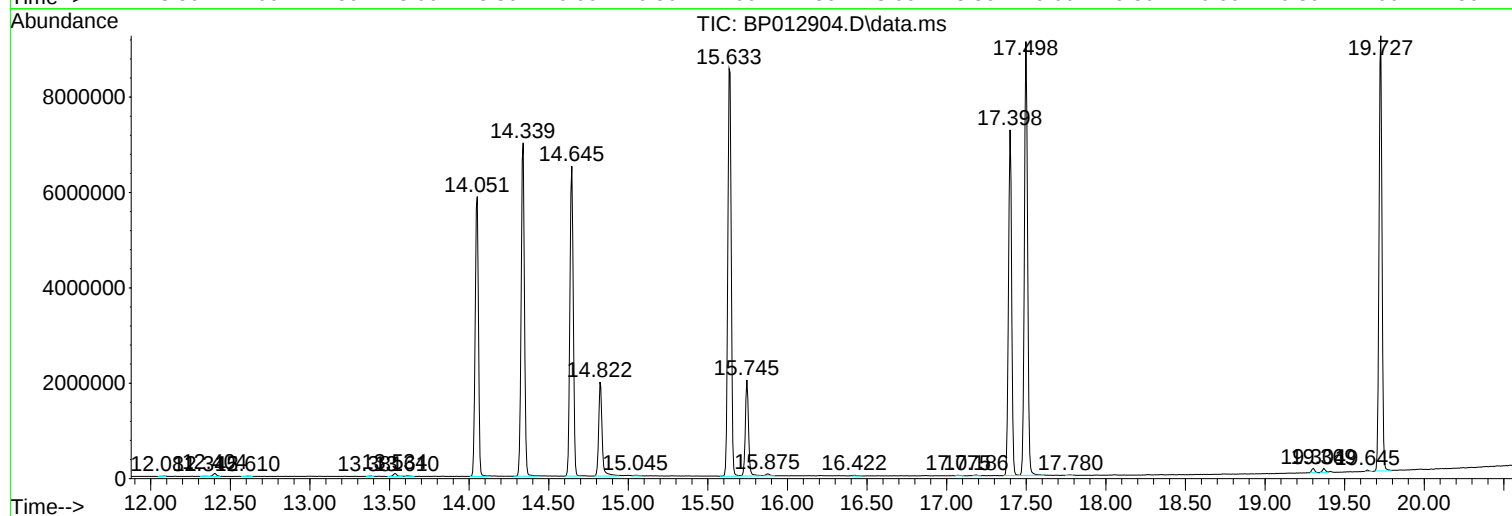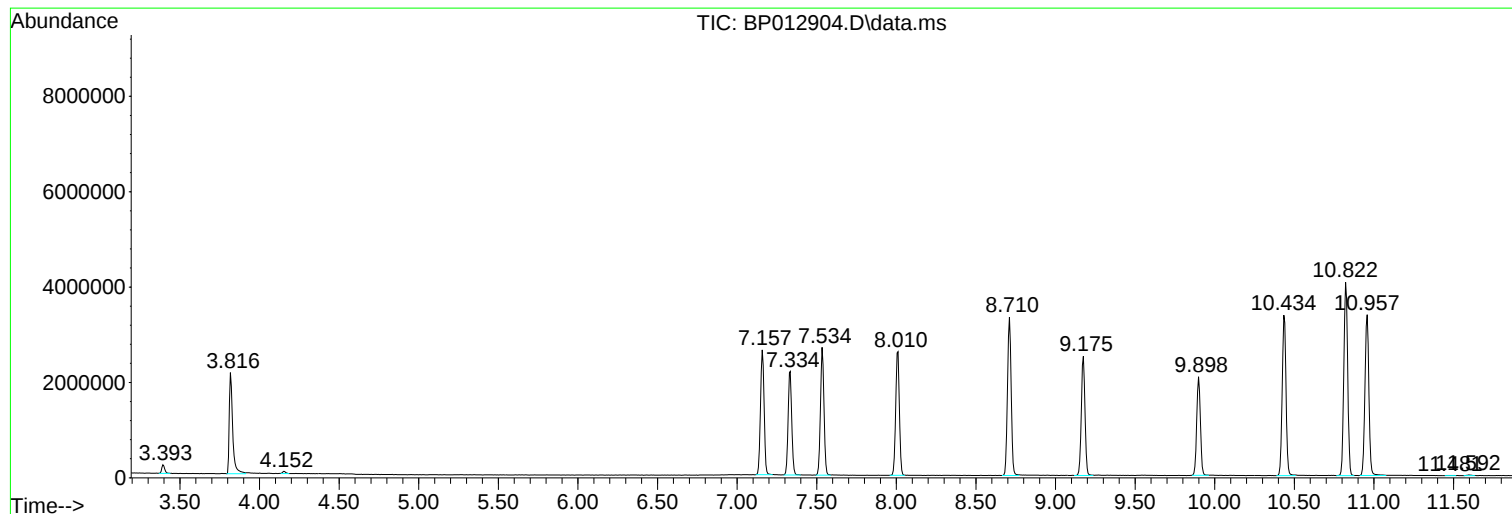

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012904.D
Acq On : 01 Dec 2022 06:20
Operator : CG/JU
Sample : PB149319BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012904.D
Acq On : 01 Dec 2022 06:20
Operator : CG/JU
Sample : PB149319BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc