

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012905.D
 Acq On : 01 Dec 2022 06:54
 Operator : CG/JU
 Sample : PB149320BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK320

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	41	rBV	172764	218358	1.46%	0.136%
2	3.817	104	107	126	rBV	2157922	3241718	21.62%	2.015%
3	4.152	160	164	171	rVB	43505	64125	0.43%	0.040%
4	7.158	668	675	691	rVB	2573867	3929868	26.21%	2.443%
5	7.334	698	705	714	rVB	2090324	3333282	22.23%	2.072%
6	7.534	731	739	753	rBV	2544471	3945531	26.32%	2.452%
7	8.005	812	819	827	rBV	2361108	3816719	25.46%	2.372%
8	8.710	930	939	953	rBV	3194748	5157240	34.40%	3.205%
9	9.175	1011	1018	1029	rBV	2377452	3859819	25.75%	2.399%
10	9.899	1134	1141	1154	rBV	1985346	3196174	21.32%	1.987%
11	10.434	1224	1232	1248	rBV	3310310	5436950	36.26%	3.379%
12	10.822	1290	1298	1310	rVB	3656805	6174513	41.18%	3.838%
13	10.957	1310	1321	1334	rBV	3245796	5471604	36.50%	3.401%
14	11.598	1426	1430	1437	rVB7	13058	22721	0.15%	0.014%
15	12.075	1505	1511	1517	rBV9	7321	17560	0.12%	0.011%
16	12.404	1560	1567	1572	rBV	56058	96927	0.65%	0.060%
17	13.381	1728	1733	1738	rBV8	8236	16481	0.11%	0.010%
18	13.540	1752	1760	1763	rBV7	14609	24316	0.16%	0.015%
19	13.616	1766	1773	1779	rVB5	13978	25810	0.17%	0.016%
20	14.045	1840	1846	1860	rBV	5859132	8440904	56.30%	5.246%
21	14.340	1888	1896	1918	rBV	6919590	10214044	68.13%	6.349%
22	14.645	1941	1948	1957	rBV	6168473	9052827	60.38%	5.627%
23	14.822	1971	1978	1999	rBV	2302464	3474944	23.18%	2.160%
24	15.634	2108	2116	2128	rBV	9068992	13028057	86.90%	8.098%
25	15.745	2129	2135	2145	rVV	2277526	2989217	19.94%	1.858%
26	15.875	2153	2157	2162	rVB2	39806	58122	0.39%	0.036%
27	16.422	2246	2250	2255	rVB7	11736	17653	0.12%	0.011%
28	17.181	2376	2379	2385	rVB3	16636	26397	0.18%	0.016%
29	17.398	2409	2416	2426	rBV	7567643	10588134	70.62%	6.581%
30	17.498	2426	2433	2444	rBV	9851510	13979353	93.24%	8.689%
31	18.269	2560	2564	2566	rBV5	10355	16360	0.11%	0.010%
32	19.304	2736	2740	2745	rVB2	110277	146354	0.98%	0.091%
33	19.369	2747	2751	2756	rBV	96551	132362	0.88%	0.082%
34	19.639	2795	2797	2802	rVB3	28374	33275	0.22%	0.021%
35	19.727	2806	2812	2823	rBV	11407739	14992366	100.00%	9.319%
36	21.480	3105	3110	3121	rBV	6273282	8559477	57.09%	5.320%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012905.D
Acq On : 01 Dec 2022 06:54
Operator : CG/JU
Sample : PB149320BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	23.827	3502	3509	3526	rBV	4747456	9948800	66.36%	6.184%
38	23.992	3530	3537	3551	rVB2	3395956	7139389	47.62%	4.437%




Sum of corrected areas: 160887751

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012905.D
Acq On : 01 Dec 2022 06:54
Operator : CG/JU
Sample : PB149320BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

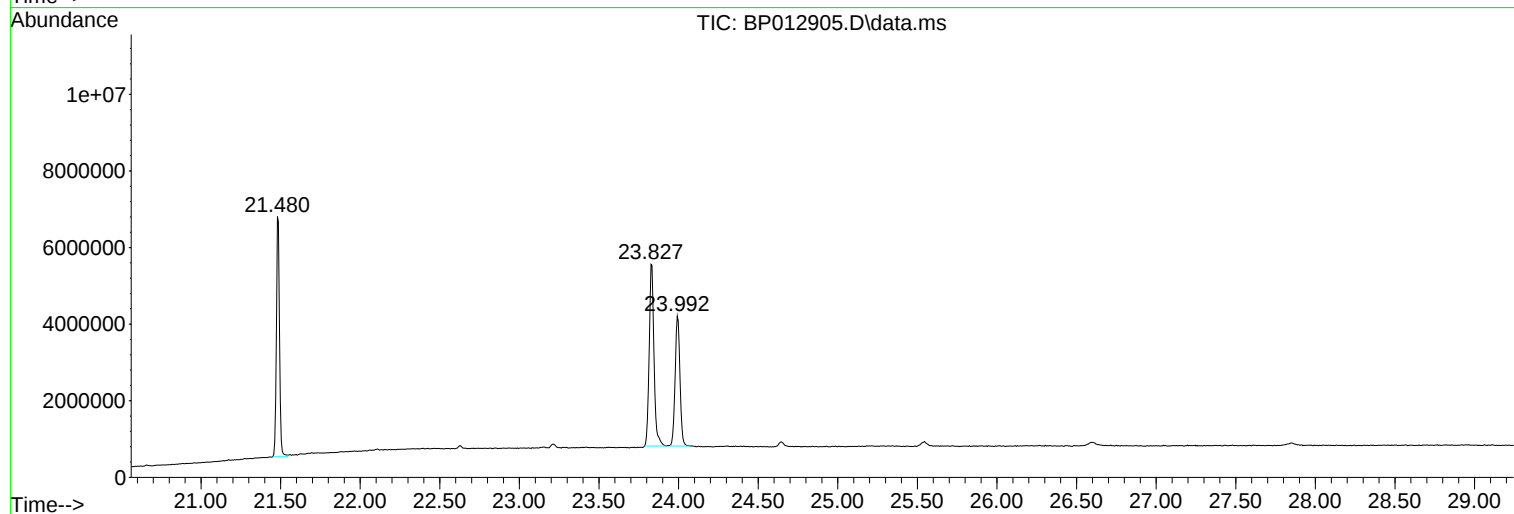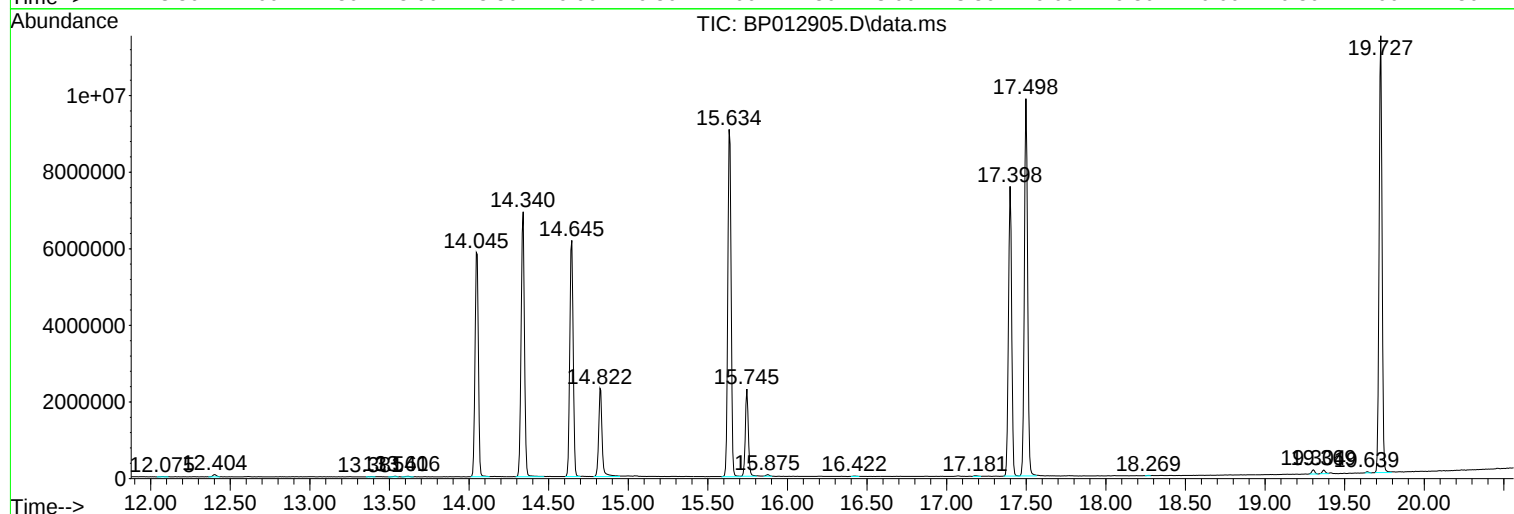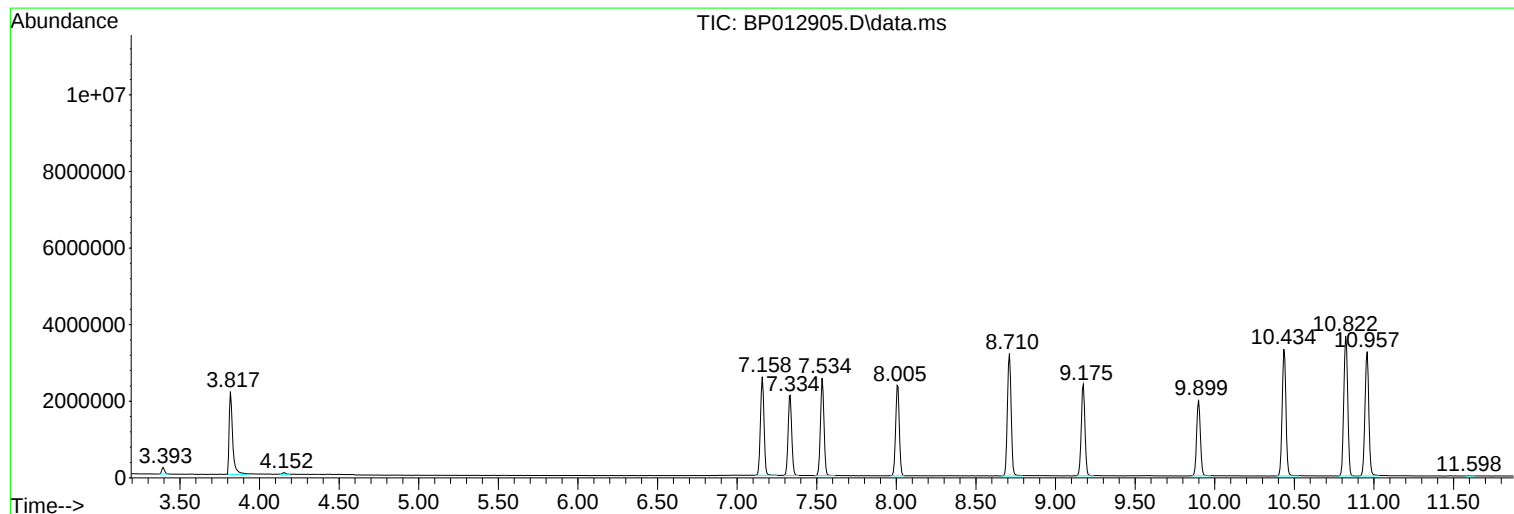

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012905.D
Acq On : 01 Dec 2022 06:54
Operator : CG/JU
Sample : PB149320BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012905.D
Acq On : 01 Dec 2022 06:54
Operator : CG/JU
Sample : PB149320BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc