

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012907.D
 Acq On : 01 Dec 2022 08:02
 Operator : CG/JU
 Sample : N5770-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	40	rBV	121856	156176	0.80%	0.094%
2	3.822	105	108	122	rBV	300053	495597	2.52%	0.298%
3	4.058	143	148	154	rVB	65400	102028	0.52%	0.061%
4	4.152	160	164	169	rBV	60161	79864	0.41%	0.048%
5	7.158	666	675	685	rVB	689007	1073482	5.47%	0.645%
6	7.334	698	705	715	rVB	2271626	3612850	18.41%	2.170%
7	7.534	731	739	748	rBV	2144715	3396798	17.31%	2.040%
8	7.622	750	754	763	rVB8	15518	24996	0.13%	0.015%
9	8.005	812	819	828	rBV	2145669	3422797	17.44%	2.055%
10	8.710	932	939	948	rBV	1957845	3099496	15.79%	1.861%
11	9.175	1010	1018	1027	rBV	2634517	4278705	21.80%	2.569%
12	9.257	1030	1032	1041	rVB10	9931	22955	0.12%	0.014%
13	9.899	1129	1141	1151	rBV	1995767	3265115	16.63%	1.961%
14	10.434	1225	1232	1250	rBV	3251846	5305050	27.03%	3.186%
15	10.822	1289	1298	1308	rBV	3304435	5594287	28.50%	3.360%
16	10.957	1310	1321	1334	rBV	1014831	1785904	9.10%	1.072%
17	12.081	1505	1512	1517	rBV2	34145	53828	0.27%	0.032%
18	12.404	1559	1567	1575	rBV3	73018	135612	0.69%	0.081%
19	13.263	1708	1713	1721	rVB	50103	76347	0.39%	0.046%
20	13.534	1753	1759	1764	rBV2	26966	40105	0.20%	0.024%
21	13.616	1767	1773	1777	rVV5	12191	21624	0.11%	0.013%
22	13.963	1826	1832	1838	rBV7	13147	24728	0.13%	0.015%
23	14.045	1840	1846	1862	rVV	6659248	9379138	47.78%	5.632%
24	14.340	1888	1896	1907	rBV	7628671	11484998	58.51%	6.897%
25	14.645	1939	1948	1957	rBV	5561311	8404645	42.82%	5.047%
26	14.822	1972	1978	1997	rBV	438973	747692	3.81%	0.449%
27	15.051	2012	2017	2022	rVB7	33962	50775	0.26%	0.030%
28	15.634	2108	2116	2128	rBV	10338006	15147951	77.17%	9.097%
29	15.745	2129	2135	2151	rVV	2199347	2949164	15.02%	1.771%
30	15.875	2151	2157	2166	rVB2	50384	90289	0.46%	0.054%
31	16.422	2247	2250	2257	rVB6	14653	23189	0.12%	0.014%
32	16.869	2320	2326	2332	rBV	64968	90754	0.46%	0.055%
33	17.075	2357	2361	2365	rVB6	13543	19960	0.10%	0.012%
34	17.181	2376	2379	2385	rVB4	13845	21475	0.11%	0.013%
35	17.398	2409	2416	2426	rBV	7226470	10216235	52.05%	6.135%
36	17.498	2426	2433	2444	rVV	11875352	17040990	86.82%	10.234%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012907.D
 Acq On : 01 Dec 2022 08:02
 Operator : CG/JU
 Sample : N5770-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.581	2444	2447	2457	rVB8	52258	93025	0.47%	0.056%
38	17.945	2505	2509	2512	rBV3	31586	38544	0.20%	0.023%
39	18.263	2559	2563	2569	rBV2	62977	91118	0.46%	0.055%
40	19.304	2735	2740	2744	rBV	146781	195052	0.99%	0.117%
41	19.369	2746	2751	2756	rVV	136825	200907	1.02%	0.121%
42	19.410	2756	2758	2764	rVB6	33162	41453	0.21%	0.025%
43	19.492	2769	2772	2776	rBV3	38053	50507	0.26%	0.030%
44	19.645	2795	2798	2802	rVB	49948	55372	0.28%	0.033%
45	19.727	2805	2812	2824	rBV	15132982	19628666	100.00%	11.788%
46	19.939	2846	2848	2853	rVB2	30055	36215	0.18%	0.022%
47	21.486	3105	3111	3122	rBV	7173791	10152540	51.72%	6.097%
48	23.833	3502	3510	3528	rVB	7223073	15644143	79.70%	9.395%
49	23.992	3530	3537	3549	rVB2	3970281	8556311	43.59%	5.138%




Sum of corrected areas: 166519452

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012907.D
Acq On : 01 Dec 2022 08:02
Operator : CG/JU
Sample : N5770-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

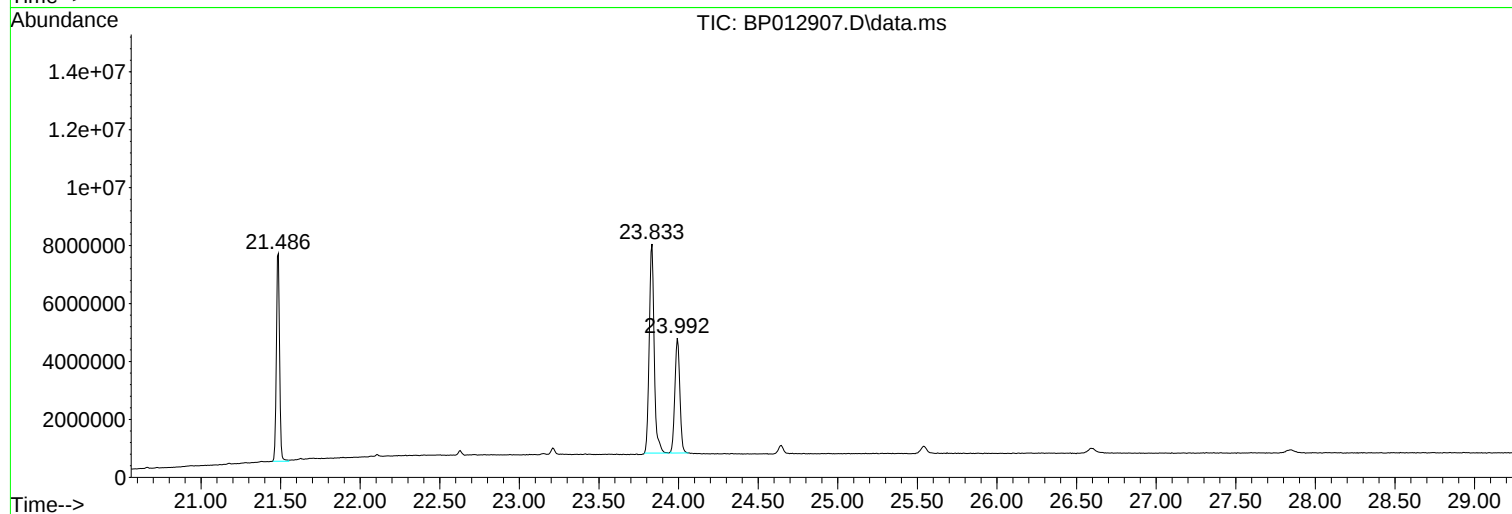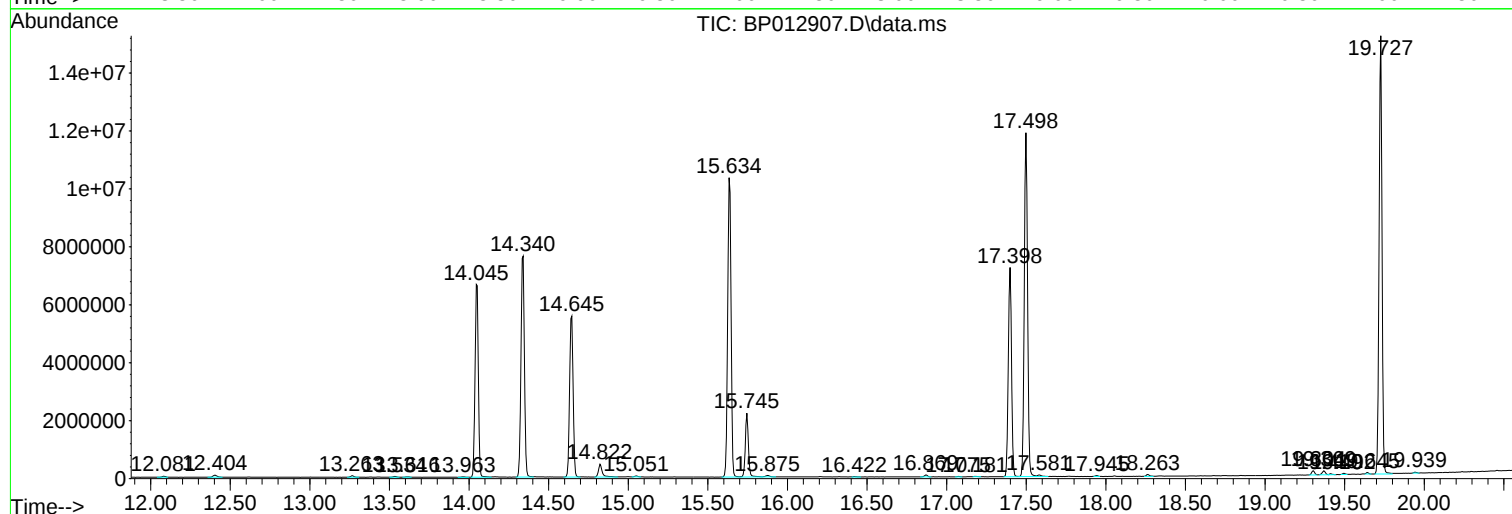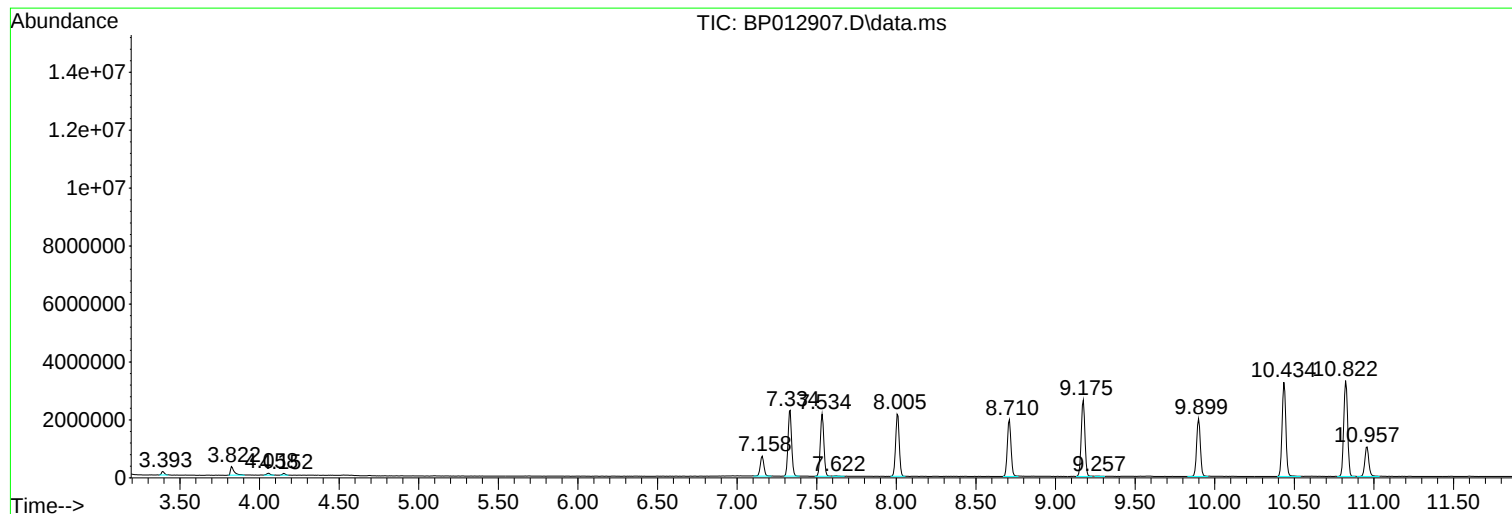

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012907.D
Acq On : 01 Dec 2022 08:02
Operator : CG/JU
Sample : N5770-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012907.D
Acq On : 01 Dec 2022 08:02
Operator : CG/JU
Sample : N5770-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc