

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012908.D
 Acq On : 01 Dec 2022 08:36
 Operator : CG/JU
 Sample : N5770-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	47	rVB	153301	227682	0.97%	0.120%
2	3.828	106	109	121	rBV	222790	368783	1.57%	0.195%
3	3.928	122	126	131	rVB	78856	102043	0.43%	0.054%
4	4.058	143	148	153	rVB	61891	95097	0.40%	0.050%
5	4.152	160	164	169	rBV	52484	71627	0.30%	0.038%
6	4.693	251	256	263	rVB6	33656	65100	0.28%	0.034%
7	5.099	319	325	329	rBV2	31882	47025	0.20%	0.025%
8	7.157	668	675	684	rVB	965406	1488380	6.33%	0.786%
9	7.334	697	705	716	rBV	2845215	4546813	19.33%	2.402%
10	7.534	732	739	749	rBV	2950682	4556134	19.37%	2.407%
11	8.010	812	820	827	rBV	1978296	3190614	13.56%	1.686%
12	8.710	929	939	951	rBV	2539224	4072662	17.31%	2.152%
13	9.175	1010	1018	1030	rBV	3366821	5445712	23.15%	2.877%
14	9.269	1030	1034	1038	rVV5	16664	29550	0.13%	0.016%
15	9.898	1133	1141	1156	rBV	2721576	4455896	18.94%	2.354%
16	10.434	1224	1232	1245	rBV	4441345	7375152	31.35%	3.897%
17	10.598	1255	1260	1265	rBV6	12907	24795	0.11%	0.013%
18	10.822	1288	1298	1306	rBV	3118510	5146461	21.88%	2.719%
19	10.957	1314	1321	1335	rBV	476293	842428	3.58%	0.445%
20	11.475	1402	1409	1416	rBV3	14718	34066	0.14%	0.018%
21	11.593	1425	1429	1434	rBV7	12626	24192	0.10%	0.013%
22	12.081	1506	1512	1521	rVB9	10937	24752	0.11%	0.013%
23	12.398	1562	1566	1575	rVB	83479	148377	0.63%	0.078%
24	12.628	1599	1605	1612	rVB2	15213	34086	0.14%	0.018%
25	12.922	1650	1655	1660	rVB2	72011	109464	0.47%	0.058%
26	13.263	1708	1713	1720	rVB	46966	75654	0.32%	0.040%
27	13.610	1765	1772	1778	rBV4	19119	38967	0.17%	0.021%
28	14.051	1839	1847	1858	rBV	8576136	12042684	51.19%	6.363%
29	14.163	1863	1866	1875	rVB	18541	34408	0.15%	0.018%
30	14.339	1889	1896	1914	rVB	9764175	14500773	61.64%	7.662%
31	14.645	1941	1948	1957	rVB	5040486	7450800	31.67%	3.937%
32	14.822	1972	1978	2001	rBV	785878	1282941	5.45%	0.678%
33	14.986	2001	2006	2011	rVV6	26888	53813	0.23%	0.028%
34	15.045	2012	2016	2025	rVB9	35716	59002	0.25%	0.031%
35	15.639	2109	2117	2129	rBV	12932210	19069979	81.07%	10.076%
36	15.745	2129	2135	2145	rBV	3875153	5182612	22.03%	2.738%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012908.D
 Acq On : 01 Dec 2022 08:36
 Operator : CG/JU
 Sample : N5770-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.875	2153	2157	2165	rVB	60251	95113	0.40%	0.050%
38	16.204	2208	2213	2220	rVB8	22495	37434	0.16%	0.020%
39	16.322	2227	2233	2236	rBV8	12925	23818	0.10%	0.013%
40	16.422	2243	2250	2255	rVB4	17652	38085	0.16%	0.020%
41	16.933	2333	2337	2342	rVB2	23855	31158	0.13%	0.016%
42	17.275	2391	2395	2398	rVB4	17743	26097	0.11%	0.014%
43	17.398	2409	2416	2426	rBV	6421802	8972543	38.14%	4.741%
44	17.498	2426	2433	2447	rBV	14240824	20173686	85.76%	10.660%
45	17.775	2472	2480	2482	rBV5	31567	59482	0.25%	0.031%
46	18.057	2524	2528	2532	rVB5	28093	34983	0.15%	0.018%
47	18.263	2559	2563	2571	rBV	264990	366678	1.56%	0.194%
48	18.345	2574	2577	2581	rVB4	21825	29773	0.13%	0.016%
49	18.592	2616	2619	2625	rBV7	23050	36287	0.15%	0.019%
50	18.680	2630	2634	2640	rVB2	86742	99965	0.42%	0.053%
51	18.745	2640	2645	2648	rBV3	55904	81646	0.35%	0.043%
52	19.304	2735	2740	2745	rBV2	197253	262122	1.11%	0.139%
53	19.369	2746	2751	2754	rBV	195576	306885	1.30%	0.162%
54	19.492	2769	2772	2778	rBV	188976	243831	1.04%	0.129%
55	19.639	2795	2797	2802	rVB2	68410	77580	0.33%	0.041%
56	19.727	2806	2812	2827	rVV	17710480	23524181	100.00%	12.430%
57	21.480	3105	3110	3121	rBV	6030694	8401690	35.72%	4.439%
58	23.833	3502	3510	3526	rVV	8237940	17186233	73.06%	9.081%
59	23.992	3530	3537	3552	rVB2	3202380	6826786	29.02%	3.607%




Sum of corrected areas: 189254580

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012908.D
Acq On : 01 Dec 2022 08:36
Operator : CG/JU
Sample : N5770-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

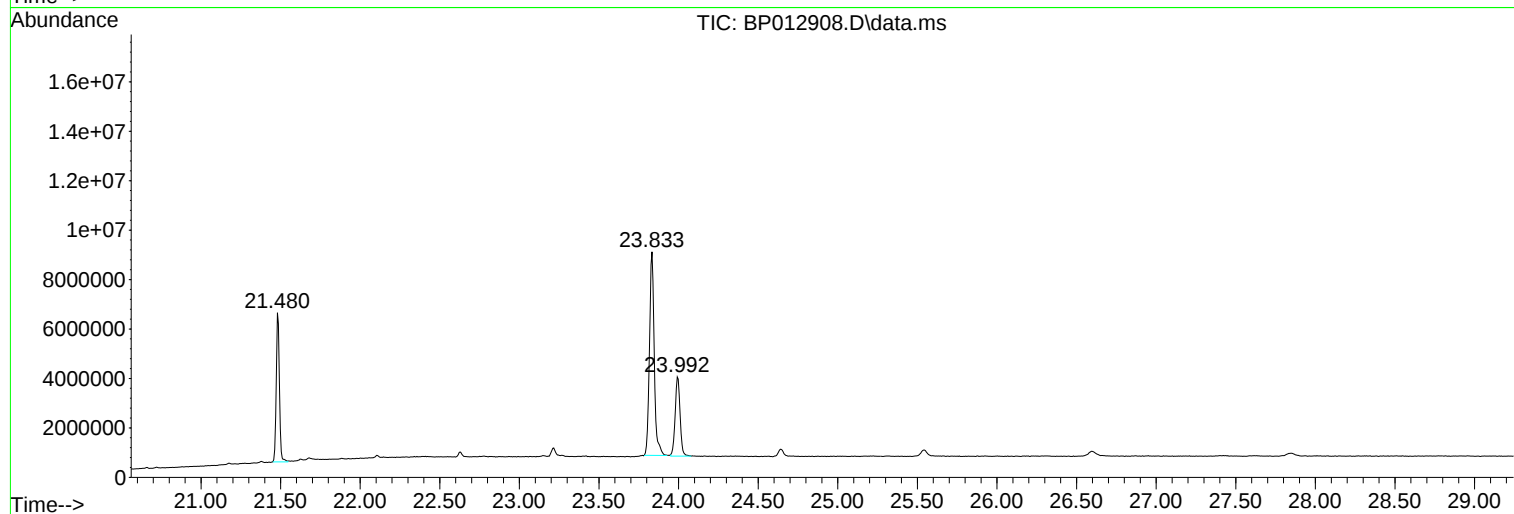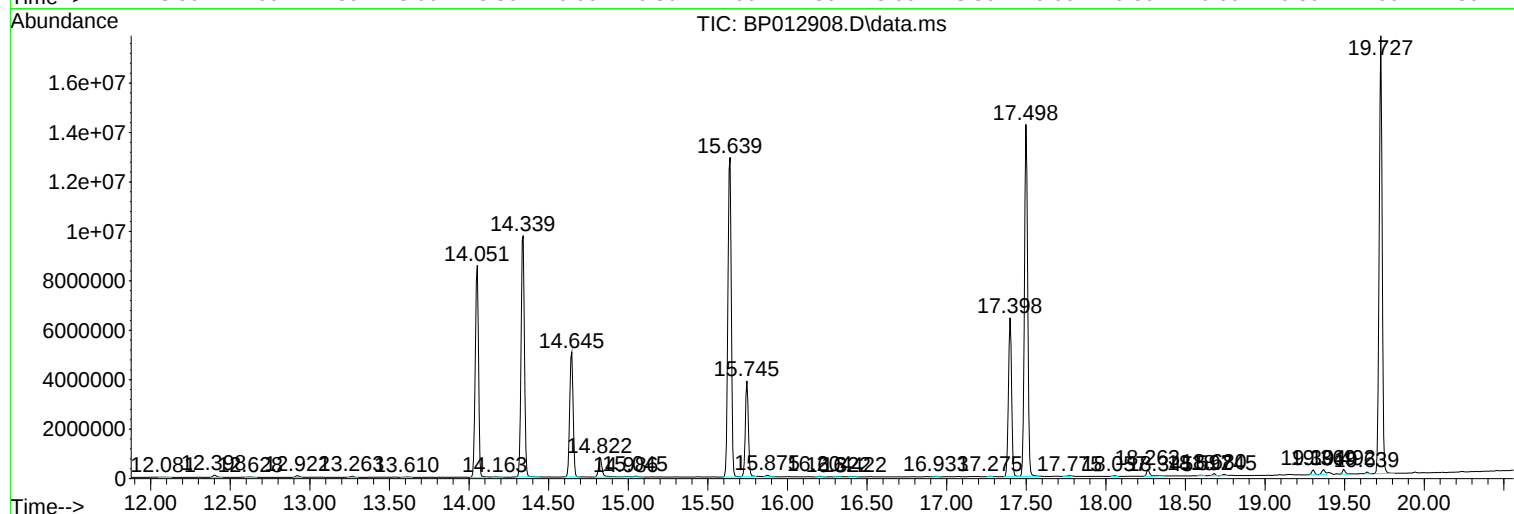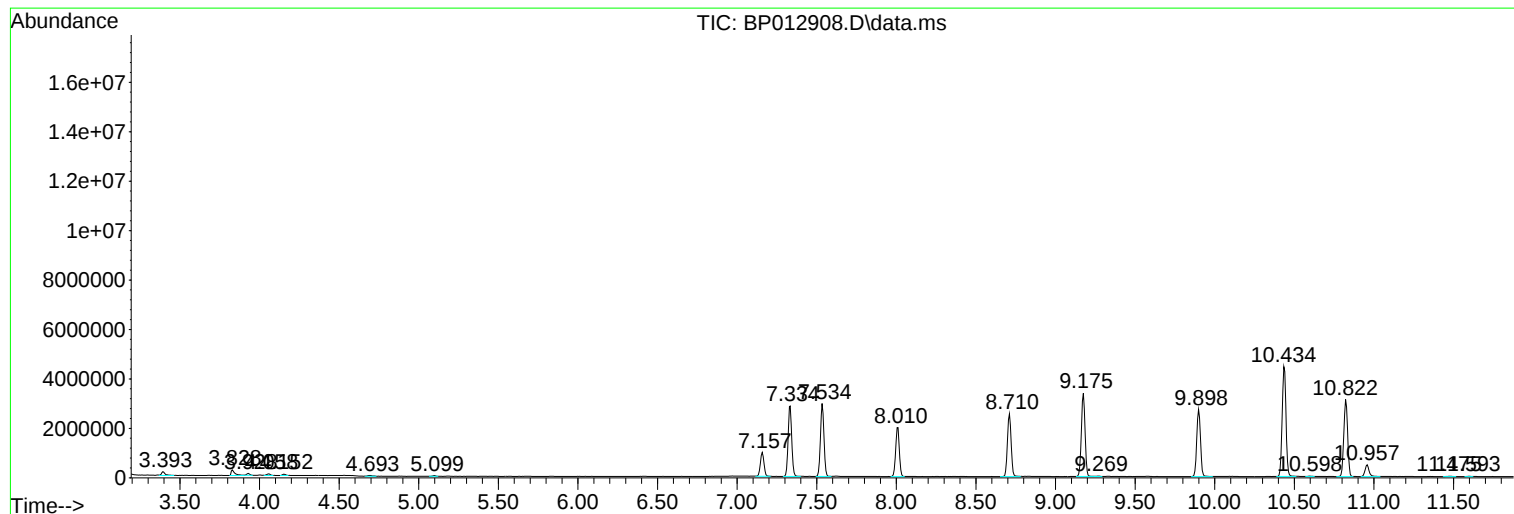

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012908.D
Acq On : 01 Dec 2022 08:36
Operator : CG/JU
Sample : N5770-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012908.D
Acq On : 01 Dec 2022 08:36
Operator : CG/JU
Sample : N5770-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
