

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012909.D
 Acq On : 01 Dec 2022 09:10
 Operator : CG/JU
 Sample : N5770-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	41	rVB	118517	148994	0.97%	0.111%
2	3.822	104	108	123	rBV	573218	944611	6.16%	0.706%
3	4.058	143	148	153	rVB	55135	88095	0.57%	0.066%
4	4.152	161	164	168	rVB	44012	54264	0.35%	0.041%
5	4.693	251	256	263	rVB	71436	109435	0.71%	0.082%
6	5.834	445	450	454	rVB	18785	28900	0.19%	0.022%
7	7.157	669	675	687	rVB	449016	732099	4.77%	0.547%
8	7.328	696	704	718	rBV	1628620	2602048	16.96%	1.945%
9	7.451	721	725	730	rBV4	9404	17169	0.11%	0.013%
10	7.534	732	739	749	rBV	1504662	2333139	15.21%	1.744%
11	7.622	751	754	760	rVB5	14120	19198	0.13%	0.014%
12	8.004	811	819	826	rBV	1954493	3108000	20.26%	2.323%
13	8.069	826	830	835	rVB6	10300	16708	0.11%	0.012%
14	8.710	930	939	949	rBV	1330738	2147713	14.00%	1.605%
15	9.175	1010	1018	1029	rBV	1814530	3001437	19.57%	2.243%
16	9.269	1029	1034	1038	rVB4	16003	27989	0.18%	0.021%
17	9.898	1134	1141	1152	rBV	1406257	2243454	14.63%	1.677%
18	10.434	1225	1232	1244	rBV	2367132	3857041	25.15%	2.883%
19	10.598	1257	1260	1267	rVB4	13850	23181	0.15%	0.017%
20	10.822	1290	1298	1310	rVB	3092590	5094303	33.21%	3.807%
21	10.957	1313	1321	1336	rBV	1286283	2247660	14.65%	1.680%
22	11.598	1425	1430	1433	rBV6	13479	22299	0.15%	0.017%
23	12.081	1509	1512	1518	rVB5	11158	17491	0.11%	0.013%
24	12.404	1561	1567	1574	rBV2	50199	88384	0.58%	0.066%
25	12.922	1647	1655	1665	rVB	162784	263968	1.72%	0.197%
26	13.269	1708	1714	1719	rBV	50863	72888	0.48%	0.054%
27	13.533	1754	1759	1766	rVV2	31367	48240	0.31%	0.036%
28	13.616	1767	1773	1776	rVB5	9447	17346	0.11%	0.013%
29	13.933	1824	1827	1838	rVB5	7725	19259	0.13%	0.014%
30	14.045	1839	1846	1859	rBV	4988411	6910196	45.05%	5.164%
31	14.169	1862	1867	1872	rVB8	16974	27480	0.18%	0.021%
32	14.339	1889	1896	1906	rBV	5560005	8119054	52.93%	6.068%
33	14.598	1932	1940	1941	rBV5	9445	15560	0.10%	0.012%
34	14.645	1941	1948	1956	rVV	5085499	7631650	49.76%	5.704%
35	14.822	1972	1978	1989	rBV	229025	421450	2.75%	0.315%
36	15.051	2013	2017	2022	rVB7	17408	28039	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012909.D
 Acq On : 01 Dec 2022 09:10
 Operator : CG/JU
 Sample : N5770-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.633	2109	2116	2129	rBV	7908947	11144103	72.65%	8.329%
38	15.745	2129	2135	2151	rVV	1520975	2058824	13.42%	1.539%
39	15.875	2151	2157	2162	rVB2	30827	62887	0.41%	0.047%
40	16.204	2206	2213	2218	rBV3	38537	65956	0.43%	0.049%
41	16.404	2245	2247	2255	rVB5	12727	25698	0.17%	0.019%
42	16.869	2321	2326	2331	rBV7	14971	25605	0.17%	0.019%
43	17.151	2370	2374	2376	rBV5	12759	16517	0.11%	0.012%
44	17.186	2376	2380	2385	rVB2	17721	23171	0.15%	0.017%
45	17.398	2409	2416	2426	rBV	6733263	9336590	60.87%	6.978%
46	17.498	2426	2433	2446	rVV	8779183	12598149	82.13%	9.415%
47	17.774	2474	2480	2489	rBV9	38231	90634	0.59%	0.068%
48	18.057	2525	2528	2533	rVB7	19609	27150	0.18%	0.020%
49	18.263	2559	2563	2568	rBV	113561	140296	0.91%	0.105%
50	18.680	2630	2634	2638	rBV	224473	243844	1.59%	0.182%
51	18.739	2642	2644	2647	rVV3	15785	15755	0.10%	0.012%
52	19.098	2701	2705	2708	rBV6	37726	56080	0.37%	0.042%
53	19.304	2736	2740	2744	rBV2	120634	149459	0.97%	0.112%
54	19.368	2746	2751	2755	rBV	122640	190720	1.24%	0.143%
55	19.492	2769	2772	2780	rBV2	83232	111190	0.72%	0.083%
56	19.645	2795	2798	2804	rVB2	55917	65357	0.43%	0.049%
57	19.727	2805	2812	2822	rBV	11371177	15338403	100.00%	11.463%
58	21.480	3105	3110	3119	rBV	6865370	9442846	61.56%	7.057%
59	23.827	3502	3509	3527	rBV2	5569050	12013699	78.32%	8.979%
60	23.992	3530	3537	3550	rVB2	3730369	8013171	52.24%	5.989%




Sum of corrected areas: 133804846

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012909.D
Acq On : 01 Dec 2022 09:10
Operator : CG/JU
Sample : N5770-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

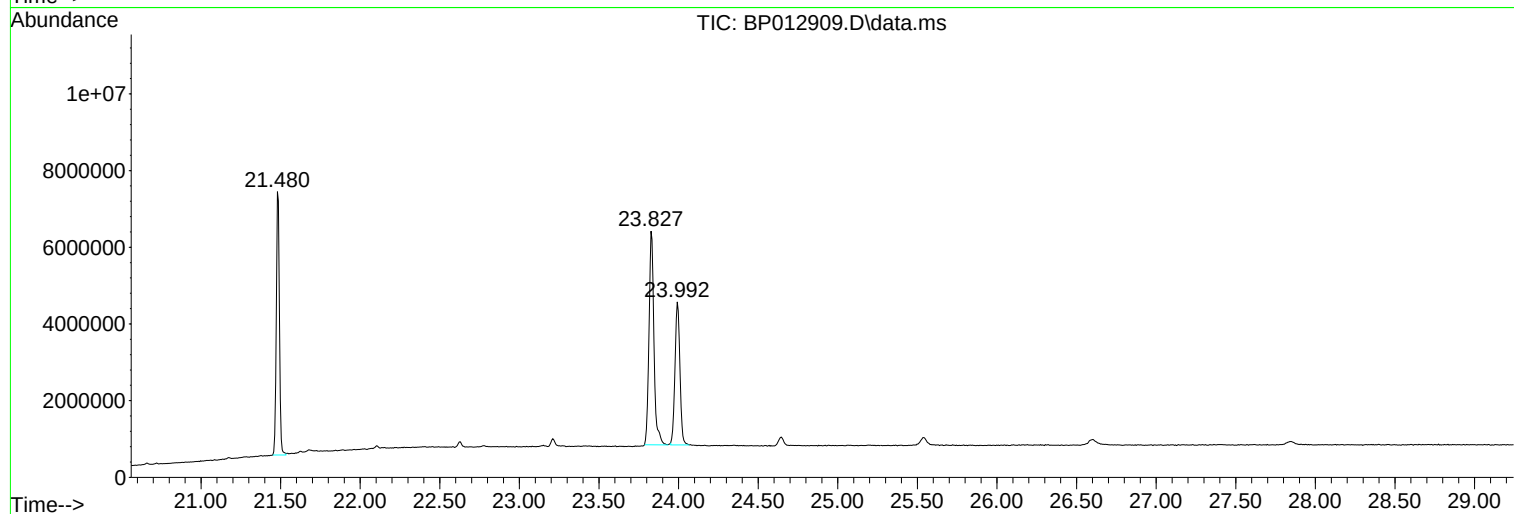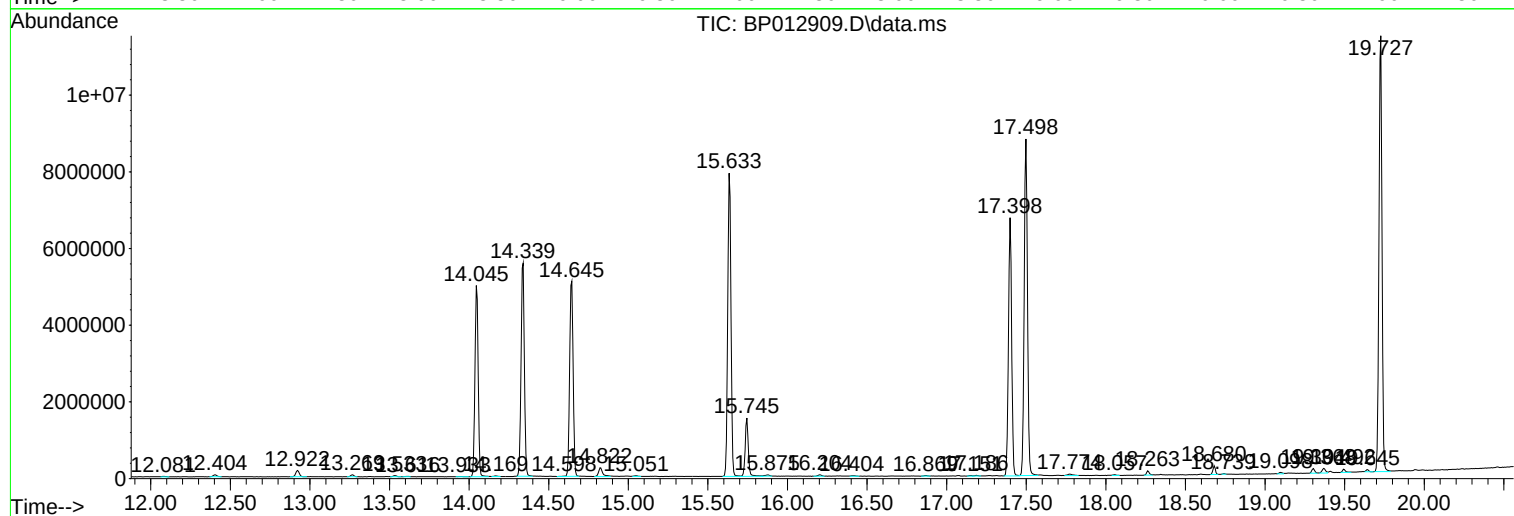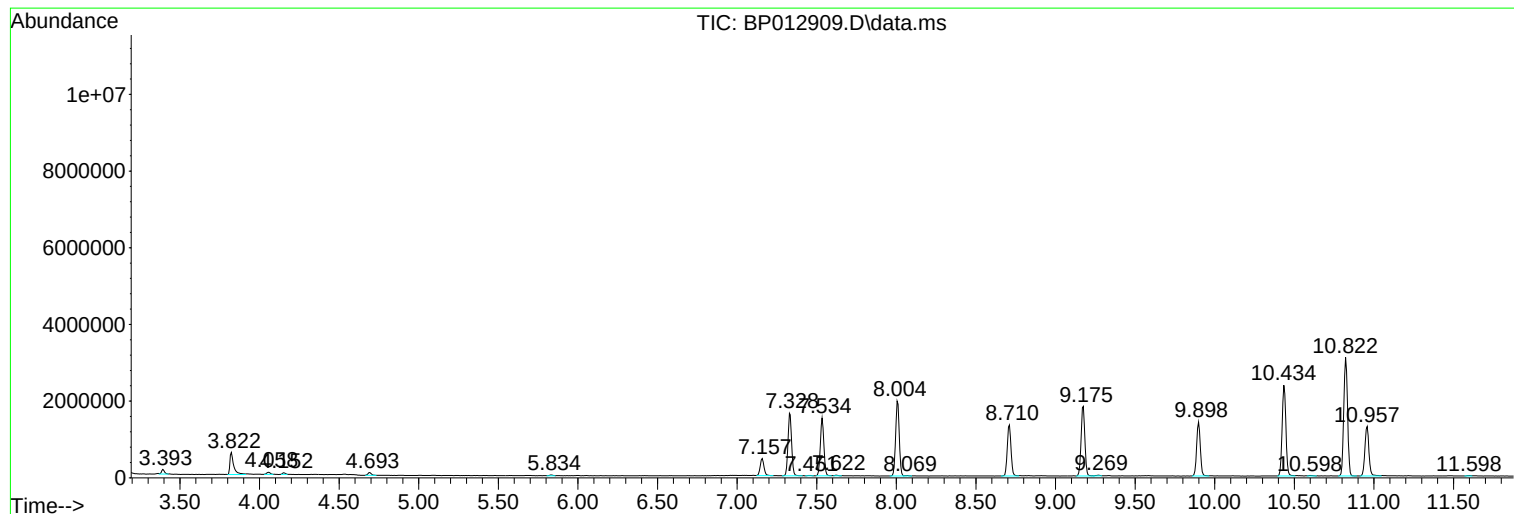

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012909.D
Acq On : 01 Dec 2022 09:10
Operator : CG/JU
Sample : N5770-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012909.D
Acq On : 01 Dec 2022 09:10
Operator : CG/JU
Sample : N5770-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
