

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012910.D
 Acq On : 01 Dec 2022 09:44
 Operator : CG/JU
 Sample : N5770-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	39	rVB	131500	155219	0.77%	0.088%
2	3.822	105	108	123	rBV	449665	697621	3.46%	0.395%
3	4.052	143	147	156	rVB	67730	114342	0.57%	0.065%
4	4.152	160	164	169	rVB	50124	67224	0.33%	0.038%
5	4.693	252	256	261	rVB5	23130	30725	0.15%	0.017%
6	7.158	668	675	689	rVB	828574	1308396	6.48%	0.741%
7	7.328	698	704	717	rBV	2552204	4067644	20.15%	2.303%
8	7.534	732	739	749	rBV	2515030	3921560	19.43%	2.220%
9	7.622	750	754	759	rVB6	18322	29884	0.15%	0.017%
10	8.005	812	819	827	rBV	2084466	3368799	16.69%	1.907%
11	8.710	932	939	955	rBV	2270416	3669149	18.18%	2.077%
12	9.175	1010	1018	1030	rBV	2976904	4820454	23.88%	2.729%
13	9.587	1083	1088	1094	rVB3	29384	47189	0.23%	0.027%
14	9.899	1133	1141	1151	rBV	2373338	3833907	18.99%	2.171%
15	10.434	1222	1232	1246	rBV	3698675	6236259	30.89%	3.531%
16	10.604	1255	1261	1266	rBV5	43207	73105	0.36%	0.041%
17	10.822	1290	1298	1306	rBV	3298160	5481757	27.16%	3.104%
18	10.957	1314	1321	1336	rBV	945810	1618791	8.02%	0.917%
19	11.593	1424	1429	1433	rBV7	14007	25004	0.12%	0.014%
20	12.081	1500	1512	1516	rBV7	16685	38076	0.19%	0.022%
21	12.234	1532	1538	1543	rBV4	15343	24524	0.12%	0.014%
22	12.404	1561	1567	1573	rBV3	79608	146096	0.72%	0.083%
23	13.263	1707	1713	1721	rVB	46061	75033	0.37%	0.042%
24	13.463	1743	1747	1754	rVB2	27283	35862	0.18%	0.020%
25	13.534	1754	1759	1765	rVB4	20098	34513	0.17%	0.020%
26	13.610	1765	1772	1776	rBV5	17160	35641	0.18%	0.020%
27	14.051	1839	1847	1862	rBV	7142658	10222109	50.64%	5.788%
28	14.163	1862	1866	1872	rVB8	21397	39112	0.19%	0.022%
29	14.340	1889	1896	1908	rBV	8443266	12620540	62.52%	7.146%
30	14.645	1938	1948	1956	rBV	5399062	8092955	40.09%	4.582%
31	14.822	1972	1978	1995	rBV	613690	1007761	4.99%	0.571%
32	15.045	2012	2016	2023	rVB7	32912	57675	0.29%	0.033%
33	15.639	2109	2117	2127	rBV	11075305	16234219	80.42%	9.192%
34	15.745	2129	2135	2150	rVV	3167948	4188482	20.75%	2.372%
35	15.875	2152	2157	2164	rVB	52494	92733	0.46%	0.053%
36	15.998	2174	2178	2183	rBV	61118	79889	0.40%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012910.D
 Acq On : 01 Dec 2022 09:44
 Operator : CG/JU
 Sample : N5770-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	16.422	2244	2250	2260	rVB	14883	33363	0.17%	0.019%
38	16.875	2321	2327	2330	rBV7	17664	34614	0.17%	0.020%
39	17.181	2375	2379	2387	rVB3	17755	32757	0.16%	0.019%
40	17.398	2409	2416	2426	rBV	7061665	9761576	48.36%	5.527%
41	17.498	2426	2433	2443	rVV	12214375	17467193	86.53%	9.890%
42	17.581	2444	2447	2454	rVB2	72845	103370	0.51%	0.059%
43	17.769	2476	2479	2487	rVB4	29088	50958	0.25%	0.029%
44	18.057	2522	2528	2531	rBV8	21632	33073	0.16%	0.019%
45	18.263	2558	2563	2570	rBV	391664	525001	2.60%	0.297%
46	18.680	2630	2634	2640	rBV	225745	260611	1.29%	0.148%
47	19.098	2702	2705	2709	rBV5	23818	30705	0.15%	0.017%
48	19.304	2735	2740	2744	rBV	161977	215392	1.07%	0.122%
49	19.369	2746	2751	2756	rVV	168781	259944	1.29%	0.147%
50	19.410	2756	2758	2762	rVB3	35610	38307	0.19%	0.022%
51	19.492	2769	2772	2781	rBV2	206277	286051	1.42%	0.162%
52	19.639	2795	2797	2801	rVB4	58167	66106	0.33%	0.037%
53	19.727	2806	2812	2825	rVV	15452510	20185585	100.00%	11.429%
54	21.174	3054	3058	3064	rBV2	330453	480458	2.38%	0.272%
55	21.480	3105	3110	3118	rBV	7123290	9678655	47.95%	5.480%
56	23.833	3502	3510	3528	rBV	7722242	16164347	80.08%	9.152%
57	23.992	3530	3537	3551	rVB2	3914755	8314207	41.19%	4.708%




Sum of corrected areas: 176614522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012910.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : N5770-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

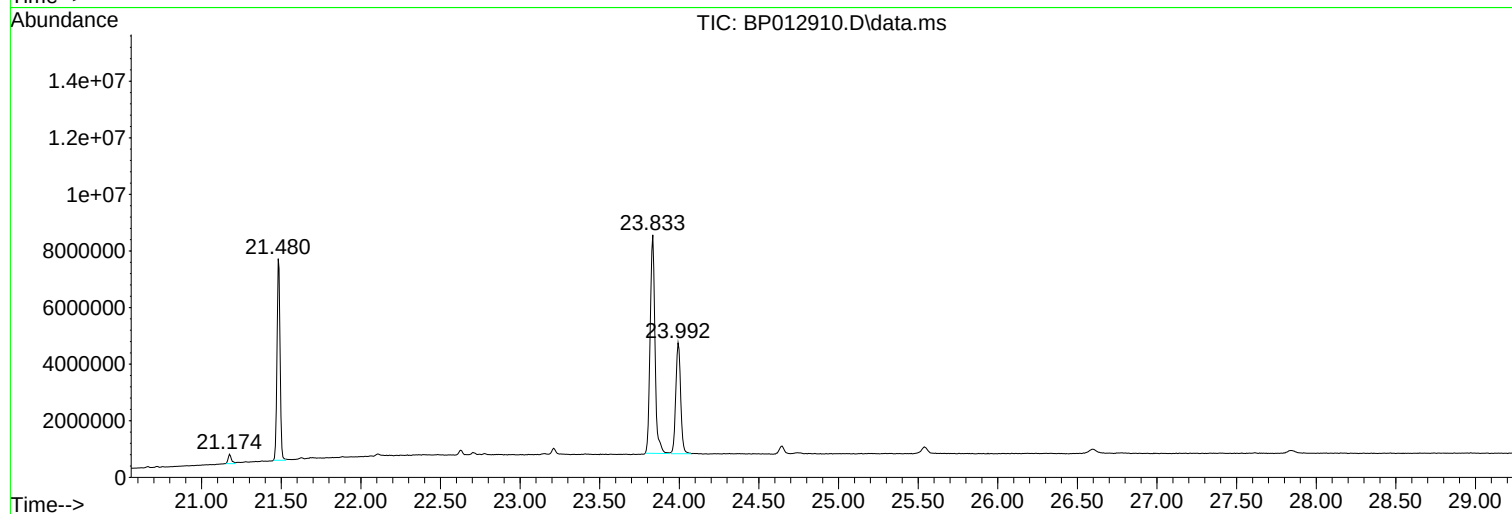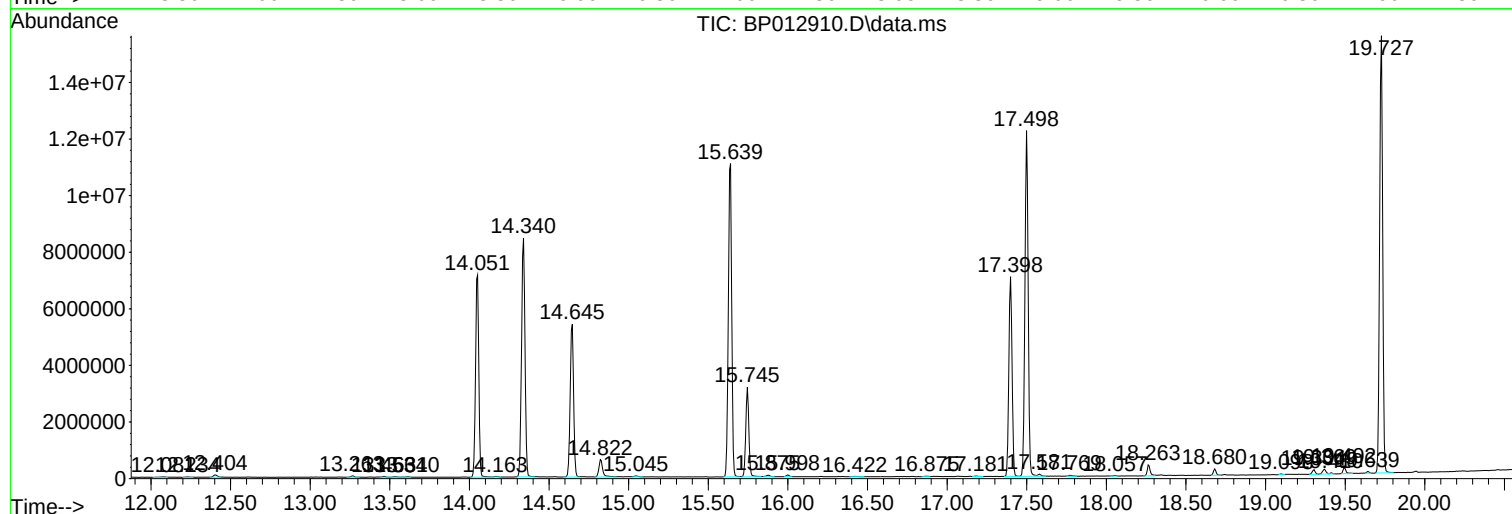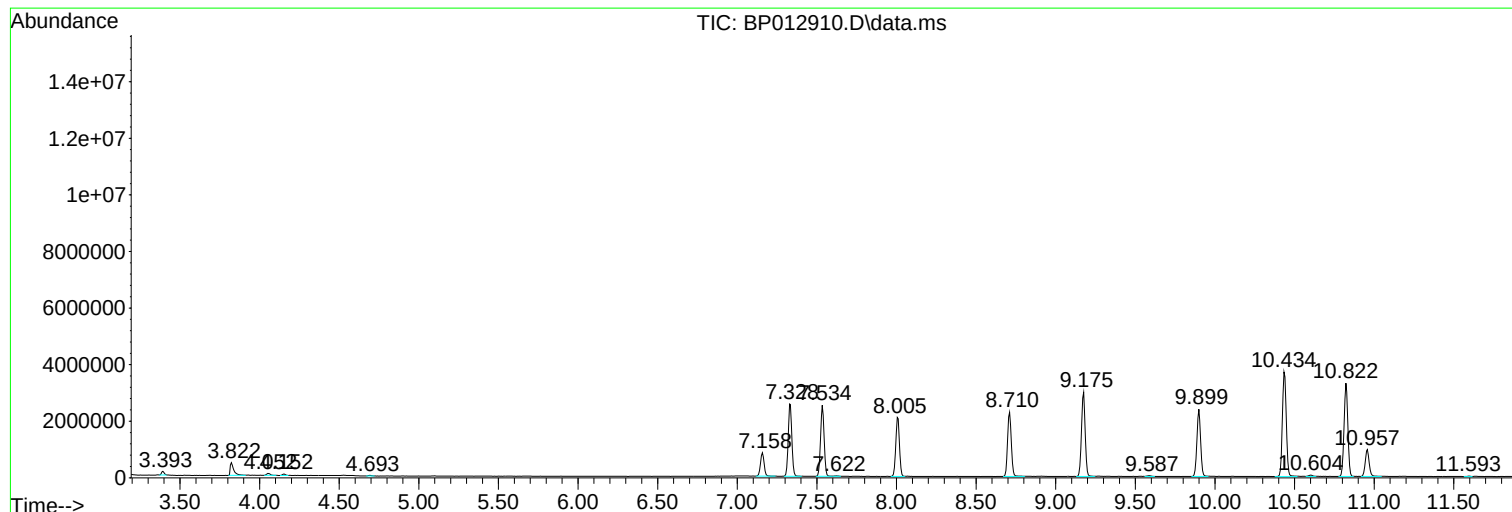

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012910.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : N5770-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012910.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : N5770-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc