

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012911.D
 Acq On : 01 Dec 2022 10:18
 Operator : CG/JU
 Sample : N5770-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	41	rVB	76021	103432	0.54%	0.064%
2	3.828	106	109	122	rBV	220083	377228	1.96%	0.234%
3	4.058	143	148	153	rVB	58332	90340	0.47%	0.056%
4	4.152	160	164	171	rVB	40178	60261	0.31%	0.037%
5	6.969	638	643	648	rBV8	8298	20309	0.11%	0.013%
6	7.158	668	675	685	rVB	676370	1043088	5.43%	0.647%
7	7.328	698	704	714	rBV	2217603	3549269	18.47%	2.202%
8	7.534	732	739	750	rBV	2140730	3354776	17.46%	2.081%
9	7.622	752	754	759	rVB6	15372	20755	0.11%	0.013%
10	8.011	812	820	827	rBV	2014442	3207173	16.69%	1.990%
11	8.710	931	939	950	rBV	1912333	3039463	15.82%	1.885%
12	9.175	1010	1018	1028	rBV	2622317	4233985	22.03%	2.626%
13	9.269	1031	1034	1041	rVB7	17777	33035	0.17%	0.020%
14	9.587	1085	1088	1094	rVB6	12447	20712	0.11%	0.013%
15	9.899	1130	1141	1154	rBV	1849346	2994757	15.58%	1.858%
16	10.434	1225	1232	1245	rBV	3171115	5303749	27.60%	3.290%
17	10.822	1290	1298	1308	rVB	3154536	5271452	27.43%	3.270%
18	10.957	1314	1321	1333	rBV	1139826	1999328	10.40%	1.240%
19	12.087	1507	1513	1518	rVB2	20498	33977	0.18%	0.021%
20	12.404	1559	1567	1575	rBV	63540	109489	0.57%	0.068%
21	13.269	1704	1714	1718	rBV	19061	33284	0.17%	0.021%
22	13.610	1766	1772	1780	rVB6	15368	31112	0.16%	0.019%
23	13.963	1826	1832	1837	rVB7	20367	34243	0.18%	0.021%
24	14.046	1839	1846	1858	rBV	6666184	9315117	48.47%	5.778%
25	14.340	1888	1896	1908	rBV	7531809	11513611	59.91%	7.142%
26	14.640	1940	1947	1957	rBV	5318862	7933486	41.28%	4.921%
27	14.822	1971	1978	1992	rBV	320289	569802	2.96%	0.353%
28	15.051	2013	2017	2024	rVB5	48683	79787	0.42%	0.049%
29	15.634	2107	2116	2128	rBV	10432965	14954472	77.81%	9.277%
30	15.745	2128	2135	2143	rBV	954241	1282965	6.68%	0.796%
31	15.875	2153	2157	2163	rVB	45984	67596	0.35%	0.042%
32	16.869	2322	2326	2332	rVB	24708	34138	0.18%	0.021%
33	17.075	2357	2361	2366	rVB8	14887	25980	0.14%	0.016%
34	17.145	2366	2373	2376	rBV9	9117	19944	0.10%	0.012%
35	17.181	2376	2379	2385	rVV3	15093	25302	0.13%	0.016%
36	17.398	2409	2416	2426	rBV	6957629	9717241	50.56%	6.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012911.D
 Acq On : 01 Dec 2022 10:18
 Operator : CG/JU
 Sample : N5770-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.498	2426	2433	2444	rVV	11709712	16366548	85.16%	10.153%
38	17.581	2444	2447	2452	rVB5	47934	70239	0.37%	0.044%
39	17.775	2475	2480	2483	rBV6	12732	19283	0.10%	0.012%
40	18.263	2560	2563	2568	rBV5	26509	31512	0.16%	0.020%
41	19.304	2735	2740	2744	rBV	146099	186295	0.97%	0.116%
42	19.369	2746	2751	2756	rBV	137320	192409	1.00%	0.119%
43	19.639	2795	2797	2802	rVB3	38462	45820	0.24%	0.028%
44	19.728	2806	2812	2825	rVV	14412379	19218458	100.00%	11.922%
45	19.945	2846	2849	2852	rBV2	31853	38335	0.20%	0.024%
46	21.480	3105	3110	3122	rBV	7342118	10092946	52.52%	6.261%
47	23.833	3502	3510	3525	rBV2	7646454	15703644	81.71%	9.741%
48	23.992	3530	3537	3553	rVB2	4087837	8734144	45.45%	5.418%




Sum of corrected areas: 161204291

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012911.D
Acq On : 01 Dec 2022 10:18
Operator : CG/JU
Sample : N5770-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

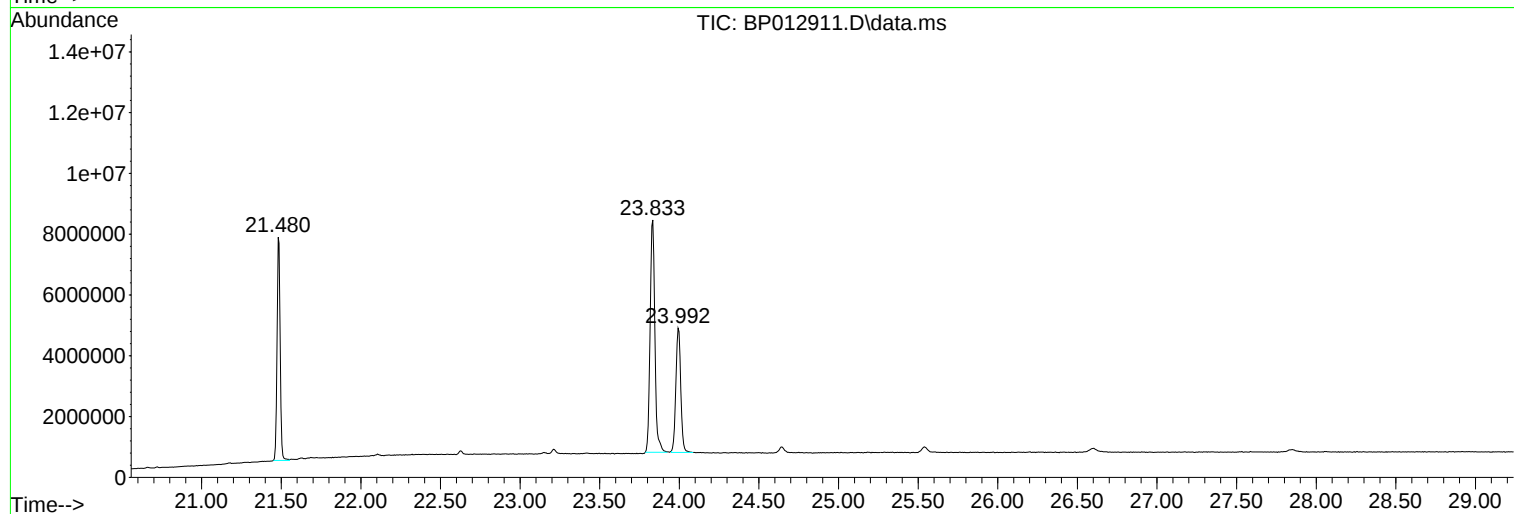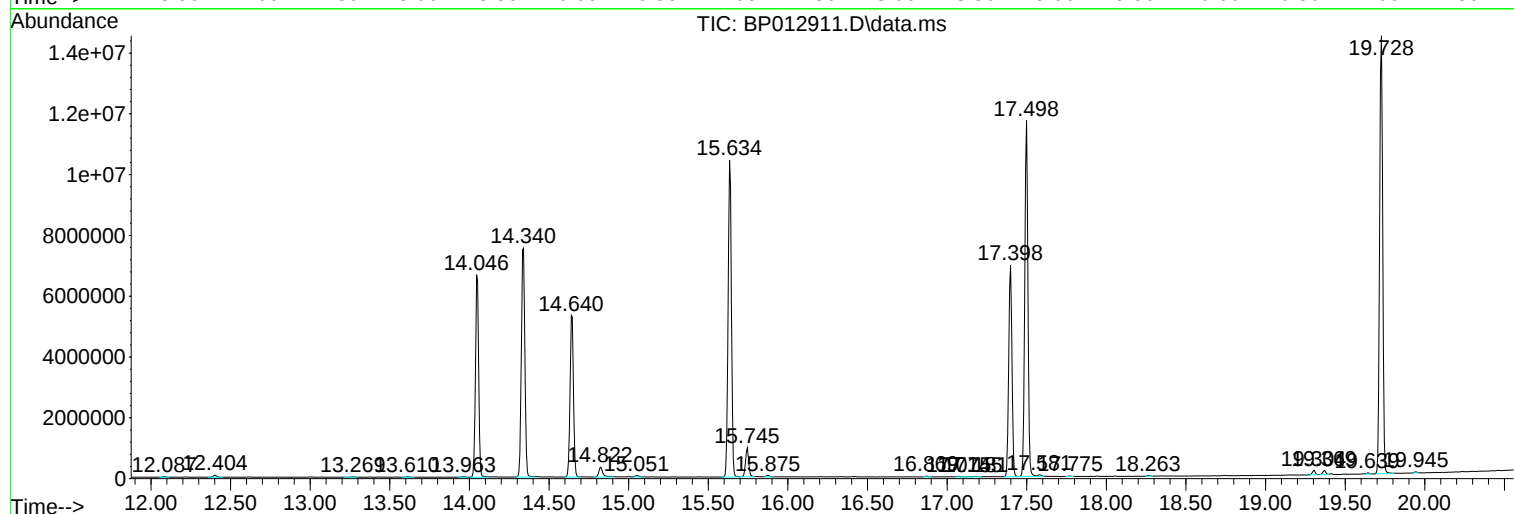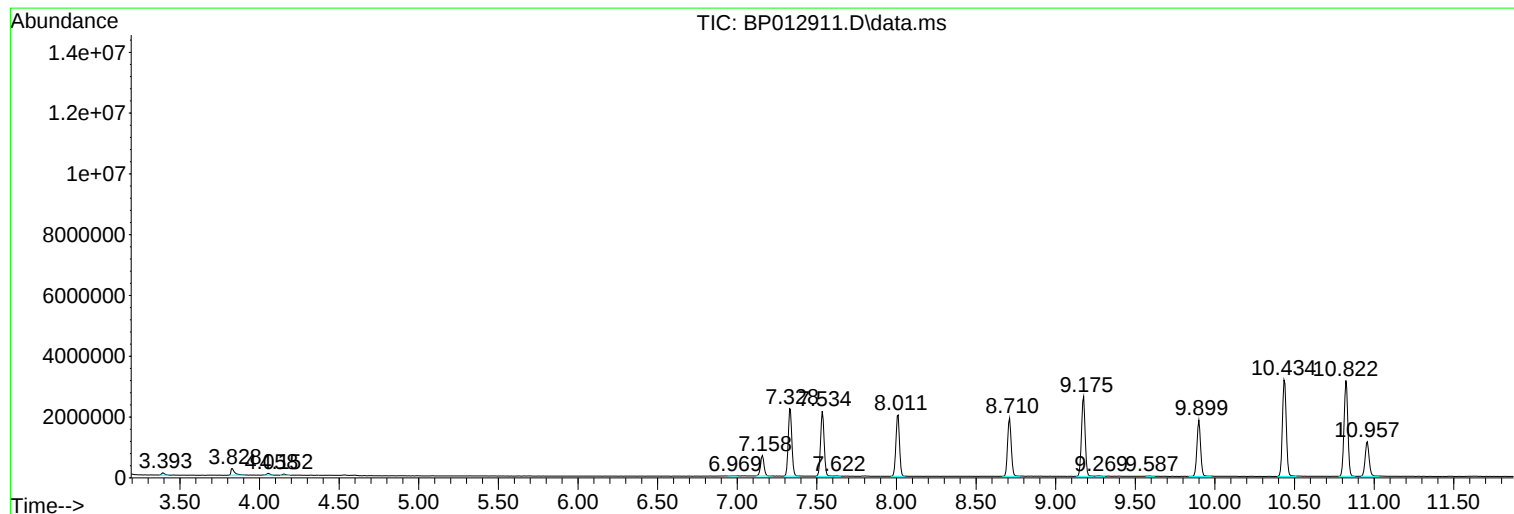

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012911.D
Acq On : 01 Dec 2022 10:18
Operator : CG/JU
Sample : N5770-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012911.D
Acq On : 01 Dec 2022 10:18
Operator : CG/JU
Sample : N5770-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1M9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc