

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012912.D
 Acq On : 01 Dec 2022 10:52
 Operator : CG/JU
 Sample : N5770-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	44	rVB	87702	119175	0.85%	0.089%
2	3.828	106	109	123	rBV	263714	438022	3.11%	0.327%
3	4.058	143	148	152	rBV	65950	93667	0.67%	0.070%
4	4.152	160	164	172	rVB	38239	53109	0.38%	0.040%
5	4.534	225	229	232	rBV5	15209	25177	0.18%	0.019%
6	7.157	668	675	685	rVB	731470	1111405	7.89%	0.831%
7	7.334	698	705	713	rBV	2292714	3600383	25.57%	2.691%
8	7.534	733	739	750	rBV	2171338	3372219	23.95%	2.520%
9	7.628	750	755	763	rVB6	15232	29268	0.21%	0.022%
10	8.010	811	820	827	rBV	2064393	3295062	23.41%	2.463%
11	8.710	931	939	953	rBV	1967662	3148430	22.36%	2.353%
12	9.175	1010	1018	1030	rBV	2578724	4176604	29.67%	3.122%
13	9.899	1133	1141	1151	rBV	1520738	2428022	17.25%	1.815%
14	10.434	1224	1232	1249	rBV	2992955	5105204	36.26%	3.816%
15	10.822	1289	1298	1311	rVB	3152180	5291673	37.59%	3.955%
16	10.957	1313	1321	1335	rBV	1283644	2178356	15.47%	1.628%
17	11.628	1431	1435	1440	rVB7	10317	16272	0.12%	0.012%
18	12.081	1509	1512	1518	rVB8	8365	14694	0.10%	0.011%
19	12.404	1560	1567	1573	rBV2	77976	154917	1.10%	0.116%
20	13.269	1709	1714	1718	rVB3	19421	28750	0.20%	0.021%
21	13.375	1727	1732	1736	rBV6	7351	15228	0.11%	0.011%
22	13.534	1753	1759	1763	rBV9	9983	14751	0.10%	0.011%
23	13.610	1767	1772	1777	rVB4	14063	27092	0.19%	0.020%
24	13.963	1827	1832	1839	rVB7	20788	31190	0.22%	0.023%
25	14.045	1839	1846	1858	rBV	6309297	8709491	61.87%	6.509%
26	14.339	1889	1896	1912	rBV	7151768	10669798	75.79%	7.974%
27	14.645	1939	1948	1957	rBV	5113943	7543547	53.58%	5.638%
28	14.822	1973	1978	1993	rBV	185246	371301	2.64%	0.278%
29	15.051	2013	2017	2022	rVB7	33462	52739	0.37%	0.039%
30	15.639	2109	2117	2128	rBV	9186659	13681278	97.18%	10.225%
31	15.745	2129	2135	2141	rVV	237066	355081	2.52%	0.265%
32	15.875	2153	2157	2162	rVB3	37478	55353	0.39%	0.041%
33	17.069	2358	2360	2365	rVB6	12190	16351	0.12%	0.012%
34	17.180	2375	2379	2383	rBV4	9553	14528	0.10%	0.011%
35	17.398	2409	2416	2426	rBV	5898729	8291002	58.89%	6.197%
36	17.498	2426	2433	2444	rVV	10054153	14077811	100.00%	10.522%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012912.D
 Acq On : 01 Dec 2022 10:52
 Operator : CG/JU
 Sample : N5770-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1N1

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.580	2444	2447	2459	rVB5	53935	98706	0.70%	0.074%
38	17.775	2476	2480	2482	rBV4	9375	14771	0.10%	0.011%
39	18.263	2559	2563	2569	rBV3	96531	129636	0.92%	0.097%
40	19.304	2735	2740	2745	rBV	109625	165886	1.18%	0.124%
41	19.369	2747	2751	2755	rVB	97299	138024	0.98%	0.103%
42	19.492	2769	2772	2775	rBV4	56809	66767	0.47%	0.050%
43	19.645	2795	2798	2804	rVB7	26875	33049	0.23%	0.025%
44	19.722	2806	2811	2823	rVV	10188139	13851421	98.39%	10.352%
45	21.480	3105	3110	3120	rBV	4268625	5689298	40.41%	4.252%
46	23.827	3502	3509	3523	rBV	4797478	9636797	68.45%	7.202%
47	23.992	3530	3537	3549	rVB	2589359	5368435	38.13%	4.012%




Sum of corrected areas: 133799740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012912.D
Acq On : 01 Dec 2022 10:52
Operator : CG/JU
Sample : N5770-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

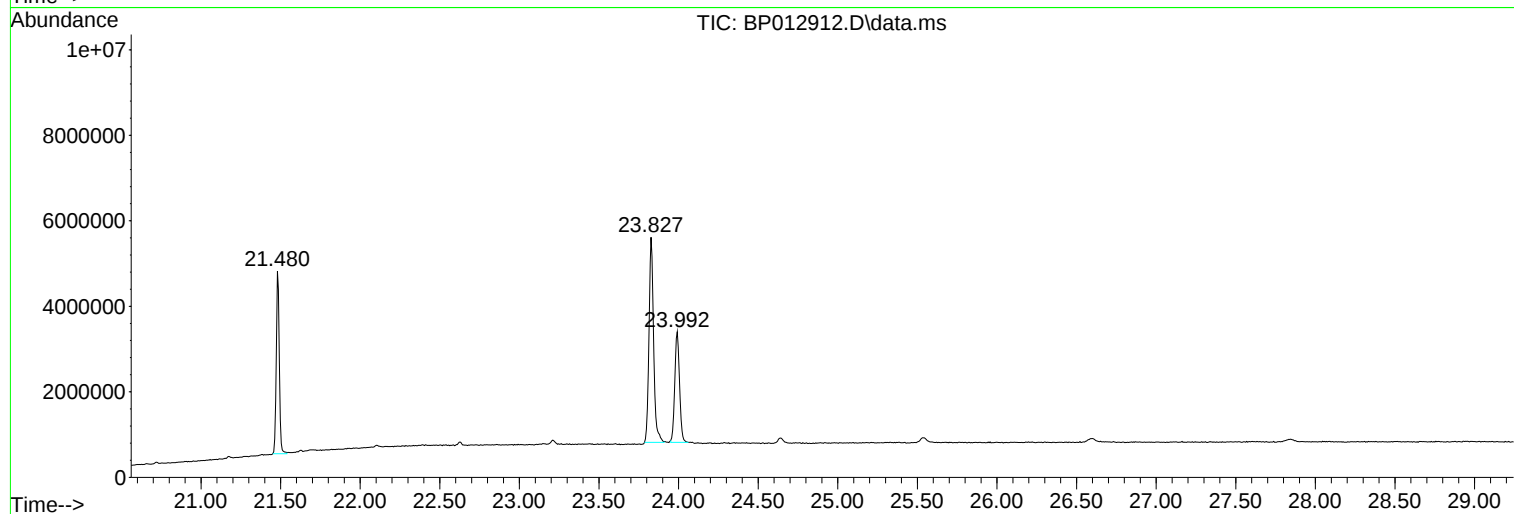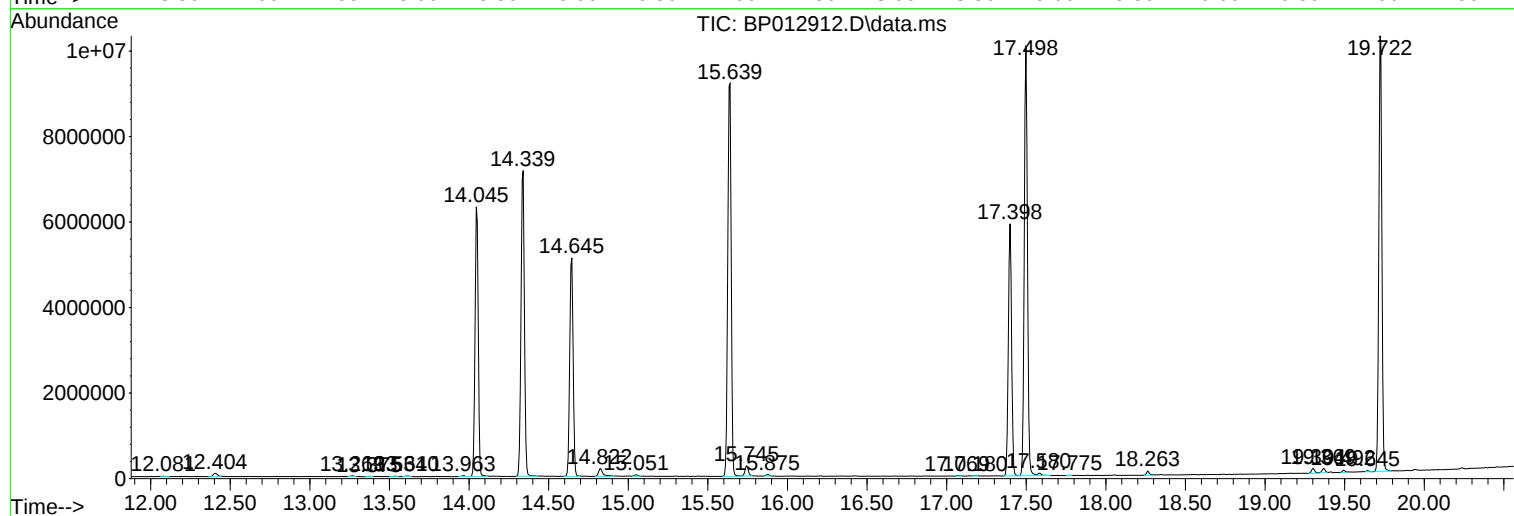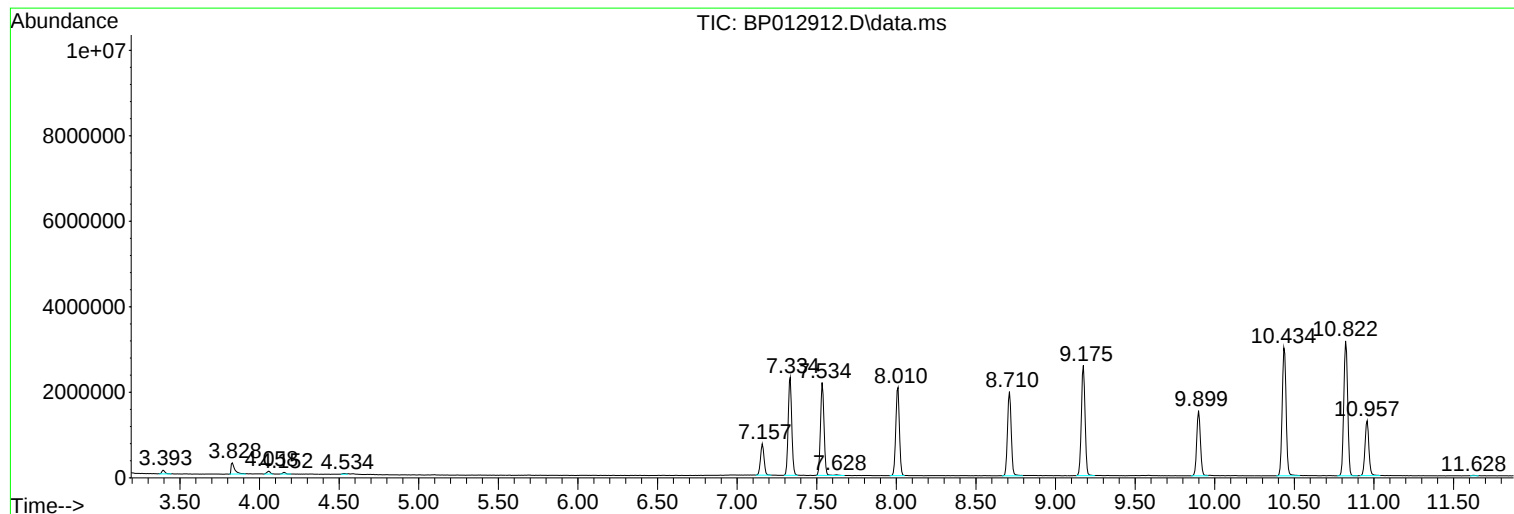

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012912.D
Acq On : 01 Dec 2022 10:52
Operator : CG/JU
Sample : N5770-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012912.D
Acq On : 01 Dec 2022 10:52
Operator : CG/JU
Sample : N5770-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
