

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012915.D
 Acq On : 01 Dec 2022 13:09
 Operator : CG/JU
 Sample : N5737-01DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4345DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	49	rVB	346646	442915	6.75%	0.842%
2	3.828	107	109	122	rBV	110646	181275	2.76%	0.344%
3	3.999	135	138	144	rBV4	12467	20909	0.32%	0.040%
4	4.152	160	164	171	rVB	37489	49904	0.76%	0.095%
5	4.599	236	240	250	rVB3	51239	89420	1.36%	0.170%
6	4.946	295	299	302	rVB5	6682	10092	0.15%	0.019%
7	5.299	352	359	367	rVB	43197	69665	1.06%	0.132%
8	5.428	376	381	387	rVB2	23679	38804	0.59%	0.074%
9	6.270	520	524	532	rVB	21807	35962	0.55%	0.068%
10	6.487	556	561	563	rBV6	8322	10792	0.16%	0.021%
11	6.658	588	590	596	rVB7	7399	10390	0.16%	0.020%
12	6.969	638	643	645	rBV5	6416	10611	0.16%	0.020%
13	7.158	670	675	681	rVB	77778	119648	1.82%	0.227%
14	7.328	698	704	711	rBV	355767	561159	8.55%	1.066%
15	7.534	733	739	747	rBV	296701	485994	7.41%	0.923%
16	7.605	747	751	756	rVB6	7558	13211	0.20%	0.025%
17	7.793	778	783	790	rBV2	54226	85115	1.30%	0.162%
18	8.005	812	819	828	rBV	1944234	3118989	47.55%	5.927%
19	8.081	828	832	845	rVB2	38907	78780	1.20%	0.150%
20	8.240	856	859	863	rBV6	5478	9675	0.15%	0.018%
21	8.364	873	880	886	rBV4	17461	36120	0.55%	0.069%
22	8.434	888	892	898	rVB8	8526	13829	0.21%	0.026%
23	8.552	911	912	917	rVB5	6091	8771	0.13%	0.017%
24	8.652	926	929	933	rVV6	6685	9382	0.14%	0.018%
25	8.711	933	939	949	rVB	239780	381988	5.82%	0.726%
26	8.811	952	956	961	rBV	50116	73836	1.13%	0.140%
27	8.999	982	988	996	rBV	107413	179233	2.73%	0.341%
28	9.116	1002	1008	1012	rBV3	15347	26147	0.40%	0.050%
29	9.175	1012	1018	1027	rVB	348204	586192	8.94%	1.114%
30	9.387	1049	1054	1056	rBV6	7709	11585	0.18%	0.022%
31	9.505	1070	1074	1077	rBV5	13361	17327	0.26%	0.033%
32	9.593	1083	1089	1098	rVB4	27218	53619	0.82%	0.102%
33	9.899	1133	1141	1149	rBV	253073	411088	6.27%	0.781%
34	10.058	1162	1168	1169	rBV6	5177	8980	0.14%	0.017%
35	10.434	1226	1232	1242	rBV	442260	768318	11.71%	1.460%
36	10.681	1269	1274	1276	rBV6	6878	9773	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012915.D
 Acq On : 01 Dec 2022 13:09
 Operator : CG/JU
 Sample : N5737-01DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4345DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	10.822	1290	1298	1307	rVB	2945538	4843353	73.84%	9.203%
38	10.958	1312	1321	1332	rBV	348805	626220	9.55%	1.190%
39	11.293	1374	1378	1384	rVB7	13463	26185	0.40%	0.050%
40	11.357	1384	1389	1391	rBV6	8181	11971	0.18%	0.023%
41	11.405	1391	1397	1399	rBV6	7711	12279	0.19%	0.023%
42	11.646	1434	1438	1442	rVB7	9579	15413	0.23%	0.029%
43	11.828	1465	1469	1471	rVB5	7411	9192	0.14%	0.017%
44	12.010	1495	1500	1503	rBV5	8912	17375	0.26%	0.033%
45	12.052	1503	1507	1513	rVV7	16133	43362	0.66%	0.082%
46	12.152	1514	1524	1536	rVB	283046	470703	7.18%	0.894%
47	12.246	1536	1540	1544	rBV3	35085	52947	0.81%	0.101%
48	12.304	1544	1550	1557	rVV5	40749	113317	1.73%	0.215%
49	12.416	1563	1569	1580	rVV	83571	161232	2.46%	0.306%
50	12.510	1580	1585	1587	rVV6	7759	12843	0.20%	0.024%
51	12.799	1627	1634	1642	rBV6	25450	54622	0.83%	0.104%
52	12.899	1649	1651	1656	rVB6	6427	9129	0.14%	0.017%
53	13.022	1663	1672	1677	rBV6	9296	26326	0.40%	0.050%
54	13.193	1696	1701	1702	rBV5	7944	10693	0.16%	0.020%
55	13.275	1710	1715	1728	rBV	268093	378300	5.77%	0.719%
56	13.375	1728	1732	1736	rVB7	9653	16828	0.26%	0.032%
57	13.475	1743	1749	1753	rBV8	7746	16548	0.25%	0.031%
58	13.528	1755	1758	1762	rVB6	8928	13206	0.20%	0.025%
59	13.693	1781	1786	1791	rBV4	16621	27521	0.42%	0.052%
60	13.899	1816	1821	1823	rBV6	6601	11135	0.17%	0.021%
61	13.946	1823	1829	1838	rVB4	16170	38191	0.58%	0.073%
62	14.046	1839	1846	1857	rBV	978740	1329629	20.27%	2.526%
63	14.193	1868	1871	1874	rVV4	12260	16449	0.25%	0.031%
64	14.228	1874	1877	1882	rVB6	9268	12443	0.19%	0.024%
65	14.334	1889	1895	1902	rBV	1011657	1468806	22.39%	2.791%
66	14.422	1905	1910	1915	rVB	51752	82008	1.25%	0.156%
67	14.563	1931	1934	1939	rVB7	23308	30085	0.46%	0.057%
68	14.640	1941	1947	1956	rBV	4465265	6490948	98.96%	12.334%
69	14.828	1975	1979	1987	rVB4	20870	36543	0.56%	0.069%
70	15.175	2034	2038	2043	rVB8	11848	21314	0.32%	0.040%
71	15.287	2055	2057	2062	rVB6	9360	13687	0.21%	0.026%
72	15.375	2068	2072	2077	rBV	50437	74078	1.13%	0.141%
73	15.534	2094	2099	2101	rBV6	6842	10737	0.16%	0.020%
74	15.634	2109	2116	2128	rBV2	1465734	2180264	33.24%	4.143%
75	15.740	2129	2134	2145	rVB	155875	253364	3.86%	0.481%
76	15.845	2149	2152	2155	rBV2	13643	16851	0.26%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
 Data File : BP012915.D
 Acq On : 01 Dec 2022 13:09
 Operator : CG/JU
 Sample : N5737-01DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4345DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

77	15.998	2172	2178	2184	rBV	268973	390151	5.95%	0.741%
78	16.045	2184	2186	2194	rVV4	29354	39237	0.60%	0.075%
79	16.140	2198	2202	2211	rVB	148305	212862	3.25%	0.404%
80	16.310	2226	2231	2239	rBV	147507	249767	3.81%	0.475%
81	16.469	2254	2258	2261	rBV3	16027	22332	0.34%	0.042%
82	16.528	2264	2268	2271	rVV6	10756	18252	0.28%	0.035%
83	16.563	2271	2274	2282	rVB8	17205	36644	0.56%	0.070%
84	16.651	2284	2289	2293	rBV	83787	126345	1.93%	0.240%
85	16.687	2293	2295	2300	rVB5	18939	26521	0.40%	0.050%
86	16.781	2309	2311	2317	rVB6	7764	11841	0.18%	0.022%
87	16.863	2320	2325	2332	rBV2	32425	67804	1.03%	0.129%
88	17.187	2375	2380	2386	rVB3	56960	85715	1.31%	0.163%
89	17.398	2409	2416	2426	rBV	4477250	6559477	100.00%	12.464%
90	17.492	2427	2432	2445	rVB	1259091	1817712	27.71%	3.454%
91	17.904	2499	2502	2507	rBV	37117	55184	0.84%	0.105%
92	18.081	2529	2532	2537	rVB2	22581	27803	0.42%	0.053%
93	18.263	2559	2563	2568	rBV4	53763	70655	1.08%	0.134%
94	18.469	2595	2598	2602	rVB2	22136	21139	0.32%	0.040%
95	19.434	2760	2762	2768	rBV4	37534	42326	0.65%	0.080%
96	19.722	2806	2811	2815	rBV	1538366	1966051	29.97%	3.736%
97	19.757	2815	2817	2827	rVB	261117	303924	4.63%	0.577%
98	21.480	3105	3110	3117	rBV	4464762	5858398	89.31%	11.132%
99	23.822	3503	3508	3514	rBV	763753	1487884	22.68%	2.827%
100	23.986	3530	3536	3547	rVB2	2801195	6034013	91.99%	11.465%




Sum of corrected areas: 52627632

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012915.D
Acq On : 01 Dec 2022 13:09
Operator : CG/JU
Sample : N5737-01DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4345DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

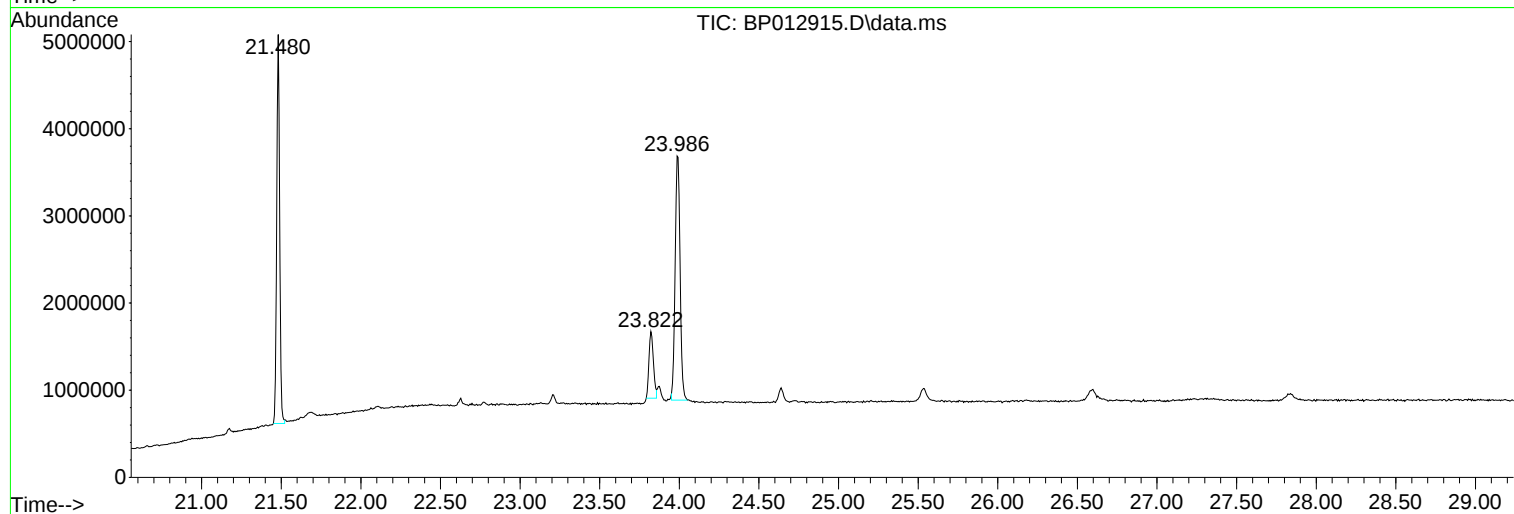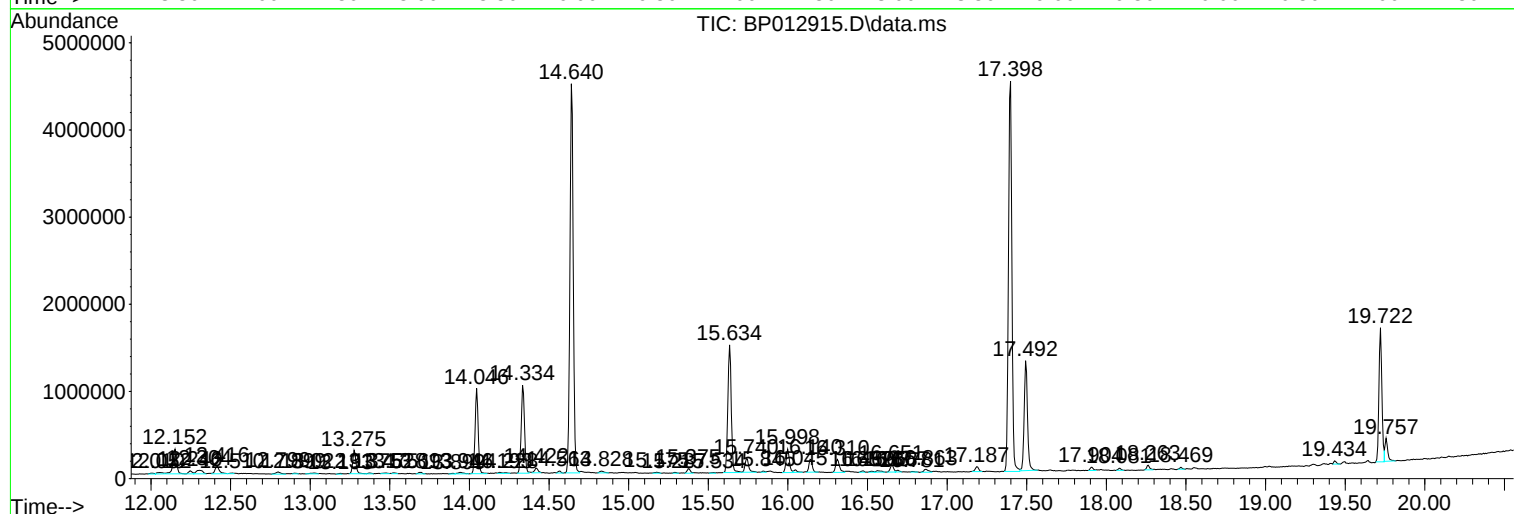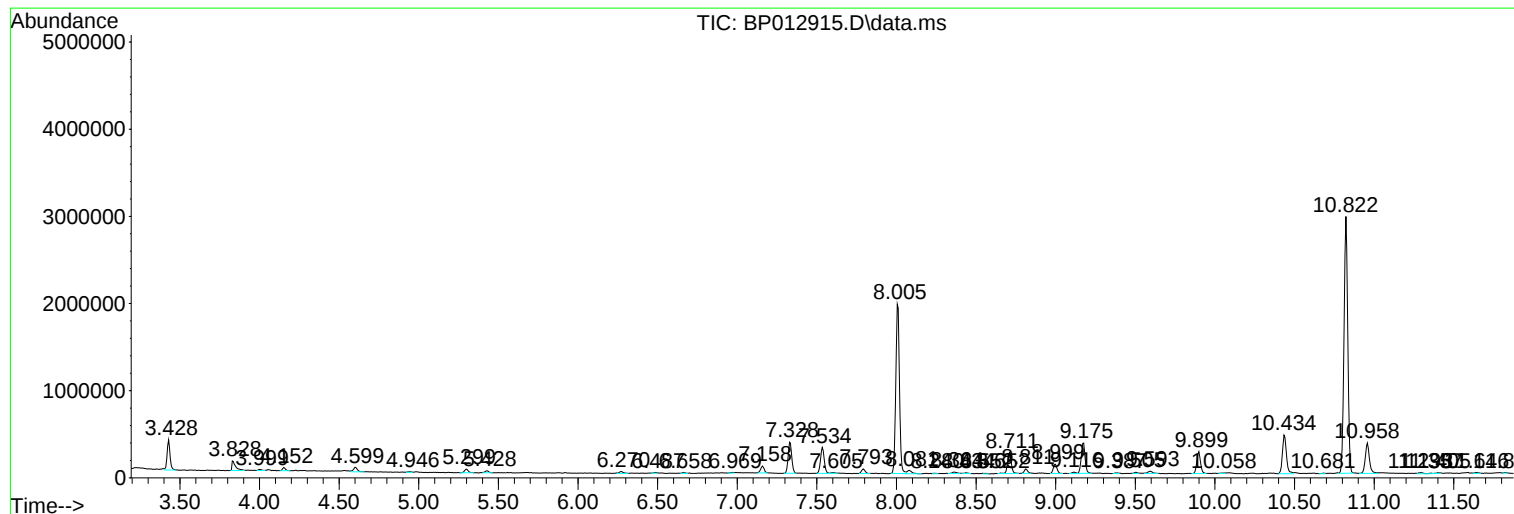

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012915.D
Acq On : 01 Dec 2022 13:09
Operator : CG/JU
Sample : N5737-01DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4345DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP113022\
Data File : BP012915.D
Acq On : 01 Dec 2022 13:09
Operator : CG/JU
Sample : N5737-01DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4345DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc