

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
 Data File : BP01294.D
 Acq On : 05 Dec 2022 16:05
 Operator : CG/JU
 Sample : N5738-16DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBNJ5DL

Quant Time: Dec 05 21:51:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 01 23:46:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	588372	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	2658562	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	1821779	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	4075402	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	3095920	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	2876065	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	4725	0.357	ng/uL	0.00
4) Pyridine-d5	3.805	84	1156	0.027	ng/ul	-0.01
7) Phenol-d5	7.158	99	78054	1.437	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	56767	1.845	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132	67615	1.698	ng/ul	0.00
15) 4-Methylphenol-d8	8.705	113	56703	1.271	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	30243	1.600	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	30164	1.394	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	66377	1.532	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	19542	0.319	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	277159	2.109	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	282756	1.949	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	13904	0.517	ng/ul	0.00
60) Fluorene-d10	15.634	176	260130	2.252	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	20550	0.859	ng/ul	0.00
73) Anthracene-d10	17.498	188	422965	2.348	ng/ul	0.00
81) Pyrene-d10	19.728	212	467592	3.073	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	281462	2.003	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	17.039	266	950137	29.112	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
Data File : BP012954.D
Acq On : 05 Dec 2022 16:05
Operator : CG/JU
Sample : N5738-16DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBNJ5DL

Quant Time: Dec 05 21:51:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 23:46:27 2022
Response via : Initial Calibration

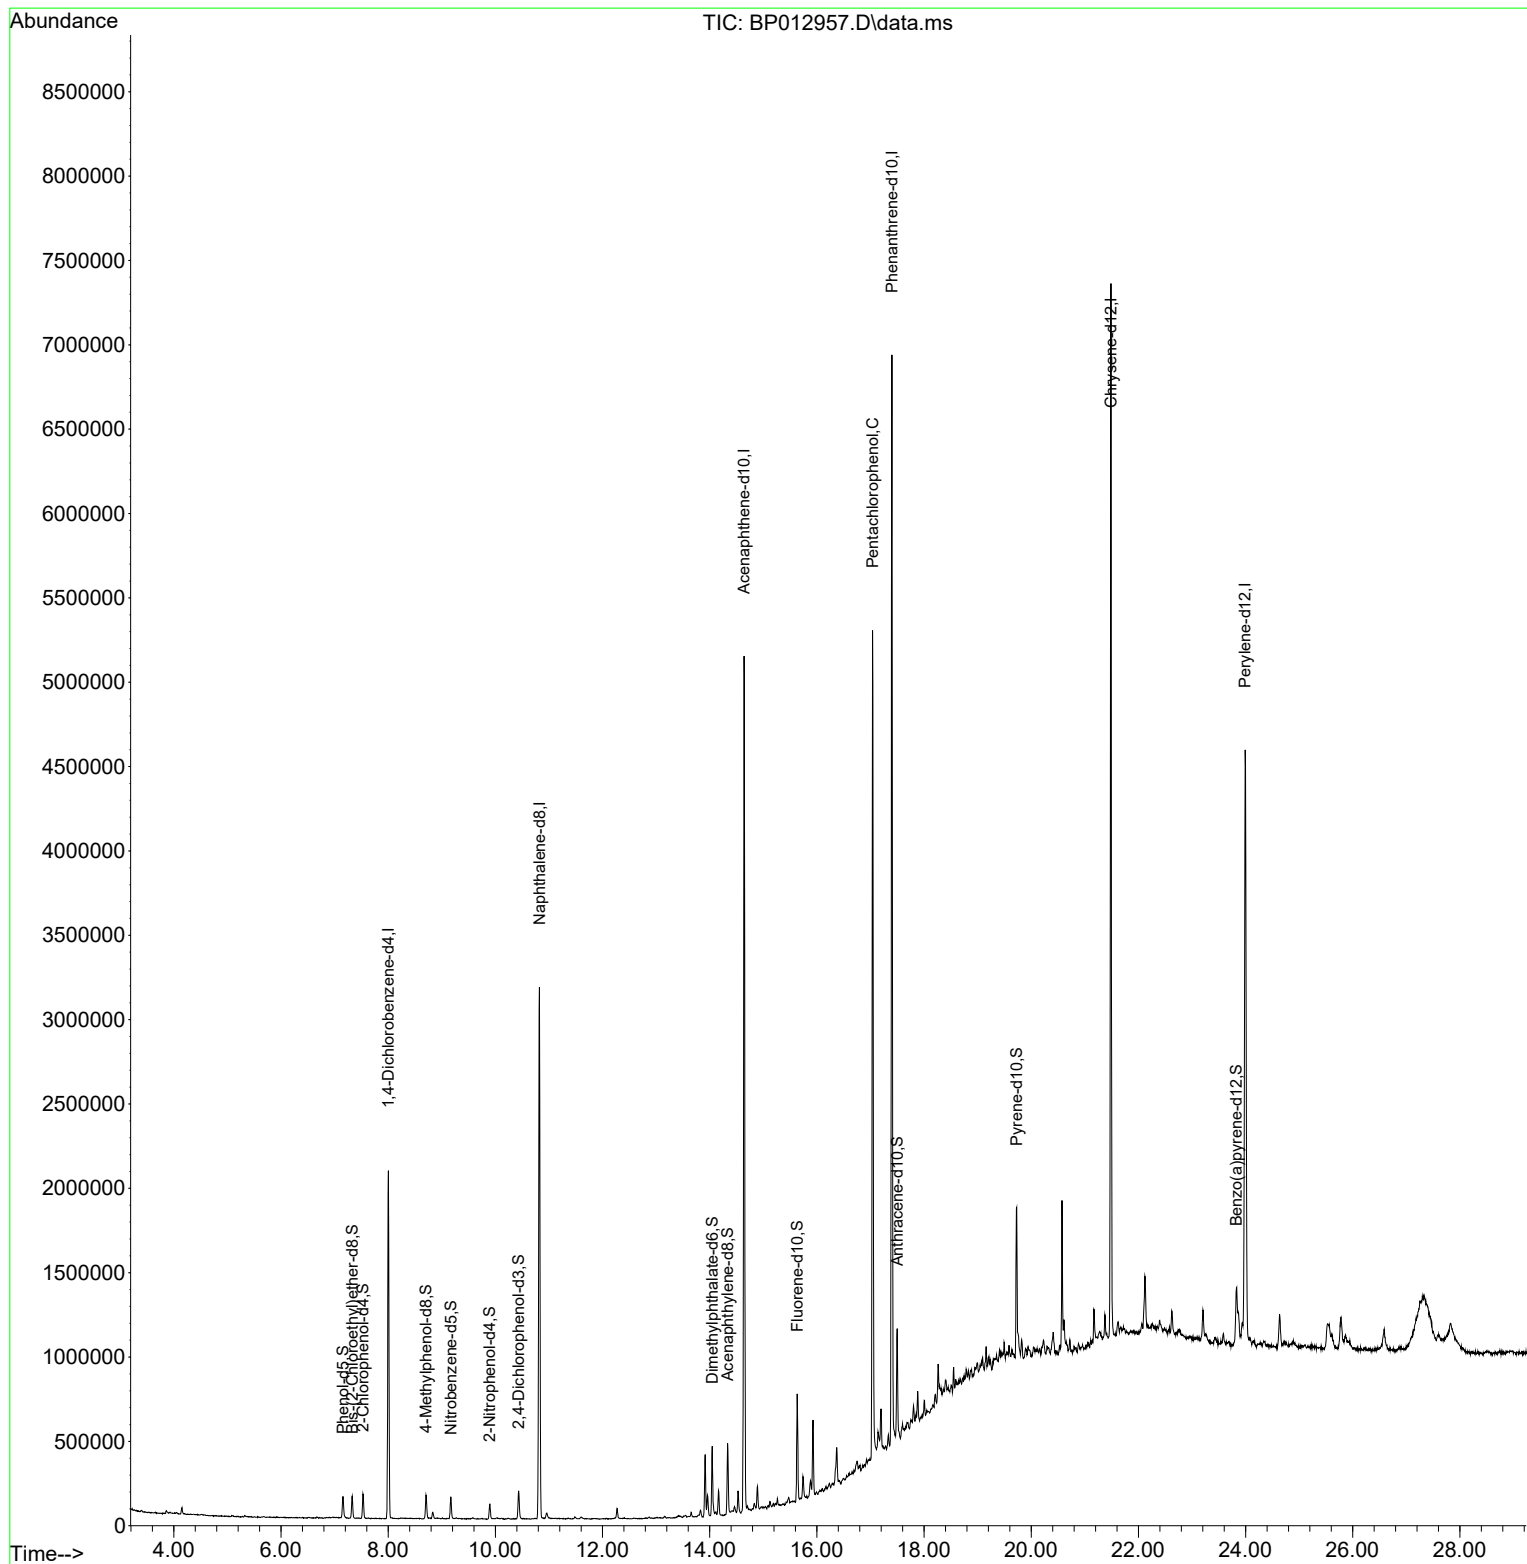

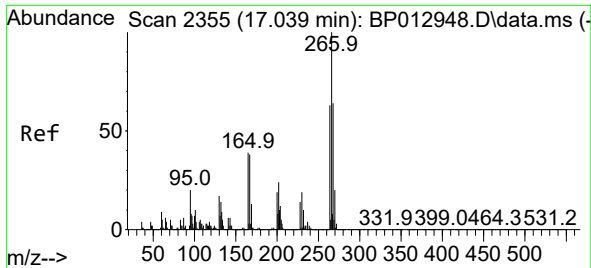

#71
 Pentachlorophenol
 Concen: 29.112 ng/ul
 RT: 17.039 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP012957.D
 Acq: 05 Dec 2022 16:05

Instrument :
 BNA_P
 ClientSampleId :
 GBNJ5DL

Tgt Ion:266 Resp: 950137
 Ion Ratio Lower Upper
 266 100
 264 62.6 50.5 75.7
 268 64.3 51.2 76.8

