

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
 Data File : BP012955.D
 Acq On : 05 Dec 2022 16:39
 Operator : CG/JU
 Sample : N5738-18DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBNJ7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.152	160	164	169	rVB	33957	46863	0.46%	0.077%
2	7.152	667	674	687	rVB	115649	213373	2.08%	0.352%
3	7.328	698	704	714	rBV	123449	195171	1.90%	0.322%
4	7.528	732	738	747	rVB	131808	223771	2.18%	0.370%
5	8.005	810	819	827	rBV	2011622	3182219	30.98%	5.256%
6	8.705	930	938	945	rBV2	112432	195553	1.90%	0.323%
7	8.828	954	959	971	rVB	29753	55760	0.54%	0.092%
8	9.169	1011	1017	1025	rBV	120685	203421	1.98%	0.336%
9	9.569	1084	1085	1095	rVB10	6645	14651	0.14%	0.024%
10	9.893	1134	1140	1147	rBV	86560	149442	1.45%	0.247%
11	10.434	1222	1232	1243	rBV	154991	290516	2.83%	0.480%
12	10.822	1290	1298	1308	rBV	2959116	5087852	49.54%	8.404%
13	10.957	1316	1321	1327	rBV2	39341	67365	0.66%	0.111%
14	11.604	1426	1431	1434	rBV7	5836	12084	0.12%	0.020%
15	12.228	1531	1537	1539	rBV7	7310	11807	0.11%	0.020%
16	12.869	1641	1646	1651	rBV9	11801	19444	0.19%	0.032%
17	13.163	1694	1696	1703	rVB8	9160	14265	0.14%	0.024%
18	13.404	1729	1737	1740	rBV8	11970	23946	0.23%	0.040%
19	13.457	1742	1746	1751	rVB5	14442	22188	0.22%	0.037%
20	13.528	1753	1758	1765	rBV	62163	111945	1.09%	0.185%
21	13.651	1776	1779	1784	rVB7	17390	25230	0.25%	0.042%
22	13.793	1797	1803	1806	rBV7	28096	43111	0.42%	0.071%
23	13.916	1818	1824	1828	rBV	162514	255641	2.49%	0.422%
24	13.957	1828	1831	1838	rVB3	80418	120693	1.18%	0.199%
25	14.045	1840	1846	1854	rBV	376985	567087	5.52%	0.937%
26	14.110	1855	1857	1861	rVV4	20884	25776	0.25%	0.043%
27	14.163	1862	1866	1872	rVB6	46137	69055	0.67%	0.114%
28	14.334	1889	1895	1902	rBV2	403473	617975	6.02%	1.021%
29	14.404	1904	1907	1910	rVB5	11111	13232	0.13%	0.022%
30	14.457	1913	1916	1918	rBV3	24418	30825	0.30%	0.051%
31	14.528	1923	1928	1934	rBV	322945	417471	4.06%	0.690%
32	14.640	1941	1947	1955	rBV	5032668	7508860	73.11%	12.403%
33	14.887	1987	1989	1994	rVB4	35408	44856	0.44%	0.074%
34	15.257	2049	2052	2058	rVB	73070	100029	0.97%	0.165%
35	15.634	2110	2116	2122	rBV	610544	921278	8.97%	1.522%
36	15.745	2131	2135	2140	rVB2	73897	109213	1.06%	0.180%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
 Data File : BP012955.D
 Acq On : 05 Dec 2022 16:39
 Operator : CG/JU
 Sample : N5738-18DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBNJ7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
 Title : SVOA CALIBRATION

37	15.887	2154	2159	2161	rBV	76026	122947	1.20%	0.203%
38	15.922	2161	2165	2171	rVB	283160	415242	4.04%	0.686%
39	16.369	2233	2241	2247	rBV	218799	448155	4.36%	0.740%
40	17.039	2349	2355	2367	rBV	7203629	10270973	100.00%	16.965%
41	17.139	2370	2372	2377	rVV	144102	224386	2.18%	0.371%
42	17.192	2378	2381	2386	rVB	248854	357824	3.48%	0.591%
43	17.328	2401	2404	2409	rVB2	212121	277256	2.70%	0.458%
44	17.398	2410	2416	2426	rBV	6299037	9207565	89.65%	15.208%
45	17.498	2428	2433	2437	rBV	584351	817858	7.96%	1.351%
46	18.263	2560	2563	2569	rBV3	243126	361482	3.52%	0.597%
47	18.545	2609	2611	2615	rVB	153358	170765	1.66%	0.282%
48	19.722	2807	2811	2819	rBV2	850650	1279092	12.45%	2.113%
49	20.575	2953	2956	2959	rBV	238795	273303	2.66%	0.451%
50	21.480	3105	3110	3121	rVB	6091074	8190378	79.74%	13.528%
51	23.992	3530	3537	3548	rVB2	3168539	7113055	69.25%	11.749%




Sum of corrected areas: 60542249

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
Data File : BP012955.D
Acq On : 05 Dec 2022 16:39
Operator : CG/JU
Sample : N5738-18DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBNJ7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

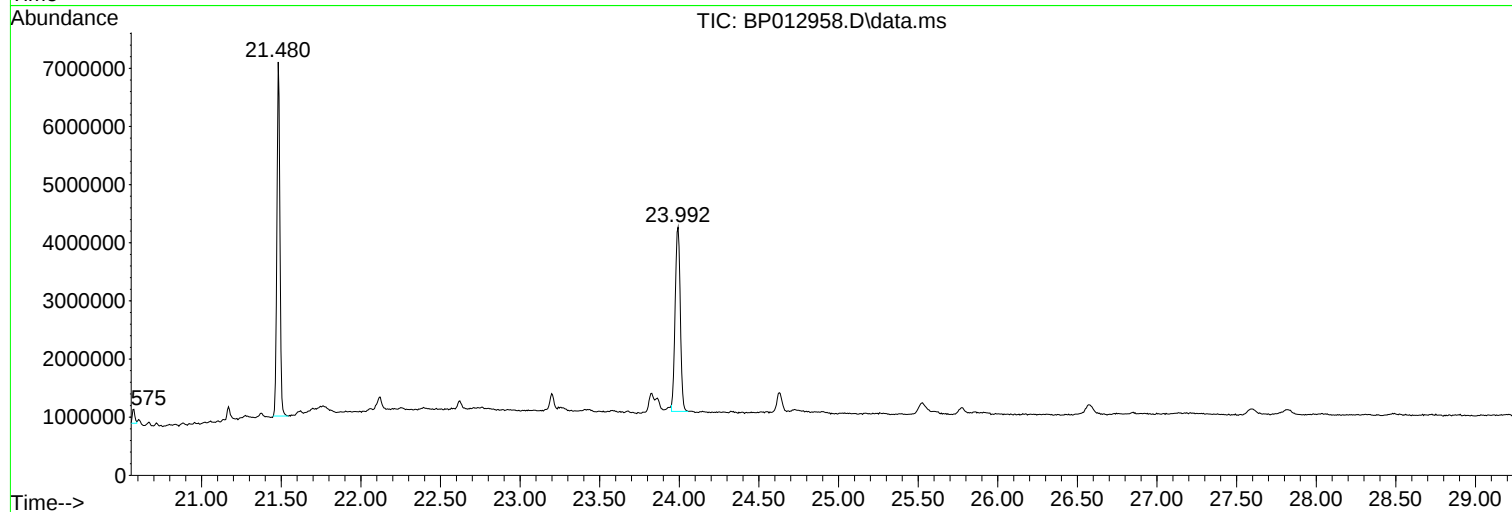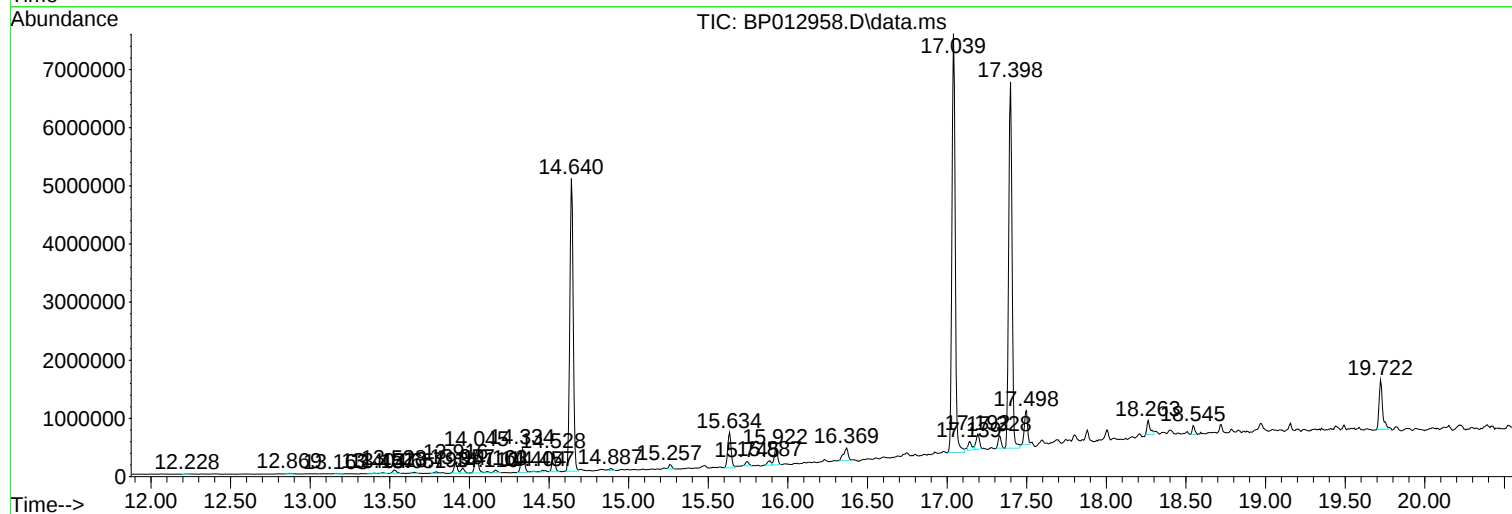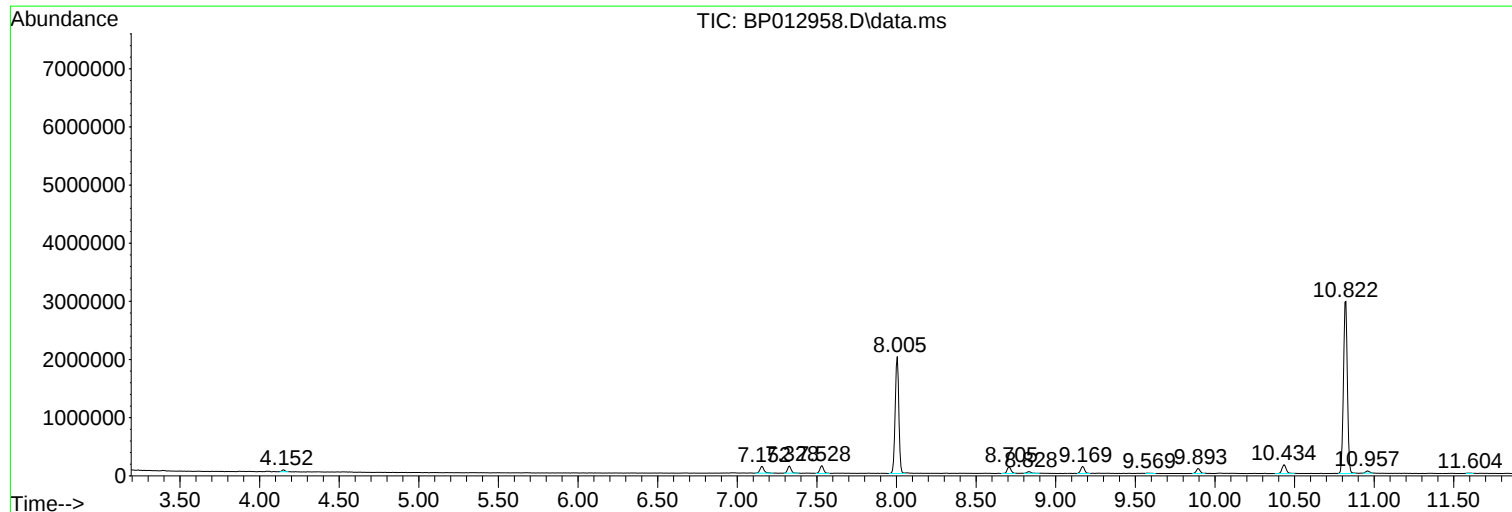

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
Data File : BP012955.D
Acq On : 05 Dec 2022 16:39
Operator : CG/JU
Sample : N5738-18DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBNJ7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120522\
Data File : BP012955.D
Acq On : 05 Dec 2022 16:39
Operator : CG/JU
Sample : N5738-18DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBNJ7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc