




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012982.D
Acq On : 08 Dec 2022 13:40
Operator : CG/JU
Sample : N5832-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK5

Manual IntegrationsAPPROVED

Quant Time: Dec 09 01:53:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 00:35:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

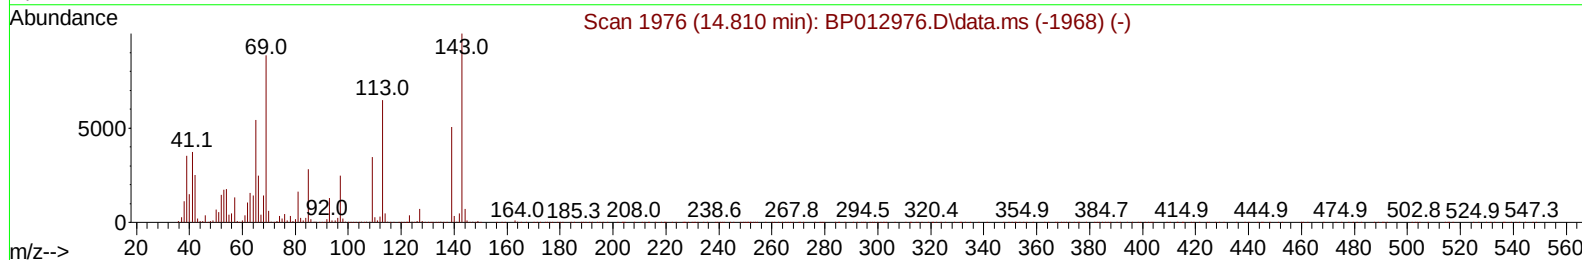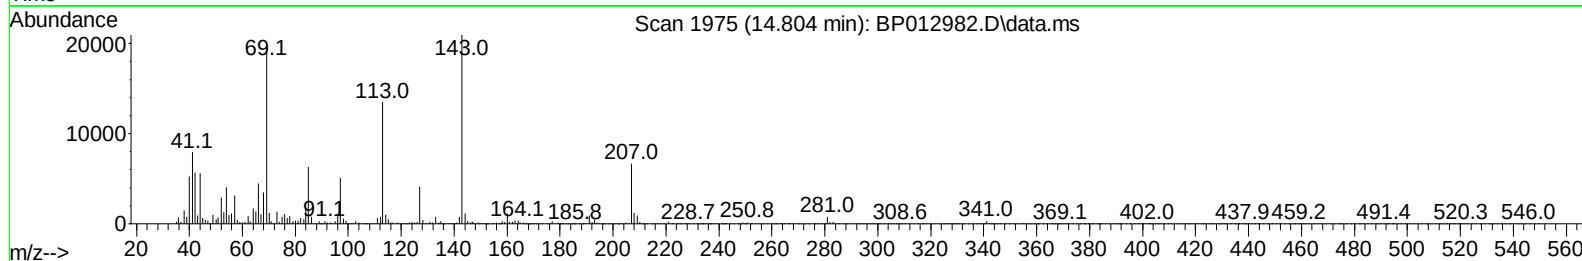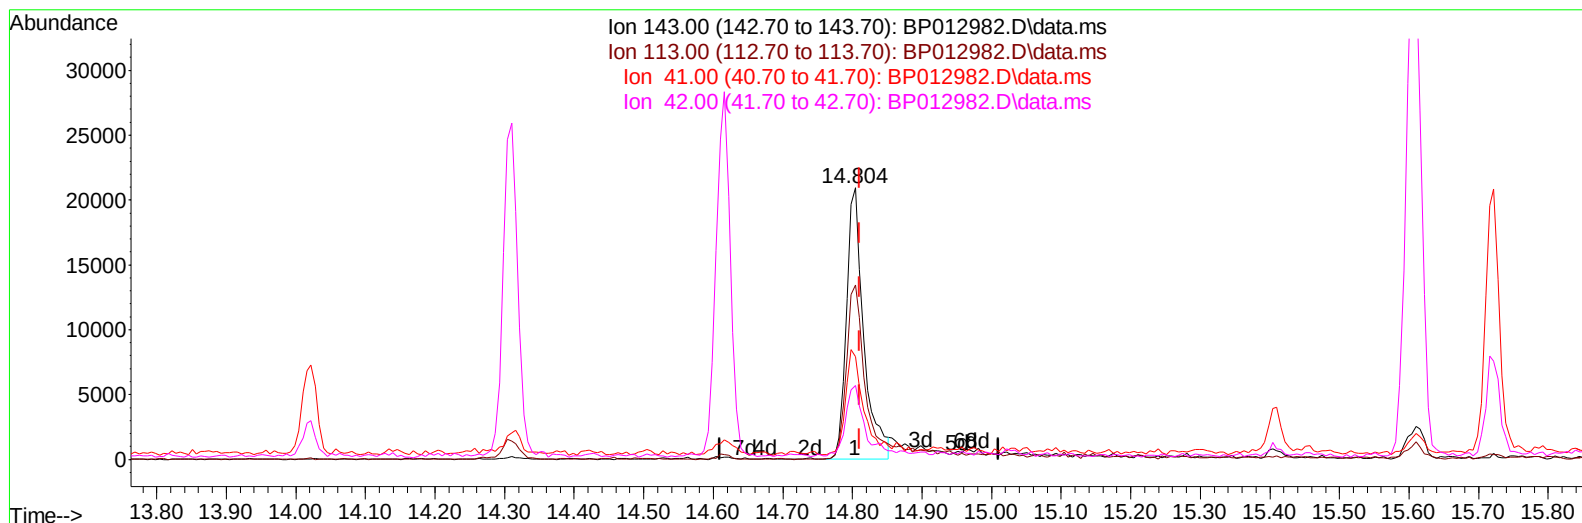

TIC: BP012982.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (-0.006) 1.72 ng/u1

response 36148

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	65.80	64.33
41.00	35.70	37.93
42.00	24.70	27.28

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012982.D
 Acq On : 08 Dec 2022 13:40
 Operator : CG/JU
 Sample : N5832-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYK5

Manual IntegrationsAPPROVED

Quant Time: Dec 09 01:53:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 00:35:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/09/2022
 Supervised By :mohammad ahmed 12/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	552736	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	2306368	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.616	164	1517998	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	3293904	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240	2350760	20.000	ng/ul	0.00
88) Perylene-d12	23.945	264	2003901	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	54297	4.200	ng/uL	0.00
4) Pyridine-d5	3.793	84	138881	3.782	ng/ul	0.00
7) Phenol-d5	7.128	99	206391	4.584	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	752401	27.704	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	717940	20.257	ng/ul	0.00
15) 4-Methylphenol-d8	8.681	113	417472	11.317	ng/ul	0.00
21) Nitrobenzene-d5	9.146	128	463963	27.380	ng/ul	0.00
24) 2-Nitrophenol-d4	9.869	143	455863	23.895	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	836938	22.586	ng/ul	0.00
31) 4-Chloroaniline-d4	10.928	131	1079021	20.627	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	3465985	29.709	ng/ul	0.00
49) Acenaphthylene-d8	14.310	160	3617625	28.220	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	38630m	1.841	ng/ul	0.00
60) Fluorene-d10	15.610	176	2963443	30.025	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	342761	16.170	ng/ul	0.00
73) Anthracene-d10	17.469	188	5107699	34.371	ng/ul	0.00
81) Pyrene-d10	19.698	212	5604787	41.537	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.780	264	3540767	35.449	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012982.D
Acq On : 08 Dec 2022 13:40
Operator : CG/JU
Sample : N5832-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

Quant Time: Dec 09 01:53:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 00:35:07 2022
Response via : Initial Calibration

