

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012977.D
 Acq On : 08 Dec 2022 09:16
 Operator : CG/JU
 Sample : PB149448BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	40	rVB	173431	244270	1.42%	0.143%
2	3.787	99	102	123	rBV	2044975	3230026	18.74%	1.885%
3	4.117	154	158	164	rBV	44761	61402	0.36%	0.036%
4	7.134	663	671	684	rBV	2306398	3687844	21.40%	2.152%
5	7.305	693	700	711	rVB	2047966	3224592	18.71%	1.881%
6	7.505	727	734	746	rBV	2480506	3894567	22.60%	2.272%
7	7.975	807	814	823	rBV	2318264	3684375	21.38%	2.150%
8	8.681	927	934	944	rBV	2931370	4726145	27.43%	2.758%
9	9.146	1006	1013	1027	rBV	2341751	3753715	21.78%	2.190%
10	9.869	1128	1136	1148	rBV	1971185	3146175	18.26%	1.836%
11	10.404	1219	1227	1243	rBV	3030025	5021917	29.14%	2.930%
12	10.793	1285	1293	1304	rVB	3370542	5543505	32.17%	3.235%
13	10.928	1308	1316	1328	rBV	3032425	5191798	30.13%	3.029%
14	12.375	1554	1562	1569	rBV	61260	102145	0.59%	0.060%
15	14.022	1835	1842	1853	rBV	6357243	8550127	49.62%	4.989%
16	14.310	1884	1891	1909	rBV	6813303	9877000	57.32%	5.763%
17	14.616	1936	1943	1951	rBV	5571034	8115047	47.09%	4.735%
18	14.804	1968	1975	1993	rBV	2518173	3756499	21.80%	2.192%
19	15.022	2009	2012	2020	rVB10	15645	28777	0.17%	0.017%
20	15.610	2105	2112	2125	rBV	8663303	12585135	73.03%	7.343%
21	15.722	2125	2131	2148	rVV	3001505	4039782	23.44%	2.357%
22	15.851	2148	2153	2158	rVB	40069	64409	0.37%	0.038%
23	16.392	2240	2245	2251	rBV9	12267	21798	0.13%	0.013%
24	17.157	2370	2375	2382	rBV	17552	30367	0.18%	0.018%
25	17.375	2405	2412	2422	rBV	6931262	10176829	59.06%	5.938%
26	17.469	2422	2428	2456	rVB	9616604	14223632	82.54%	8.299%
27	17.751	2473	2476	2482	rVB6	10770	19249	0.11%	0.011%
28	18.239	2556	2559	2563	rVB5	14291	20352	0.12%	0.012%
29	19.275	2731	2735	2740	rBV	125049	171012	0.99%	0.100%
30	19.345	2743	2747	2751	rBV	127510	174121	1.01%	0.102%
31	19.704	2801	2808	2823	rBV	12473657	17231765	100.00%	10.054%
32	21.457	3101	3106	3115	rBV	8274374	10717229	62.19%	6.253%
33	23.786	3495	3502	3521	rVB2	7680079	15692147	91.07%	9.156%
34	23.951	3522	3530	3545	rVB2	4850944	10376687	60.22%	6.055%

Sum of corrected areas: 171384440

Instrument :

BNA_P

ClientSampleId :




SBLK448

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012977.D
Acq On : 08 Dec 2022 09:16
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

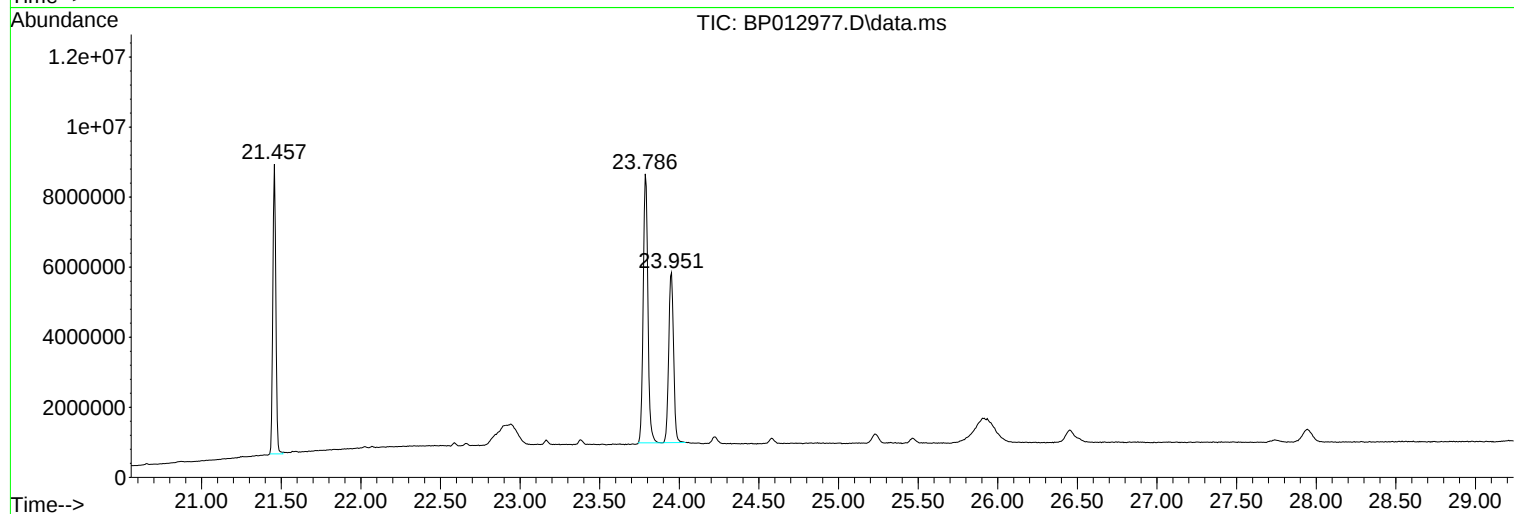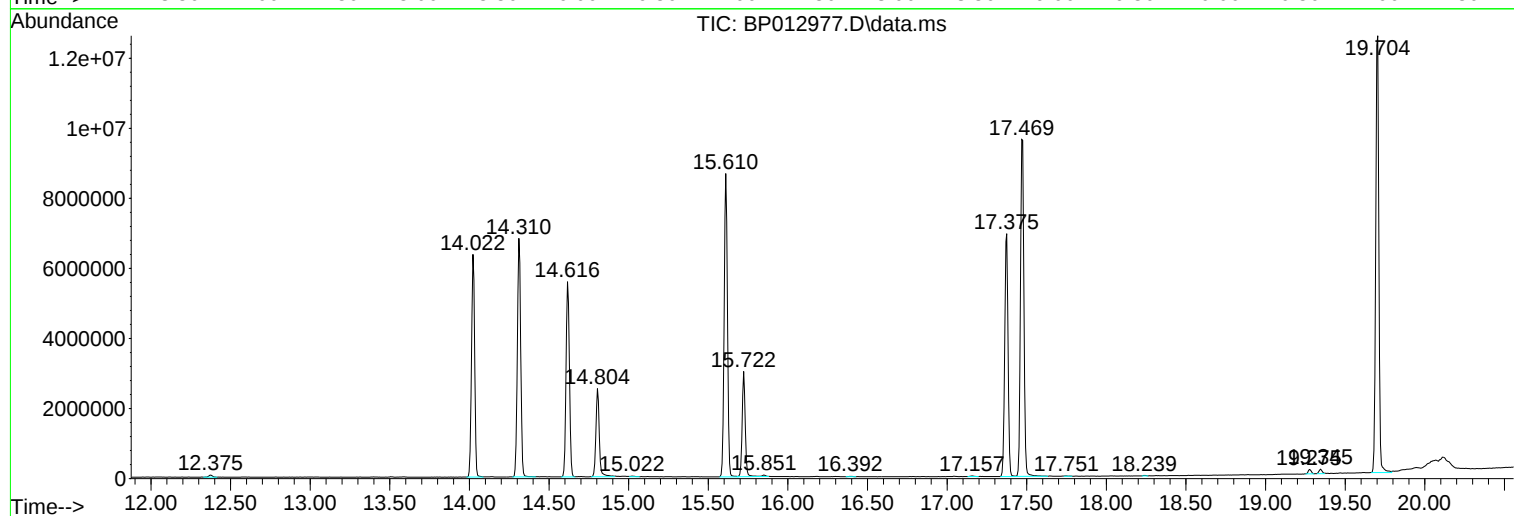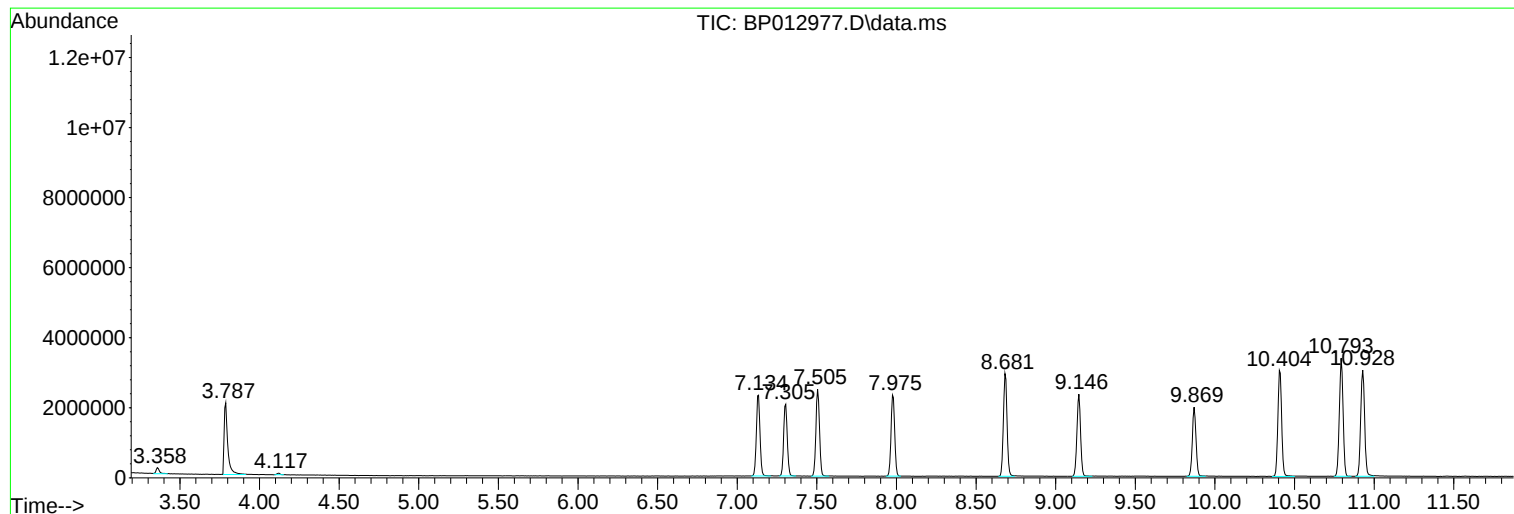

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012977.D
Acq On : 08 Dec 2022 09:16
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012977.D
Acq On : 08 Dec 2022 09:16
Operator : CG/JU
Sample : PB149448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc