

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012982.D
 Acq On : 08 Dec 2022 13:40
 Operator : CG/JU
 Sample : N5832-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	37	rBV	116263	158230	1.12%	0.132%
2	3.793	100	103	124	rBV	239011	415650	2.95%	0.346%
3	4.022	137	142	147	rVB	55433	84732	0.60%	0.071%
4	4.116	155	158	165	rVB	42715	63590	0.45%	0.053%
5	5.063	316	319	323	rVB4	10936	19223	0.14%	0.016%
6	7.128	662	670	682	rVB	354886	595037	4.22%	0.496%
7	7.299	692	699	710	rVB	1741943	2704592	19.18%	2.253%
8	7.505	726	734	742	rBV	1571892	2433373	17.26%	2.027%
9	7.593	746	749	756	rVB8	12155	24359	0.17%	0.020%
10	7.975	807	814	822	rBV	2023200	3133010	22.22%	2.610%
11	8.681	928	934	946	rBV	1115806	1776244	12.60%	1.480%
12	9.146	1005	1013	1027	rBV	1887184	3141305	22.28%	2.617%
13	9.551	1078	1082	1090	rVB	87971	139295	0.99%	0.116%
14	9.869	1127	1136	1144	rBV	1405056	2277337	16.15%	1.897%
15	10.404	1220	1227	1238	rBV	2195740	3643514	25.84%	3.035%
16	10.793	1284	1293	1302	rBV	2766396	4617059	32.75%	3.846%
17	10.928	1307	1316	1331	rBV	1938959	3406822	24.17%	2.838%
18	12.051	1501	1507	1517	rVB2	148969	229231	1.63%	0.191%
19	12.375	1557	1562	1569	rVB	44613	74988	0.53%	0.062%
20	12.975	1657	1664	1670	rBV8	13396	26621	0.19%	0.022%
21	13.222	1703	1706	1713	rVB7	15230	21872	0.16%	0.018%
22	13.398	1731	1736	1741	rBV8	6588	16341	0.12%	0.014%
23	13.504	1749	1754	1760	rBV8	8449	15573	0.11%	0.013%
24	13.587	1764	1768	1774	rVB7	10380	17711	0.13%	0.015%
25	14.022	1835	1842	1855	rBV	5139055	7087302	50.27%	5.903%
26	14.134	1859	1861	1866	rVB6	10651	14685	0.10%	0.012%
27	14.310	1884	1891	1902	rBV	5684292	7968610	56.52%	6.638%
28	14.616	1936	1943	1954	rBV	4483669	6525516	46.29%	5.435%
29	14.804	1968	1975	1987	rBV	128369	262668	1.86%	0.219%
30	15.028	2007	2013	2017	rBV5	38253	60575	0.43%	0.050%
31	15.410	2071	2078	2083	rBV	71453	113330	0.80%	0.094%
32	15.610	2103	2112	2124	rBV	7470562	10732497	76.13%	8.940%
33	15.722	2125	2131	2148	rVV	1668403	2310655	16.39%	1.925%
34	15.851	2148	2153	2159	rVB	34787	58958	0.42%	0.049%
35	16.392	2240	2245	2251	rVB10	9657	17629	0.13%	0.015%
36	17.045	2354	2356	2361	rVB6	13029	18829	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012982.D
 Acq On : 08 Dec 2022 13:40
 Operator : CG/JU
 Sample : N5832-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.157	2371	2375	2381	rVB5	11921	19733	0.14%	0.016%
38	17.369	2404	2411	2421	rBV	5408351	7698937	54.61%	6.413%
39	17.469	2421	2428	2441	rBV	8536480	12509760	88.73%	10.420%
40	17.651	2457	2459	2466	rVB5	10273	14870	0.11%	0.012%
41	17.980	2511	2515	2519	rBV6	8902	15998	0.11%	0.013%
42	18.233	2555	2558	2566	rBV8	21973	36086	0.26%	0.030%
43	19.274	2731	2735	2740	rVB	106253	142973	1.01%	0.119%
44	19.345	2743	2747	2751	rBV	94956	128559	0.91%	0.107%
45	19.698	2801	2807	2819	rBV	10462759	14098132	100.00%	11.743%
46	21.457	3100	3106	3115	rBV	4621307	6515996	46.22%	5.428%
47	23.780	3495	3501	3519	rVB2	4599307	9421770	66.83%	7.848%
48	23.945	3523	3529	3545	rVB2	2521509	5244267	37.20%	4.368%




Sum of corrected areas: 120054044

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012982.D
Acq On : 08 Dec 2022 13:40
Operator : CG/JU
Sample : N5832-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

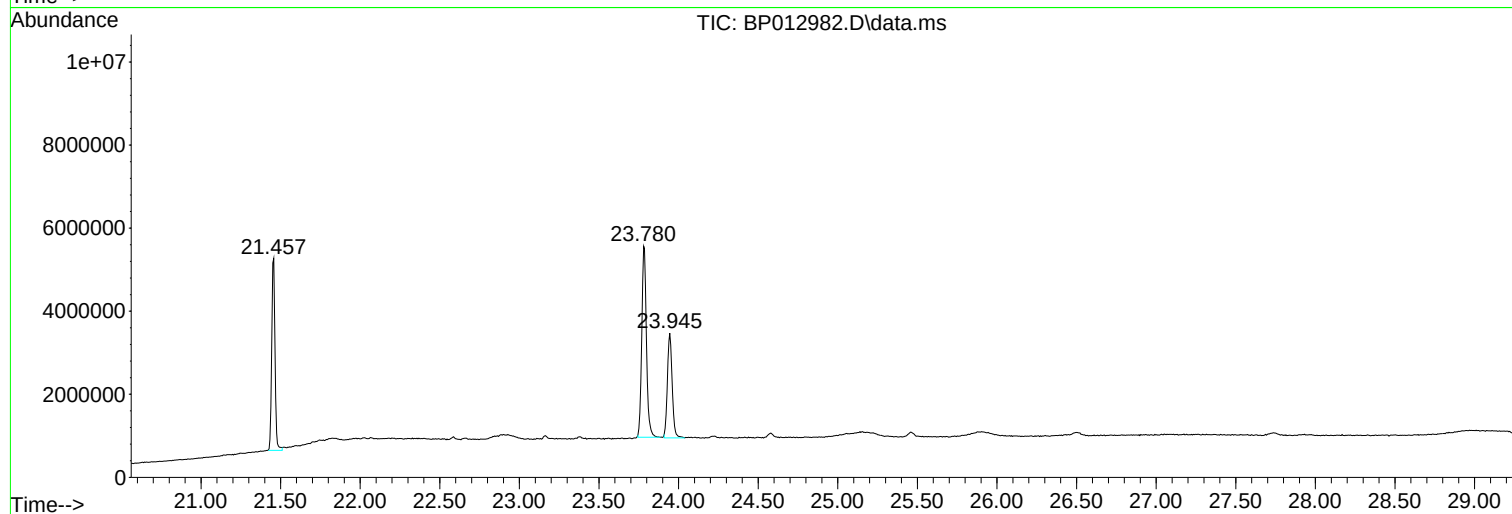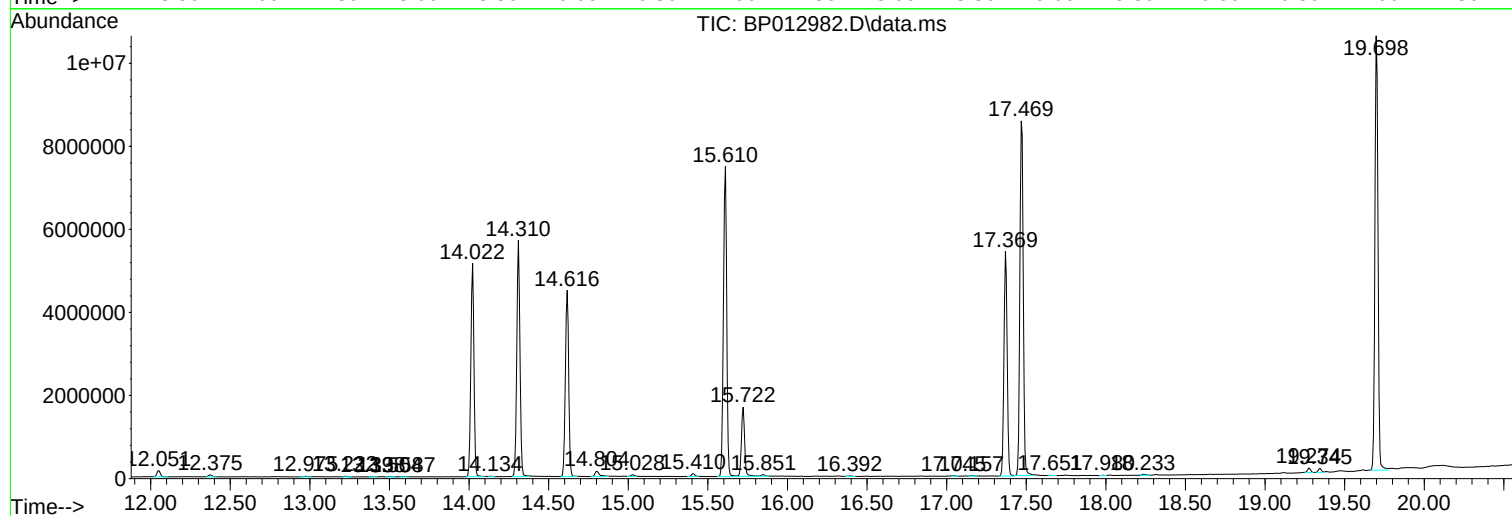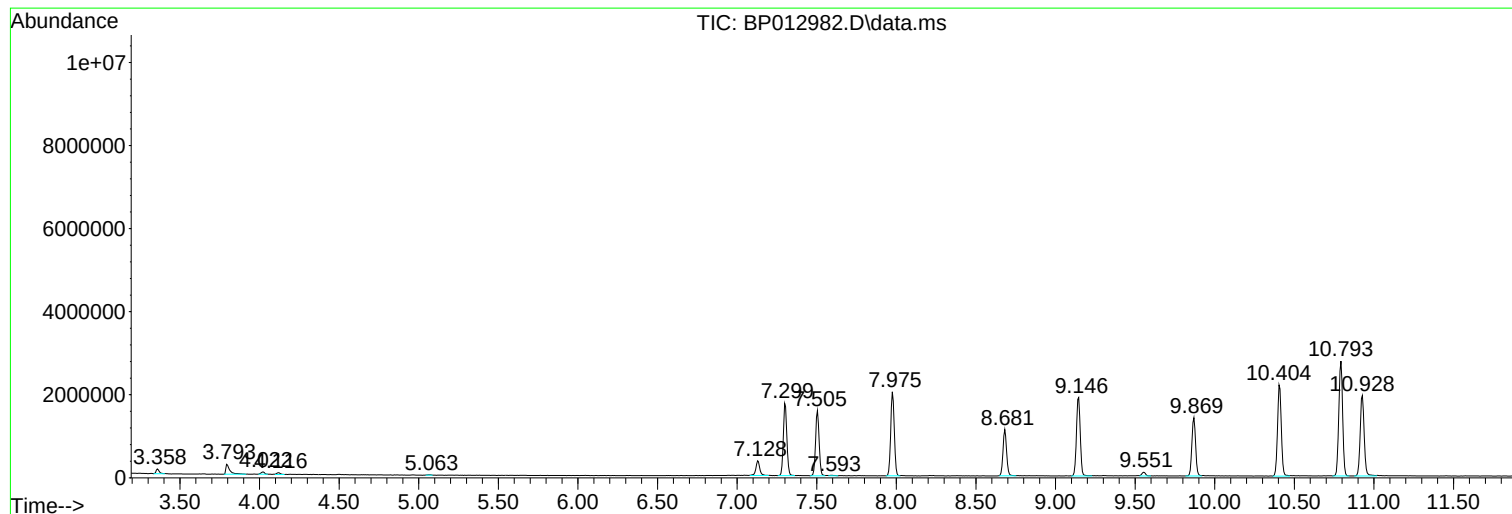

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012982.D
Acq On : 08 Dec 2022 13:40
Operator : CG/JU
Sample : N5832-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012982.D
Acq On : 08 Dec 2022 13:40
Operator : CG/JU
Sample : N5832-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc