

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012987.D
 Acq On : 08 Dec 2022 16:32
 Operator : CG/JU
 Sample : PB149469BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK469

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	37	rVB	137767	204044	1.24%	0.130%
2	3.781	97	101	117	rBV	1699915	2717374	16.46%	1.730%
3	4.117	154	158	165	rVB	31086	48999	0.30%	0.031%
4	7.128	661	670	680	rBV	2164037	3323447	20.13%	2.116%
5	7.299	693	699	713	rVB	1879970	2909019	17.62%	1.852%
6	7.505	726	734	744	rBV	2172146	3428325	20.77%	2.183%
7	7.975	807	814	824	rVB	1925307	2994289	18.14%	1.906%
8	8.681	923	934	949	rBV	2718030	4315842	26.14%	2.748%
9	9.140	1005	1012	1022	rBV	2042097	3400721	20.60%	2.165%
10	9.869	1126	1136	1147	rBV	1733669	2810895	17.03%	1.790%
11	10.405	1218	1227	1239	rBV	2787775	4548683	27.55%	2.896%
12	10.793	1284	1293	1303	rBV	2766442	4614615	27.95%	2.938%
13	10.928	1307	1316	1334	rBV	2674395	4656682	28.21%	2.965%
14	12.375	1556	1562	1568	rBV	49946	87212	0.53%	0.056%
15	13.504	1750	1754	1760	rVB5	16009	25978	0.16%	0.017%
16	14.022	1834	1842	1851	rBV	5824470	7793967	47.21%	4.962%
17	14.310	1882	1891	1912	rBV	6230347	8969901	54.33%	5.711%
18	14.616	1936	1943	1952	rBV	4651803	6811998	41.26%	4.337%
19	14.804	1967	1975	1996	rBV	2305322	3501235	21.21%	2.229%
20	14.975	2000	2004	2008	rVV7	11666	23038	0.14%	0.015%
21	15.022	2008	2012	2016	rVB6	10793	18343	0.11%	0.012%
22	15.610	2104	2112	2124	rBV	8439123	11788435	71.40%	7.505%
23	15.722	2124	2131	2148	rVV	2690349	3570137	21.62%	2.273%
24	15.851	2148	2153	2160	rVB2	40727	67907	0.41%	0.043%
25	17.045	2353	2356	2361	rVB7	13448	16712	0.10%	0.011%
26	17.157	2370	2375	2381	rVB5	14682	27011	0.16%	0.017%
27	17.369	2405	2411	2421	rBV	5947084	8560846	51.85%	5.450%
28	17.469	2421	2428	2449	rVV	9366869	13464168	81.55%	8.572%
29	19.281	2731	2736	2741	rBV2	116863	173031	1.05%	0.110%
30	19.345	2743	2747	2755	rVV	101850	158965	0.96%	0.101%
31	19.698	2802	2807	2819	rBV	12191519	16284861	98.64%	10.368%
32	21.457	3101	3106	3115	rBV	7193661	9439496	57.18%	6.010%
33	23.786	3495	3502	3518	rVB2	8070859	16509774	100.00%	10.511%
34	23.951	3522	3530	3541	rVB2	4600463	9807570	59.40%	6.244%

Sum of corrected areas: 157073520

Instrument :

BNA_P

ClientSampleId :




SBLK469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012987.D
Acq On : 08 Dec 2022 16:32
Operator : CG/JU
Sample : PB149469BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

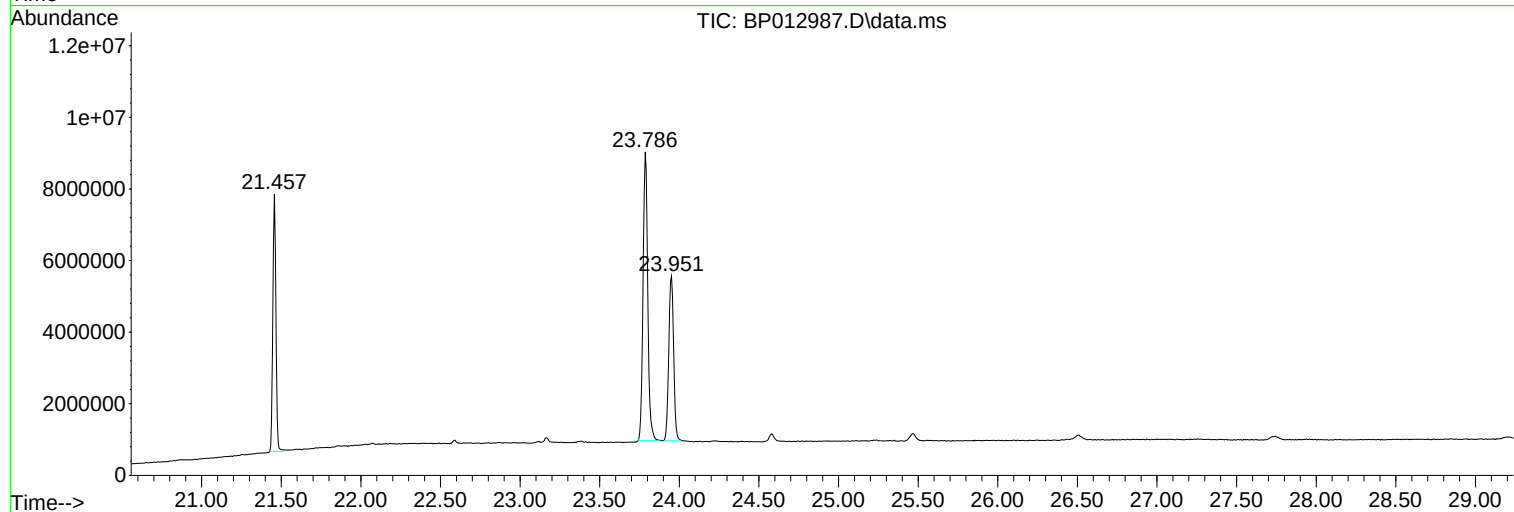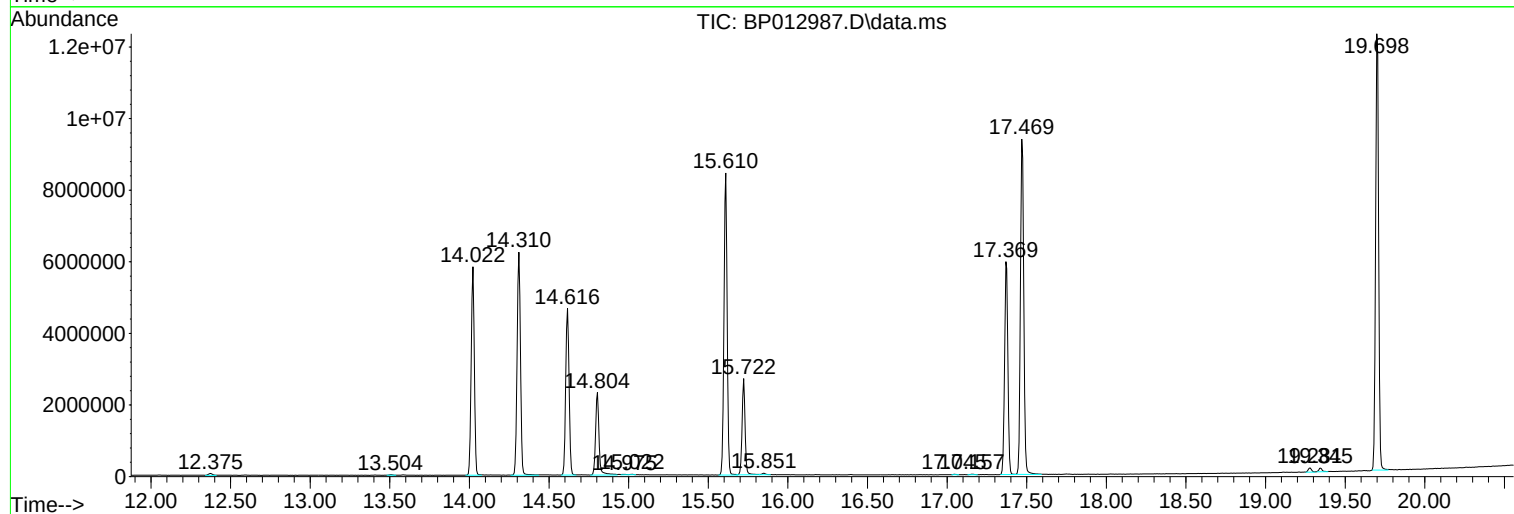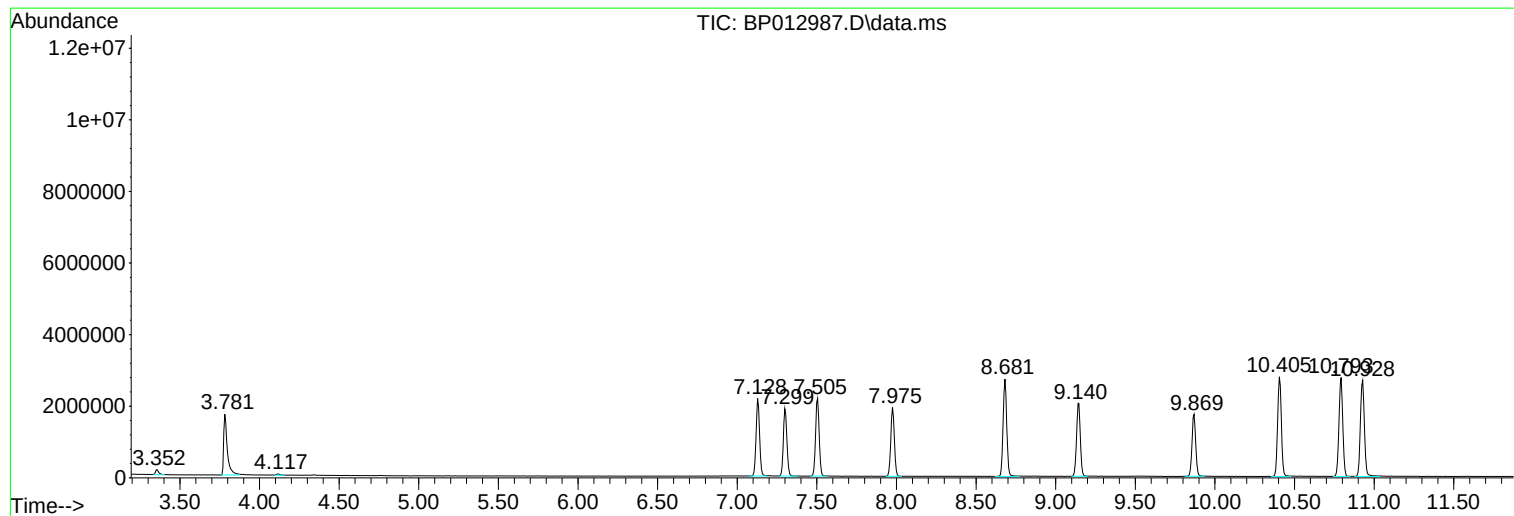

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012987.D
Acq On : 08 Dec 2022 16:32
Operator : CG/JU
Sample : PB149469BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012987.D
Acq On : 08 Dec 2022 16:32
Operator : CG/JU
Sample : PB149469BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc