

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012988.D
 Acq On : 08 Dec 2022 17:06
 Operator : CG/JU
 Sample : PB149470BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	36	rBV	154161	223938	1.26%	0.130%
2	3.781	97	101	124	rBV	2082772	3254059	18.37%	1.884%
3	4.117	153	158	163	rBV	37306	53775	0.30%	0.031%
4	7.128	663	670	687	rBV	2470549	3841345	21.69%	2.224%
5	7.299	693	699	708	rBV	2174078	3321750	18.75%	1.923%
6	7.505	727	734	745	rBV	2472693	3928213	22.18%	2.274%
7	7.975	806	814	825	rBV	2116079	3292835	18.59%	1.906%
8	8.681	926	934	950	rBV	3163316	4970713	28.06%	2.878%
9	9.146	1005	1013	1024	rBV	2371402	3911919	22.08%	2.265%
10	9.869	1126	1136	1148	rBV	2000241	3242772	18.31%	1.877%
11	10.405	1219	1227	1238	rBV	3174044	5178557	29.23%	2.998%
12	10.793	1285	1293	1301	rBV	2966868	5010299	28.28%	2.901%
13	10.928	1307	1316	1336	rBV	3150106	5401105	30.49%	3.127%
14	12.375	1554	1562	1572	rBV	53234	95153	0.54%	0.055%
15	13.504	1748	1754	1762	rBV4	22972	35718	0.20%	0.021%
16	13.581	1762	1767	1775	rVB6	11948	23121	0.13%	0.013%
17	14.022	1834	1842	1858	rBV	6694049	8900413	50.25%	5.153%
18	14.310	1883	1891	1907	rBV	7009755	10138586	57.23%	5.870%
19	14.616	1936	1943	1953	rBV	5188249	7383204	41.68%	4.275%
20	14.804	1968	1975	1997	rBV	2668544	4003786	22.60%	2.318%
21	15.028	2008	2013	2018	rVB6	19002	30363	0.17%	0.018%
22	15.610	2103	2112	2125	rBV	9392908	13297373	75.07%	7.699%
23	15.722	2125	2131	2147	rVV	3071647	4084081	23.06%	2.365%
24	15.845	2148	2152	2163	rVB2	45269	84521	0.48%	0.049%
25	16.392	2240	2245	2252	rBV8	11027	19408	0.11%	0.011%
26	17.151	2370	2374	2379	rBV2	12467	22071	0.12%	0.013%
27	17.369	2404	2411	2421	rBV	6414239	9189777	51.88%	5.320%
28	17.469	2421	2428	2449	rVV	10253301	14814036	83.63%	8.577%
29	19.275	2731	2735	2740	rBV2	124223	172645	0.97%	0.100%
30	19.345	2742	2747	2752	rVV	118088	169204	0.96%	0.098%
31	19.698	2801	2807	2820	rBV	13434194	17713995	100.00%	10.256%
32	21.457	3100	3106	3114	rBV	7002340	9857846	55.65%	5.707%
33	23.786	3494	3502	3518	rVV2	8140430	17216389	97.19%	9.968%
34	23.945	3522	3529	3547	rVB2	4677641	9841356	55.56%	5.698%

Sum of corrected areas: 172724326




Instrument :
BNA_P
ClientSampleId :
SBLK470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012988.D
Acq On : 08 Dec 2022 17:06
Operator : CG/JU
Sample : PB149470BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

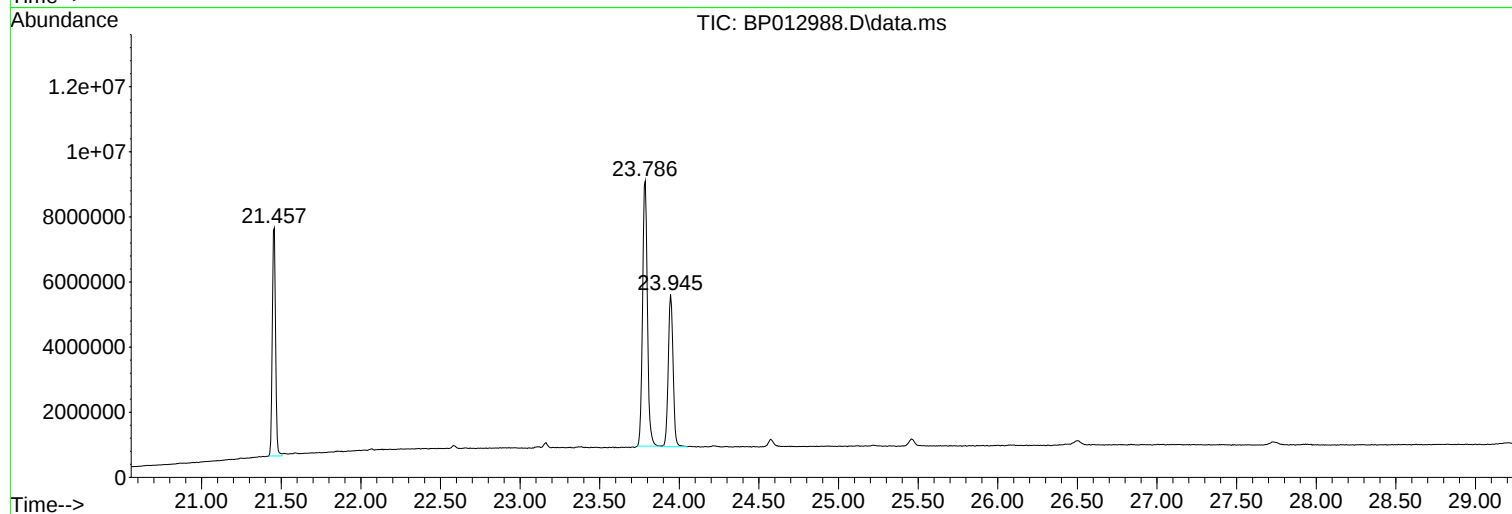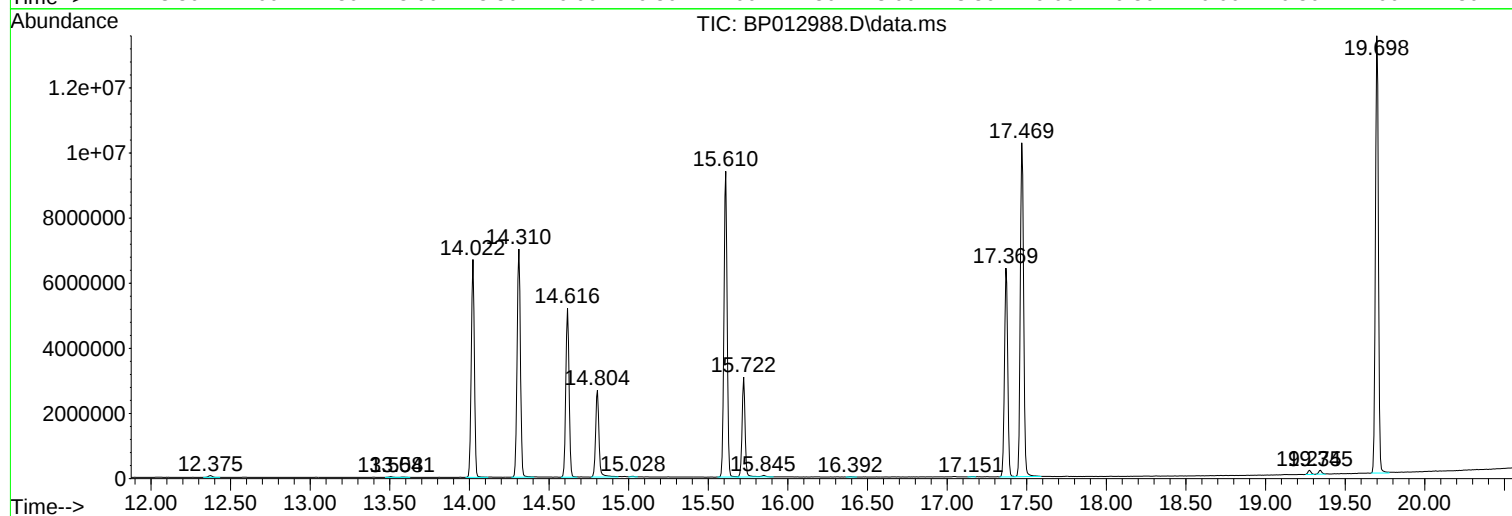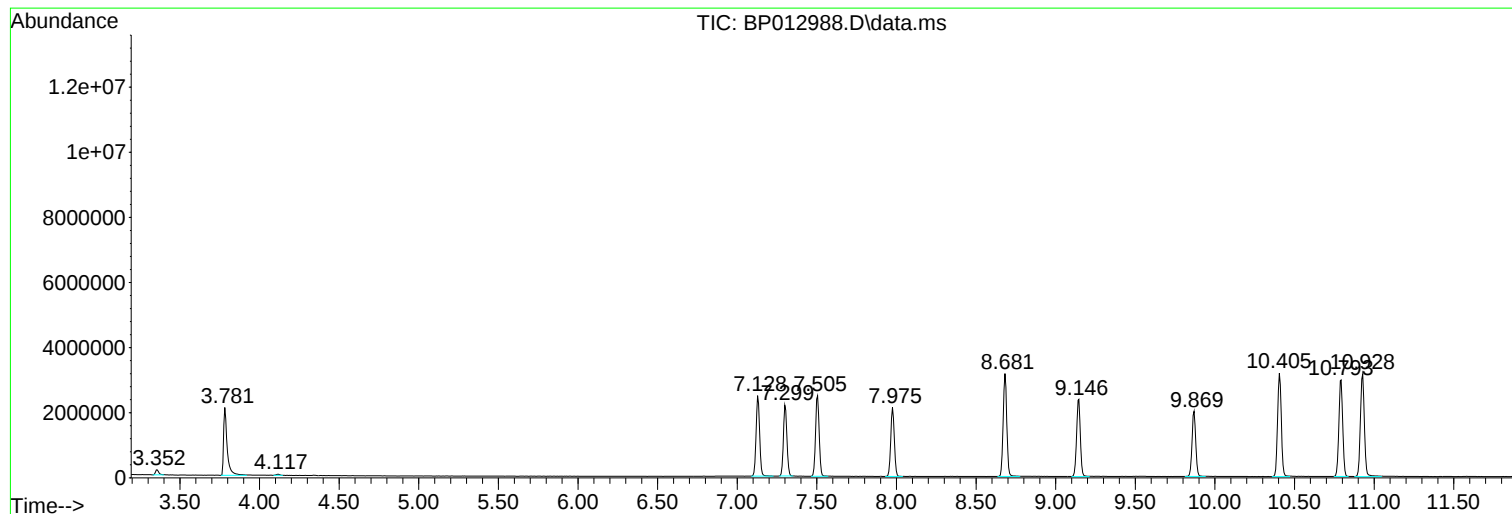

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012988.D
Acq On : 08 Dec 2022 17:06
Operator : CG/JU
Sample : PB149470BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012988.D
Acq On : 08 Dec 2022 17:06
Operator : CG/JU
Sample : PB149470BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc