

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012989.D
 Acq On : 08 Dec 2022 17:40
 Operator : CG/JU
 Sample : N5894-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	37	rVB	120414	173409	0.87%	0.106%
2	3.787	100	102	125	rBV	350492	622877	3.11%	0.379%
3	4.016	137	141	147	rVB	49057	77834	0.39%	0.047%
4	4.116	154	158	164	rVB	43241	66433	0.33%	0.040%
5	7.128	663	670	678	rBV	426354	664613	3.32%	0.404%
6	7.299	692	699	709	rBV	1833050	2823569	14.09%	1.718%
7	7.505	727	734	745	rBV	1577330	2494566	12.45%	1.518%
8	7.975	807	814	821	rBV	2235150	3489482	17.41%	2.123%
9	8.057	823	828	834	rVB	33243	53905	0.27%	0.033%
10	8.246	855	860	868	rVB	26276	41999	0.21%	0.026%
11	8.681	926	934	948	rBV	1295573	2049413	10.23%	1.247%
12	9.140	1005	1012	1022	rBV	2053614	3407997	17.01%	2.074%
13	9.869	1127	1136	1145	rBV	1602605	2566590	12.81%	1.562%
14	10.004	1153	1159	1168	rBV	36831	73022	0.36%	0.044%
15	10.404	1218	1227	1243	rBV	2380295	3904876	19.49%	2.376%
16	10.793	1284	1293	1303	rBV	3156157	5354932	26.72%	3.259%
17	10.928	1307	1316	1327	rBV	1728377	3001117	14.98%	1.826%
18	11.575	1418	1426	1434	rBV2	146773	266209	1.33%	0.162%
19	12.375	1556	1562	1568	rVB2	57434	93138	0.46%	0.057%
20	13.222	1702	1706	1714	rVB8	12715	25037	0.12%	0.015%
21	13.504	1749	1754	1759	rBV	44197	71207	0.36%	0.043%
22	13.587	1761	1768	1774	rVB6	12984	30513	0.15%	0.019%
23	14.022	1835	1842	1855	rVV	6322095	8531868	42.58%	5.192%
24	14.251	1874	1881	1884	rBV9	12982	23573	0.12%	0.014%
25	14.310	1884	1891	1905	rVV	6626337	9443650	47.13%	5.747%
26	14.616	1936	1943	1953	rBV	5308235	7838791	39.12%	4.770%
27	14.804	1968	1975	1991	rBV	379889	656274	3.28%	0.399%
28	15.028	2007	2013	2021	rVB6	50202	88671	0.44%	0.054%
29	15.404	2073	2077	2085	rBV2	47705	82463	0.41%	0.050%
30	15.610	2103	2112	2125	rBV	9544727	13540228	67.57%	8.240%
31	15.722	2125	2131	2147	rVV	3093478	4155561	20.74%	2.529%
32	15.845	2147	2152	2158	rVB2	44037	76648	0.38%	0.047%
33	15.969	2169	2173	2177	rVB5	18874	22005	0.11%	0.013%
34	17.045	2352	2356	2361	rBV7	12948	23228	0.12%	0.014%
35	17.157	2371	2375	2382	rVB4	16112	31234	0.16%	0.019%
36	17.275	2392	2395	2400	rVB6	17179	21802	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012989.D
 Acq On : 08 Dec 2022 17:40
 Operator : CG/JU
 Sample : N5894-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.369	2403	2411	2421	rBV	7155884	9849861	49.16%	5.994%
38	17.469	2421	2428	2440	rVV2	11288951	16395178	81.82%	9.977%
39	17.557	2440	2443	2452	rVV4	71307	138146	0.69%	0.084%
40	17.651	2455	2459	2468	rVB	42884	72422	0.36%	0.044%
41	17.745	2472	2475	2481	rBV5	15573	24686	0.12%	0.015%
42	18.027	2519	2523	2528	rVB5	71044	91861	0.46%	0.056%
43	18.233	2554	2558	2565	rBV2	111593	153983	0.77%	0.094%
44	18.316	2568	2572	2579	rVB	101798	133592	0.67%	0.081%
45	19.063	2696	2699	2704	rBV3	78888	90723	0.45%	0.055%
46	19.274	2731	2735	2740	rBV	152165	211113	1.05%	0.128%
47	19.345	2742	2747	2751	rBV	154092	245979	1.23%	0.150%
48	19.469	2765	2768	2772	rBV5	41098	47596	0.24%	0.029%
49	19.616	2790	2793	2796	rVB3	40961	43861	0.22%	0.027%
50	19.698	2801	2807	2822	rBV	15304528	20038323	100.00%	12.194%
51	21.139	3050	3052	3059	rBV3	106057	150909	0.75%	0.092%
52	21.451	3100	3105	3114	rBV	7439417	10520358	52.50%	6.402%
53	23.786	3494	3502	3516	rVB2	9417414	19729883	98.46%	12.006%
54	23.945	3522	3529	3541	rVB2	5137099	10499917	52.40%	6.390%




Sum of corrected areas: 164327125

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012989.D
Acq On : 08 Dec 2022 17:40
Operator : CG/JU
Sample : N5894-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

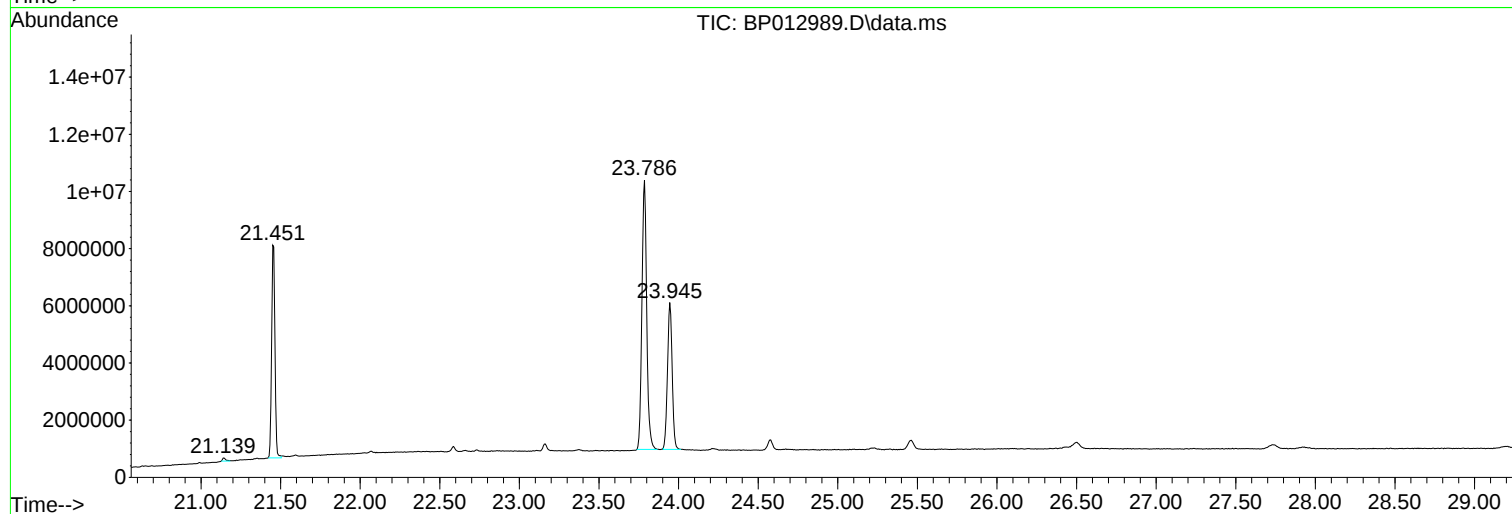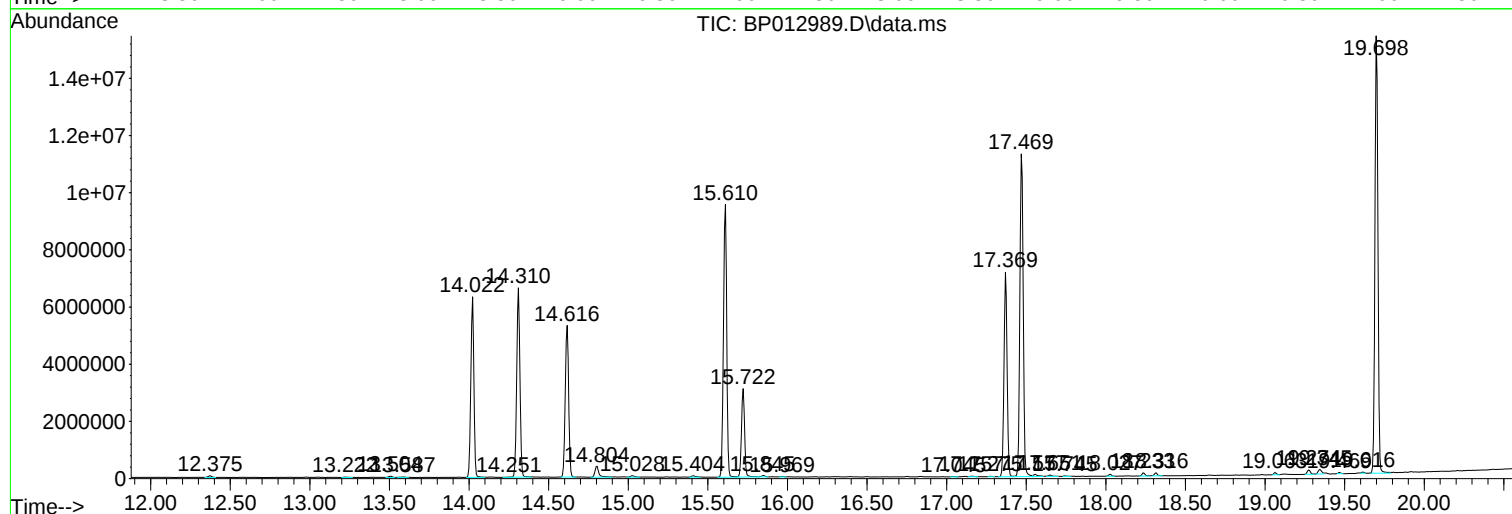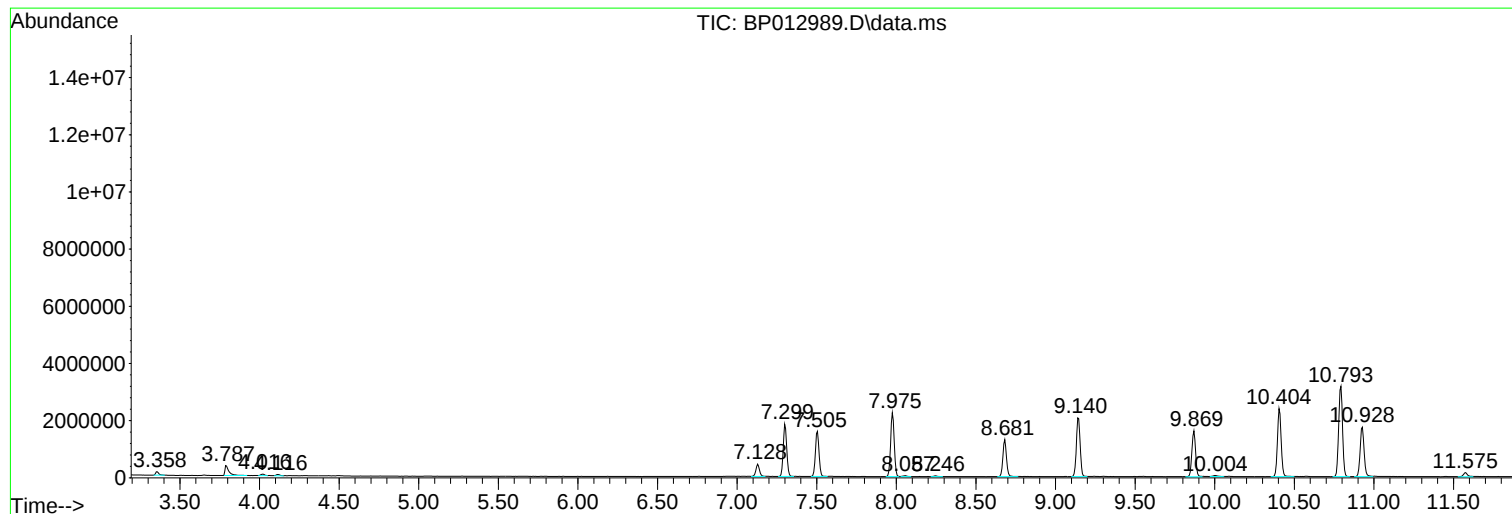

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012989.D
Acq On : 08 Dec 2022 17:40
Operator : CG/JU
Sample : N5894-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012989.D
Acq On : 08 Dec 2022 17:40
Operator : CG/JU
Sample : N5894-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc