

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012990.D
 Acq On : 08 Dec 2022 18:14
 Operator : CG/JU
 Sample : N5894-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	39	rVB	119196	176587	0.89%	0.108%
2	3.793	101	103	117	rBV	240588	423629	2.14%	0.258%
3	4.016	136	141	148	rBV	66556	109139	0.55%	0.067%
4	4.116	154	158	163	rVB	41131	57401	0.29%	0.035%
5	4.493	220	222	229	rVB7	15785	26850	0.14%	0.016%
6	7.128	663	670	682	rBV	559717	864974	4.37%	0.527%
7	7.299	692	699	711	rBV	1979512	3058832	15.45%	1.865%
8	7.505	727	734	743	rBV	1771555	2788431	14.09%	1.700%
9	7.975	807	814	821	rBV	2215406	3416187	17.26%	2.083%
10	8.052	823	827	832	rVB	25301	44320	0.22%	0.027%
11	8.246	855	860	865	rVB	22543	37577	0.19%	0.023%
12	8.681	926	934	945	rBV	1555540	2408133	12.17%	1.468%
13	9.140	1004	1012	1023	rBV	2275653	3691817	18.65%	2.251%
14	9.546	1078	1081	1087	rVB6	12301	19808	0.10%	0.012%
15	9.869	1126	1136	1151	rBV	1716787	2819236	14.24%	1.719%
16	10.004	1151	1159	1164	rBV6	16052	35454	0.18%	0.022%
17	10.404	1220	1227	1243	rBV	2527127	4188940	21.16%	2.554%
18	10.793	1284	1293	1300	rBV	3100802	5162749	26.08%	3.147%
19	10.928	1308	1316	1328	rBV	1701648	2973848	15.03%	1.813%
20	11.569	1419	1425	1435	rBV2	61900	117981	0.60%	0.072%
21	12.375	1554	1562	1566	rBV2	55558	91645	0.46%	0.056%
22	13.234	1700	1708	1713	rBV10	8442	21067	0.11%	0.013%
23	13.504	1749	1754	1759	rBV4	30009	46983	0.24%	0.029%
24	13.581	1759	1767	1775	rVB9	18604	40765	0.21%	0.025%
25	13.934	1820	1827	1832	rBV10	9945	22885	0.12%	0.014%
26	14.022	1835	1842	1852	rBV	6412323	8619530	43.55%	5.255%
27	14.251	1876	1881	1884	rBV5	16765	24530	0.12%	0.015%
28	14.310	1884	1891	1903	rVV	6983118	9883484	49.94%	6.025%
29	14.616	1936	1943	1952	rVB	5197954	7497847	37.88%	4.571%
30	14.804	1968	1975	1989	rBV	451340	796156	4.02%	0.485%
31	15.028	2007	2013	2021	rVB6	70761	130294	0.66%	0.079%
32	15.410	2073	2078	2084	rBV2	67548	102046	0.52%	0.062%
33	15.610	2103	2112	2122	rBV	9431881	13583577	68.63%	8.281%
34	15.722	2124	2131	2143	rVV	3160414	4029680	20.36%	2.457%
35	15.845	2148	2152	2159	rVB3	46271	80655	0.41%	0.049%
36	16.392	2239	2245	2250	rVB4	14139	21516	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012990.D
 Acq On : 08 Dec 2022 18:14
 Operator : CG/JU
 Sample : N5894-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	16.751	2303	2306	2313	rVB8	15588	25032	0.13%	0.015%
38	17.116	2362	2368	2371	rBV6	23330	41259	0.21%	0.025%
39	17.151	2371	2374	2384	rVB4	21066	44265	0.22%	0.027%
40	17.275	2393	2395	2399	rVB5	22935	26022	0.13%	0.016%
41	17.369	2404	2411	2421	rBV	6756949	9434968	47.67%	5.752%
42	17.469	2422	2428	2440	rVV	11084802	15823499	79.95%	9.646%
43	17.557	2440	2443	2446	rVB4	27482	37080	0.19%	0.023%
44	17.651	2455	2459	2469	rVB	45632	79327	0.40%	0.048%
45	18.027	2519	2523	2527	rVB2	58922	72849	0.37%	0.044%
46	18.239	2554	2559	2567	rBV	454879	611887	3.09%	0.373%
47	18.316	2568	2572	2576	rVB	52168	71919	0.36%	0.044%
48	19.063	2695	2699	2703	rBV3	86484	104950	0.53%	0.064%
49	19.274	2731	2735	2739	rBV2	165976	221315	1.12%	0.135%
50	19.345	2742	2747	2751	rBV	154888	235489	1.19%	0.144%
51	19.469	2764	2768	2775	rBV	314898	404954	2.05%	0.247%
52	19.698	2801	2807	2820	rBV	14918038	19792580	100.00%	12.066%
53	21.457	3100	3106	3114	rBV	7202364	10205632	51.56%	6.222%
54	23.786	3494	3502	3516	rVB2	9048007	19344107	97.73%	11.793%
55	23.945	3522	3529	3541	rVB2	4779802	10044345	50.75%	6.123%




Sum of corrected areas: 164036032

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012990.D
Acq On : 08 Dec 2022 18:14
Operator : CG/JU
Sample : N5894-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

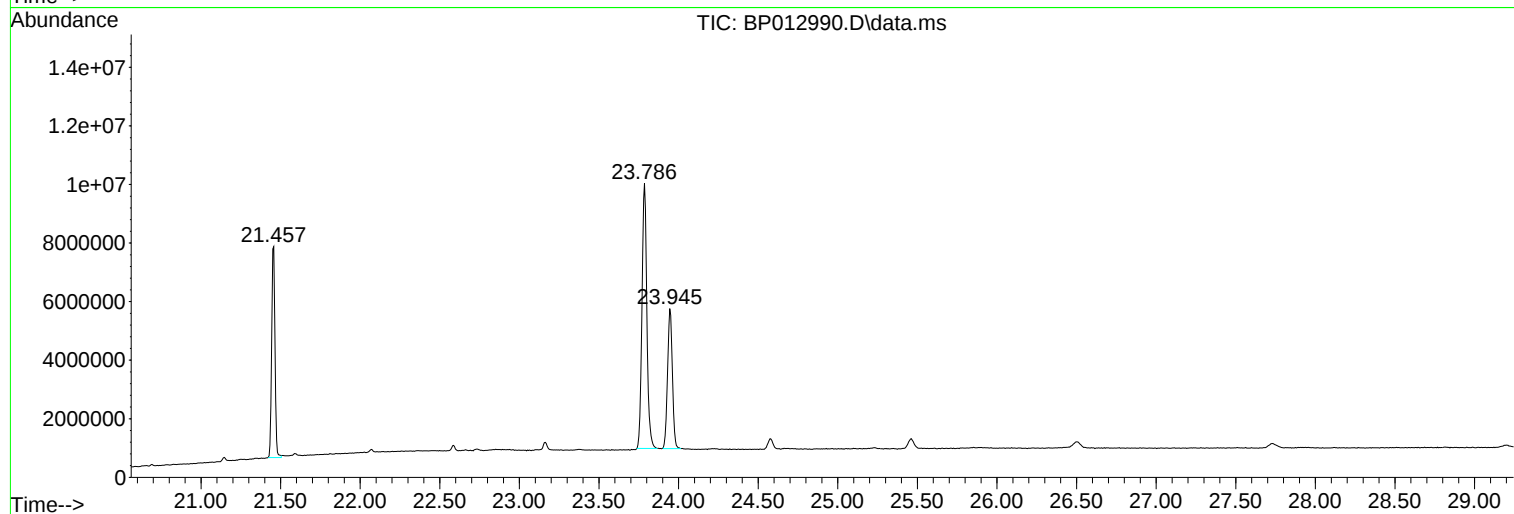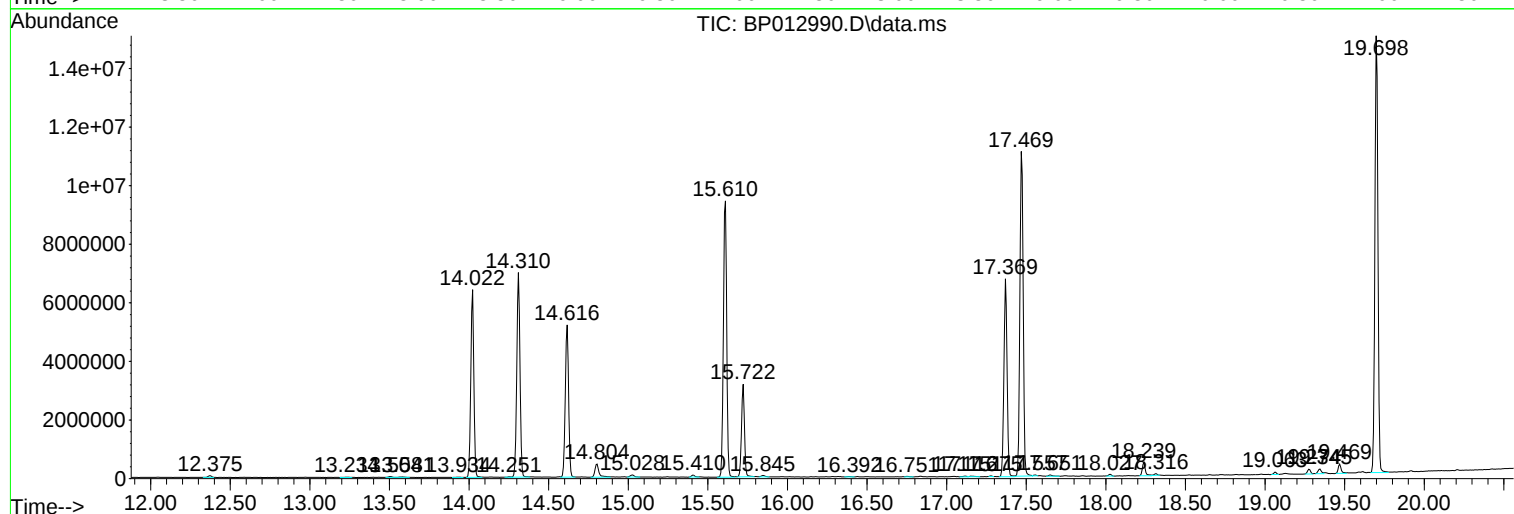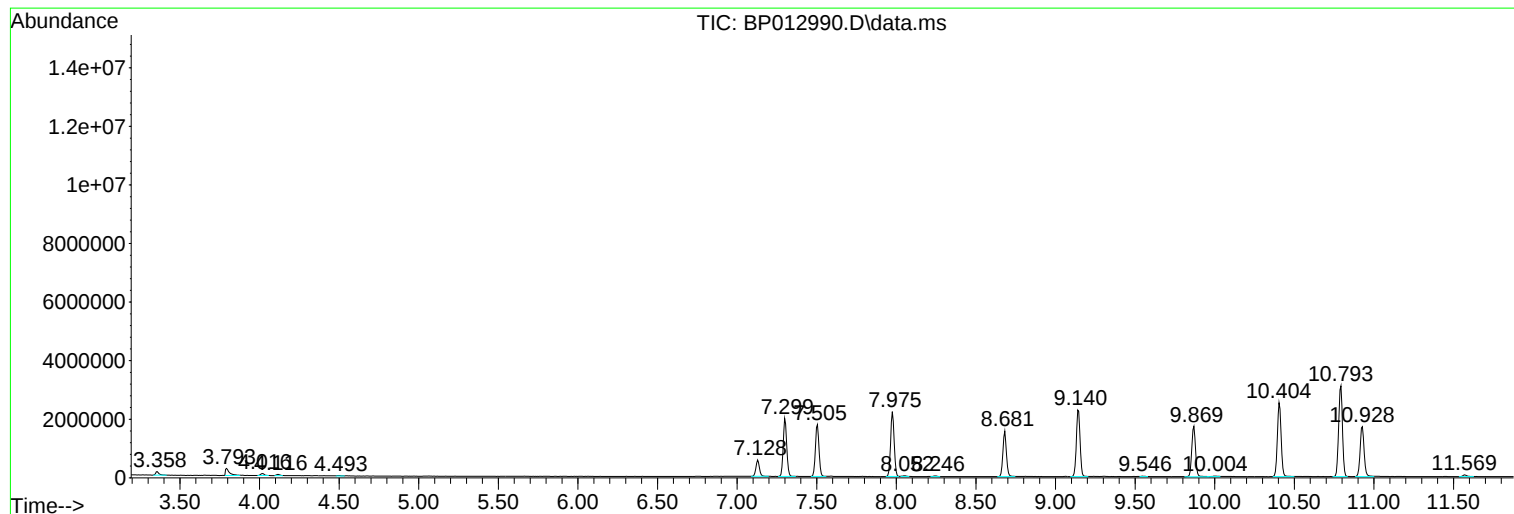

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012990.D
Acq On : 08 Dec 2022 18:14
Operator : CG/JU
Sample : N5894-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012990.D
Acq On : 08 Dec 2022 18:14
Operator : CG/JU
Sample : N5894-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
