

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012994.D
 Acq On : 08 Dec 2022 20:31
 Operator : CG/JU
 Sample : N5894-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	39	rVB	125288	184000	0.91%	0.109%
2	3.793	100	103	120	rBV	276403	490665	2.43%	0.290%
3	4.017	137	141	146	rVB	65204	91492	0.45%	0.054%
4	4.117	154	158	167	rVB	64110	95585	0.47%	0.057%
5	5.064	314	319	327	rVB5	12582	28287	0.14%	0.017%
6	7.128	661	670	679	rBV	539929	810176	4.02%	0.479%
7	7.299	692	699	708	rBV	2099249	3209277	15.93%	1.898%
8	7.505	725	734	743	rBV	1628087	2604694	12.93%	1.540%
9	7.975	806	814	822	rBV	2256812	3528039	17.51%	2.086%
10	8.681	924	934	942	rBV	1451081	2267253	11.25%	1.341%
11	9.140	1005	1012	1022	rBV	2410456	3946750	19.59%	2.334%
12	9.869	1127	1136	1148	rVB	1646931	2733523	13.57%	1.616%
13	9.999	1152	1158	1169	rBV	36717	77715	0.39%	0.046%
14	10.404	1219	1227	1237	rBV	2463534	4058528	20.14%	2.400%
15	10.787	1283	1292	1303	rBV	3117050	5322728	26.41%	3.148%
16	10.922	1307	1315	1329	rBV	1766413	3108724	15.43%	1.838%
17	11.446	1397	1404	1410	rVB	31267	54219	0.27%	0.032%
18	11.569	1419	1425	1437	rBV3	100391	194797	0.97%	0.115%
19	11.799	1459	1464	1469	rVB7	13399	23645	0.12%	0.014%
20	12.040	1499	1505	1510	rBV	159311	241384	1.20%	0.143%
21	12.098	1510	1515	1524	rVB2	148095	257765	1.28%	0.152%
22	12.369	1555	1561	1569	rVB	66419	107716	0.53%	0.064%
23	12.575	1589	1596	1601	rBV2	34201	55095	0.27%	0.033%
24	13.028	1669	1673	1680	rVB8	10366	20797	0.10%	0.012%
25	13.151	1686	1694	1703	rBV	189228	300278	1.49%	0.178%
26	13.510	1747	1755	1760	rBV2	64076	121021	0.60%	0.072%
27	13.569	1760	1765	1775	rVB4	47602	85239	0.42%	0.050%
28	13.740	1791	1794	1800	rBV7	14201	24450	0.12%	0.014%
29	13.898	1815	1821	1824	rBV8	11597	21956	0.11%	0.013%
30	14.022	1835	1842	1858	rBV	6378860	9010599	44.72%	5.328%
31	14.163	1863	1866	1873	rVB3	41379	56039	0.28%	0.033%
32	14.310	1884	1891	1900	rBV	7622863	10909239	54.14%	6.451%
33	14.569	1928	1935	1937	rBV3	115049	174185	0.86%	0.103%
34	14.616	1937	1943	1952	rVB2	5584947	8557905	42.47%	5.061%
35	14.798	1968	1974	1983	rBV	425748	687882	3.41%	0.407%
36	15.028	2008	2013	2018	rVB4	64588	105094	0.52%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012994.D
 Acq On : 08 Dec 2022 20:31
 Operator : CG/JU
 Sample : N5894-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	15.404	2072	2077	2088	rVB2	77501	141723	0.70%	0.084%
38	15.610	2103	2112	2118	rBV	9874811	14617258	72.54%	8.644%
39	15.722	2124	2131	2143	rBV	2780148	3800204	18.86%	2.247%
40	15.845	2146	2152	2156	rVV2	47106	64897	0.32%	0.038%
41	16.304	2226	2230	2237	rVB10	10256	21471	0.11%	0.013%
42	16.369	2237	2241	2243	rBV2	17941	24084	0.12%	0.014%
43	16.839	2316	2321	2324	rBV3	16289	28132	0.14%	0.017%
44	16.957	2336	2341	2343	rBV2	20892	28598	0.14%	0.017%
45	16.986	2343	2346	2352	rVV3	22273	34451	0.17%	0.020%
46	17.039	2352	2355	2363	rVB7	16317	27531	0.14%	0.016%
47	17.157	2371	2375	2383	rVB3	14120	26785	0.13%	0.016%
48	17.369	2404	2411	2421	rBV	6800959	9510220	47.20%	5.624%
49	17.469	2421	2428	2440	rVV	11768275	16680486	82.78%	9.864%
50	17.557	2440	2443	2445	rVV3	36153	49847	0.25%	0.029%
51	17.586	2445	2448	2455	rVB	43022	56484	0.28%	0.033%
52	17.651	2455	2459	2461	rBV	22453	29088	0.14%	0.017%
53	17.833	2487	2490	2494	rBV4	12356	21265	0.11%	0.013%
54	18.028	2519	2523	2530	rBV5	48706	67101	0.33%	0.040%
55	18.210	2550	2554	2556	rBV3	66231	84657	0.42%	0.050%
56	18.233	2556	2558	2561	rVV	104689	117413	0.58%	0.069%
57	18.269	2561	2564	2567	rVV2	57858	69111	0.34%	0.041%
58	18.310	2569	2571	2577	rVB2	15186	23606	0.12%	0.014%
59	18.439	2589	2593	2598	rBV	113492	155975	0.77%	0.092%
60	18.486	2599	2601	2605	rVV4	30905	40869	0.20%	0.024%
61	18.522	2605	2607	2613	rVB6	21392	31453	0.16%	0.019%
62	18.739	2641	2644	2649	rVB5	31365	41829	0.21%	0.025%
63	19.063	2696	2699	2704	rBV4	51062	58163	0.29%	0.034%
64	19.275	2731	2735	2740	rVB	158033	210041	1.04%	0.124%
65	19.339	2742	2746	2751	rBV	157636	220033	1.09%	0.130%
66	19.463	2765	2767	2776	rVB7	44229	59057	0.29%	0.035%
67	19.610	2790	2792	2795	rBV3	27474	31920	0.16%	0.019%
68	19.698	2801	2807	2818	rBV	15456655	20150531	100.00%	11.916%
69	21.451	3100	3105	3112	rBV	7559680	9999322	49.62%	5.913%
70	23.780	3493	3501	3516	rBV2	9022553	19281370	95.69%	11.402%
71	23.939	3521	3528	3541	rVB2	4868440	9730737	48.29%	5.754%




Sum of corrected areas: 169102453

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012994.D
Acq On : 08 Dec 2022 20:31
Operator : CG/JU
Sample : N5894-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

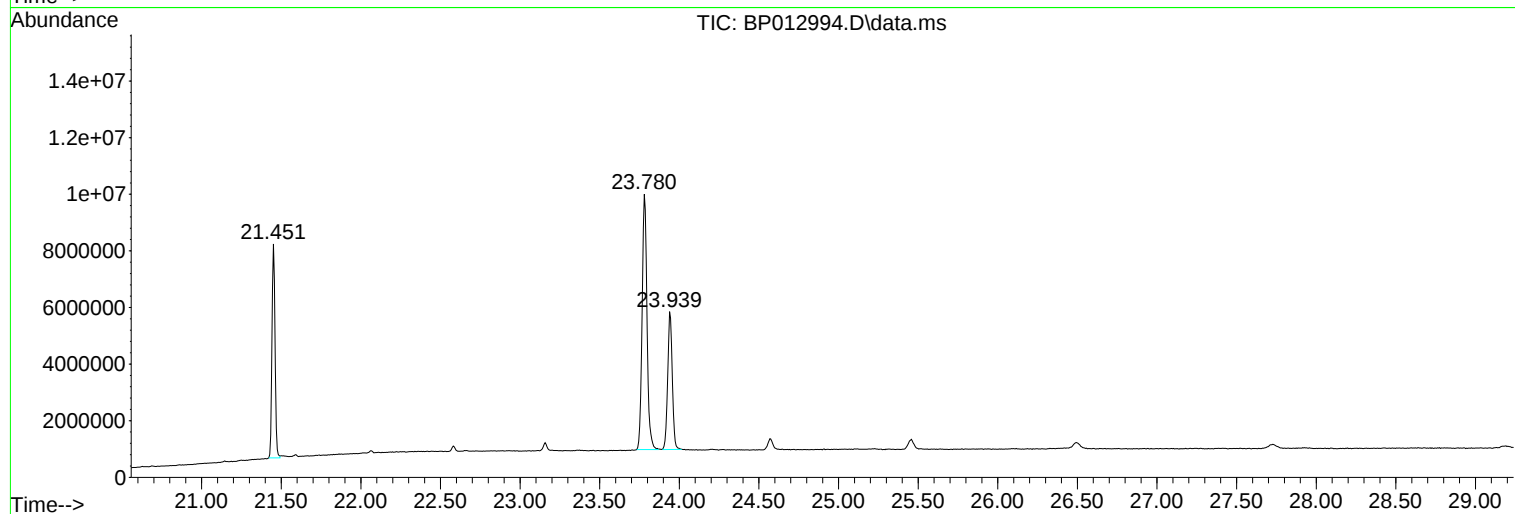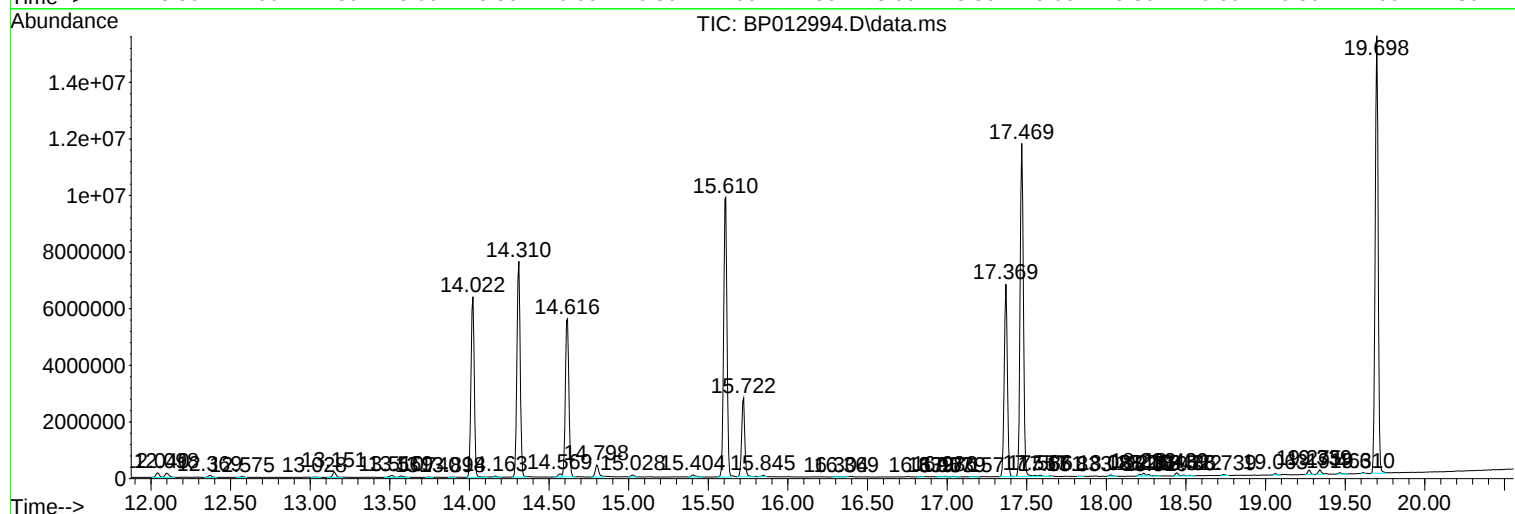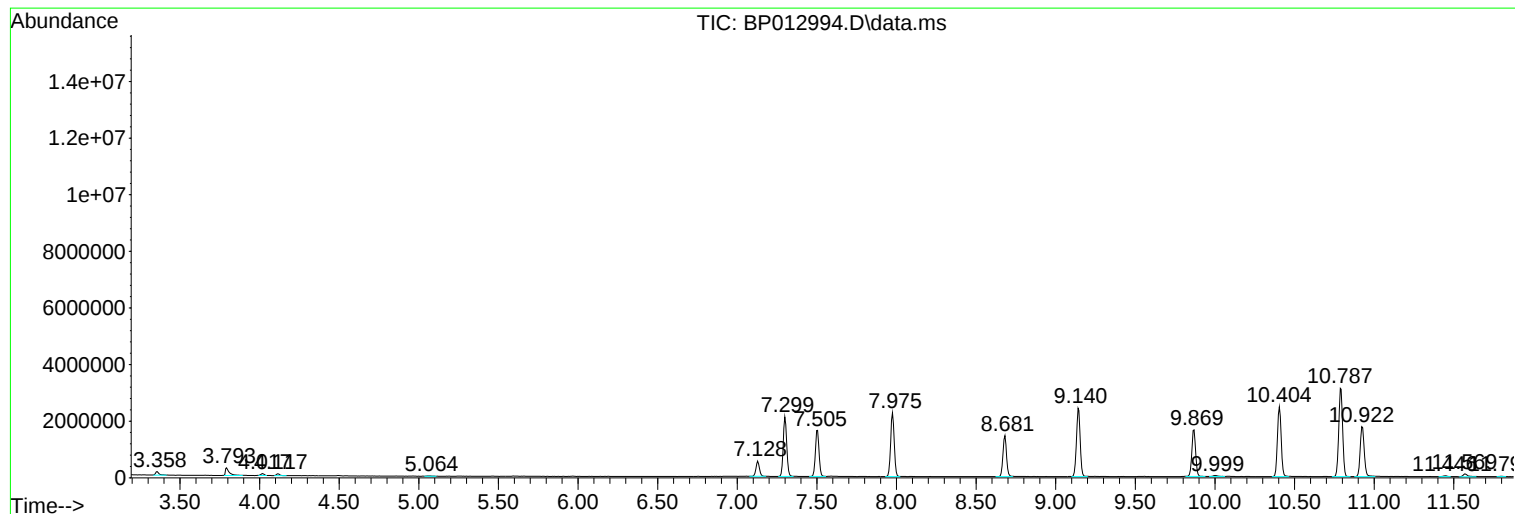

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012994.D
Acq On : 08 Dec 2022 20:31
Operator : CG/JU
Sample : N5894-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012994.D
Acq On : 08 Dec 2022 20:31
Operator : CG/JU
Sample : N5894-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc