

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
 Data File : BP012995.D
 Acq On : 08 Dec 2022 21:05
 Operator : CG/JU
 Sample : N5894-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	36	rVB	129424	183870	0.25%	0.058%
2	3.787	99	102	122	rBV	499055	839873	1.13%	0.267%
3	4.017	136	141	147	rVB	59977	96414	0.13%	0.031%
4	4.117	153	158	164	rBV	56427	86791	0.12%	0.028%
5	5.270	346	354	369	rBV2	32110093	74457127	100.00%	23.678%
6	7.128	664	670	684	rVB2	563190	1263185	1.70%	0.402%
7	7.299	692	699	711	rBV	2622635	4065366	5.46%	1.293%
8	7.505	726	734	745	rBV	1690993	2955365	3.97%	0.940%
9	7.693	759	766	773	rVB	98466	161510	0.22%	0.051%
10	7.864	787	795	802	rBV	938080	1464580	1.97%	0.466%
11	8.016	807	821	834	rBV	21223918	40149557	53.92%	12.768%
12	8.334	866	875	892	rBV	19742676	34834865	46.79%	11.078%
13	8.681	927	934	943	rBV	1418607	2269599	3.05%	0.722%
14	9.140	1005	1012	1021	rBV	2474511	3983060	5.35%	1.267%
15	9.810	1120	1126	1129	rBV	74244	122391	0.16%	0.039%
16	9.869	1129	1136	1145	rVB	1611850	2701697	3.63%	0.859%
17	9.999	1153	1158	1168	rBV	39160	85003	0.11%	0.027%
18	10.405	1219	1227	1234	rBV	2489632	4099305	5.51%	1.304%
19	10.469	1234	1238	1246	rVB	55349	104913	0.14%	0.033%
20	10.652	1262	1269	1282	rBV3	275709	666629	0.90%	0.212%
21	10.787	1284	1292	1305	rBV	2754026	4698633	6.31%	1.494%
22	10.922	1305	1315	1327	rBV	2612562	4879986	6.55%	1.552%
23	11.569	1420	1425	1438	rBV	92855	180812	0.24%	0.058%
24	12.369	1556	1561	1568	rBV2	65643	103424	0.14%	0.033%
25	14.022	1834	1842	1852	rBV	6341449	8999402	12.09%	2.862%
26	14.310	1884	1891	1903	rBV	7223821	10670891	14.33%	3.393%
27	14.616	1936	1943	1952	rBV	4571983	6947498	9.33%	2.209%
28	14.798	1968	1974	1991	rBV	442107	761419	1.02%	0.242%
29	15.604	2104	2111	2119	rBV	9941110	14465297	19.43%	4.600%
30	15.722	2124	2131	2148	rVV	2839971	3890150	5.22%	1.237%
31	15.845	2148	2152	2158	rVB	51144	80360	0.11%	0.026%
32	17.369	2404	2411	2420	rBV	6256785	8723347	11.72%	2.774%
33	17.469	2421	2428	2440	rVV2	11751850	16651545	22.36%	5.295%
34	18.234	2554	2558	2563	rBV3	89238	120922	0.16%	0.038%
35	19.275	2731	2735	2739	rBV	159997	205172	0.28%	0.065%
36	19.339	2742	2746	2751	rBV	149261	217809	0.29%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012995.D
Acq On : 08 Dec 2022 21:05
Operator : CG/JU
Sample : N5894-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	19.698	2801	2807	2821	rBV	16030845	20298092	27.26%	6.455%
38	21.451	3100	3105	3112	rBV	6919575	9268793	12.45%	2.948%
39	23.780	3494	3501	3515	rVB2	9241427	19437023	26.10%	6.181%
40	23.945	3522	3529	3546	rVB	4443128	9263334	12.44%	2.946%




Sum of corrected areas: 314455009

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012995.D
Acq On : 08 Dec 2022 21:05
Operator : CG/JU
Sample : N5894-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

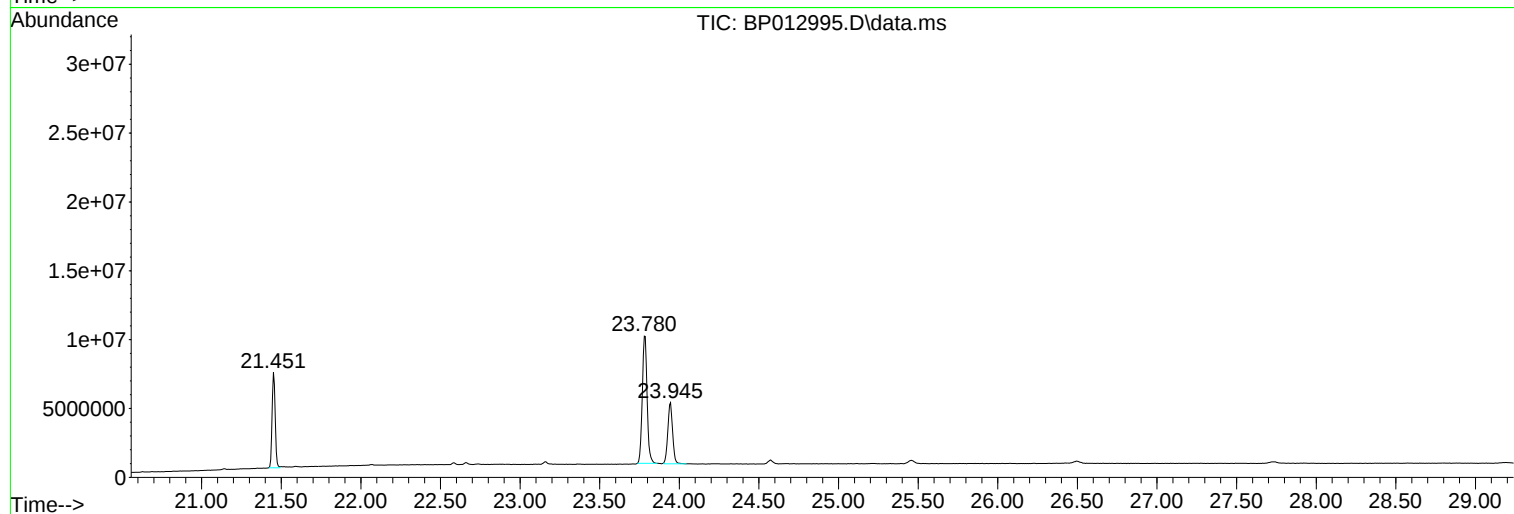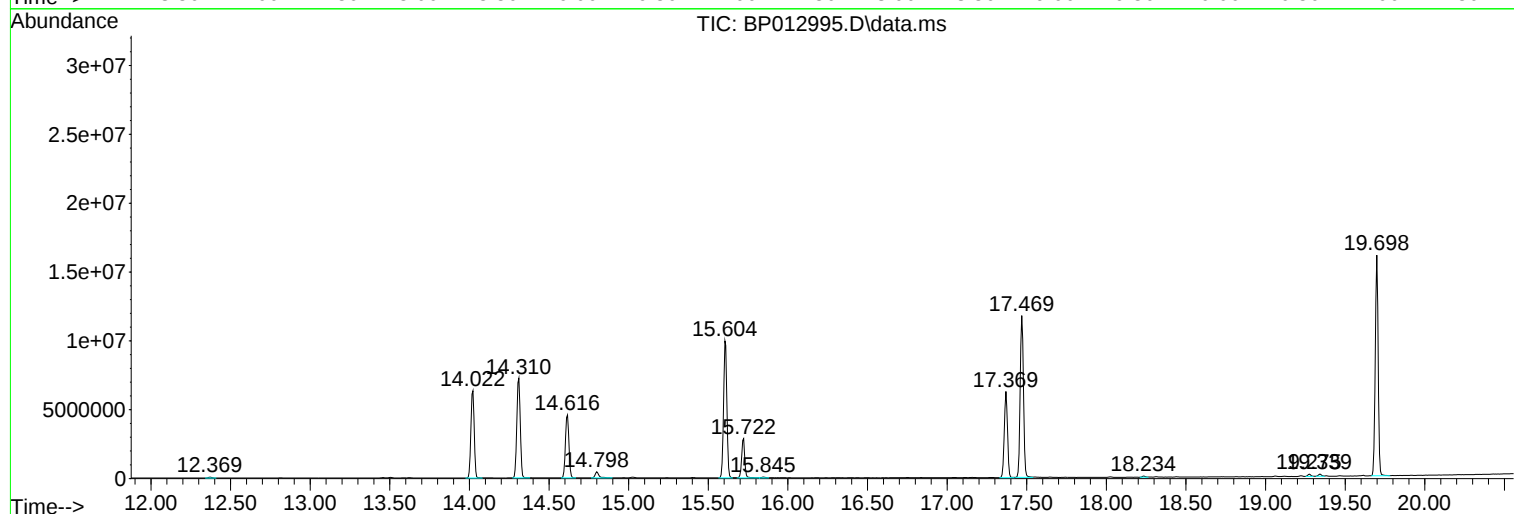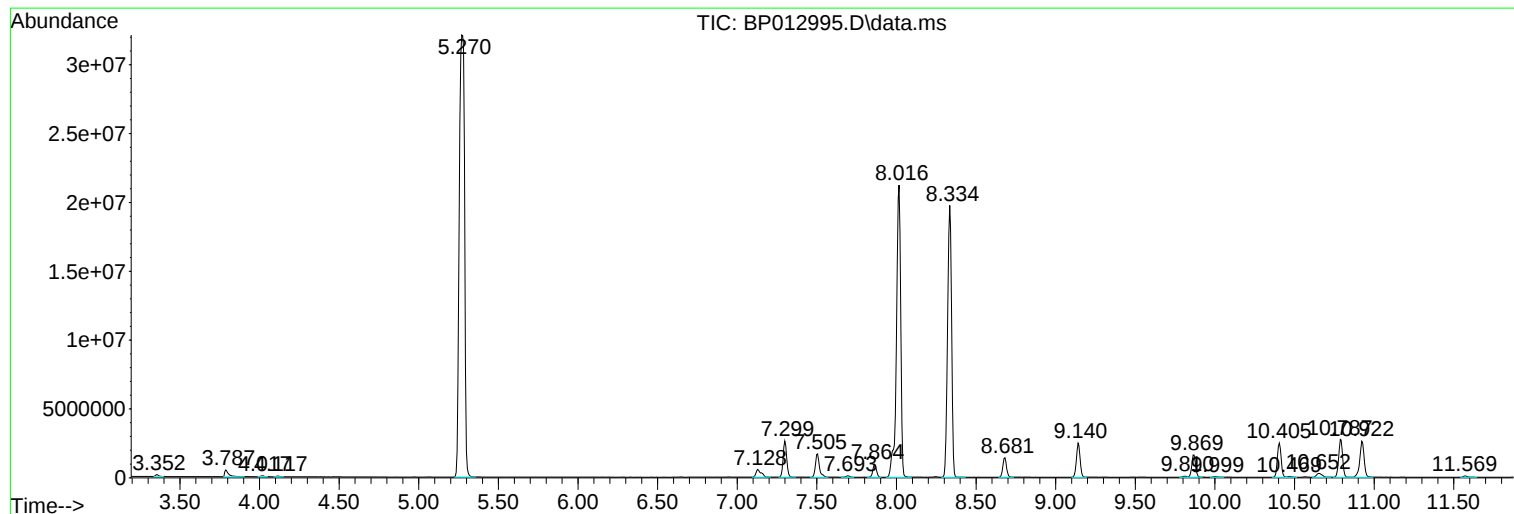

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012995.D
Acq On : 08 Dec 2022 21:05
Operator : CG/JU
Sample : N5894-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120822\
Data File : BP012995.D
Acq On : 08 Dec 2022 21:05
Operator : CG/JU
Sample : N5894-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc