




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023438.D
Acq On : 16 Dec 2024 17:49
Operator : RC/JU
Sample : PB165644BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK644

Manual IntegrationsAPPROVED

Quant Time: Dec 17 00:00:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

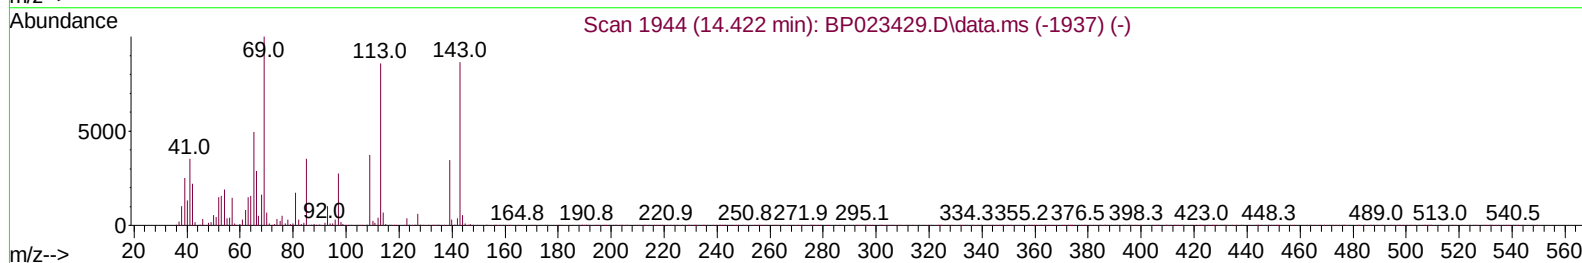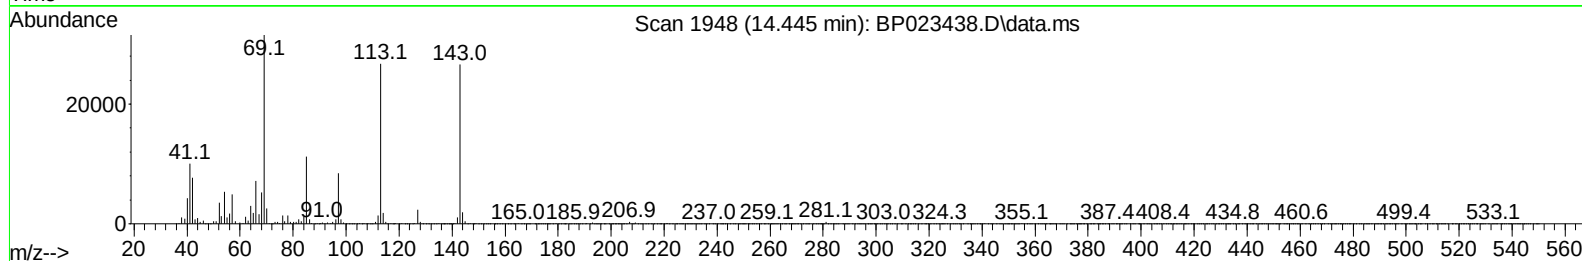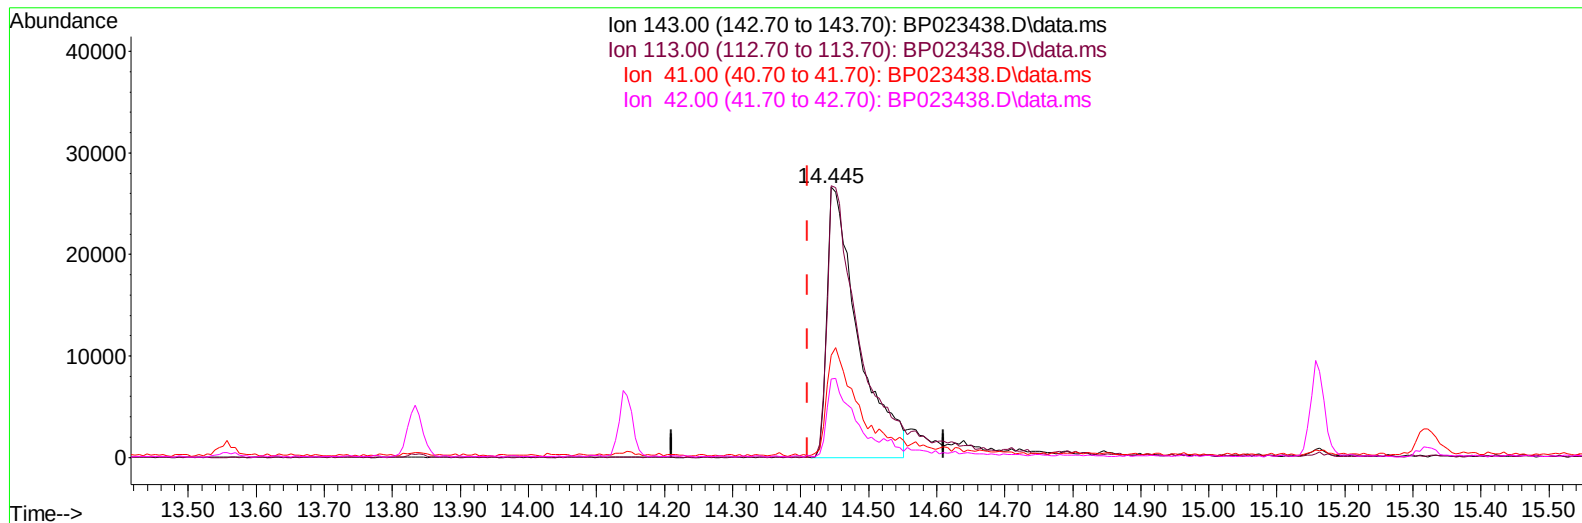

TIC: BP023438.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.445min (+ 0.035) 26.73 ng/ul

response 84182

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	100.48
41.00	45.60	37.92
42.00	31.70	29.03




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023438.D
Acq On : 16 Dec 2024 17:49
Operator : RC/JU
Sample : PB165644BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK644

Manual IntegrationsAPPROVED

Quant Time: Dec 17 00:00:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

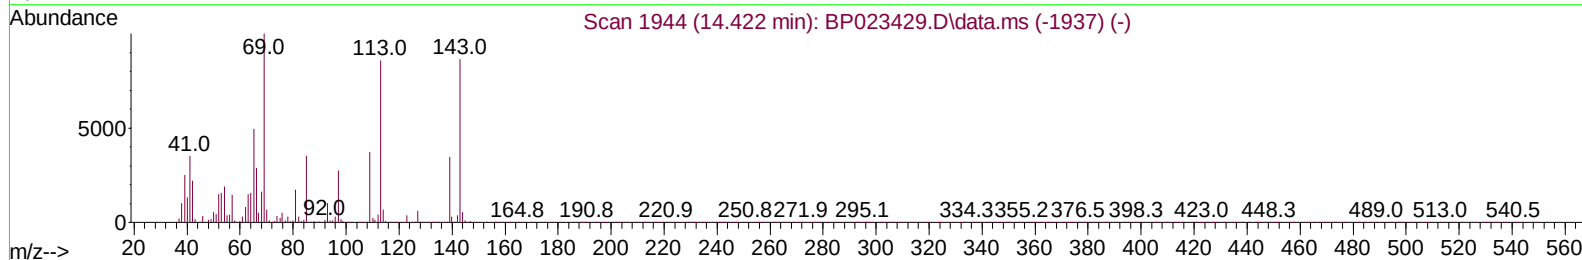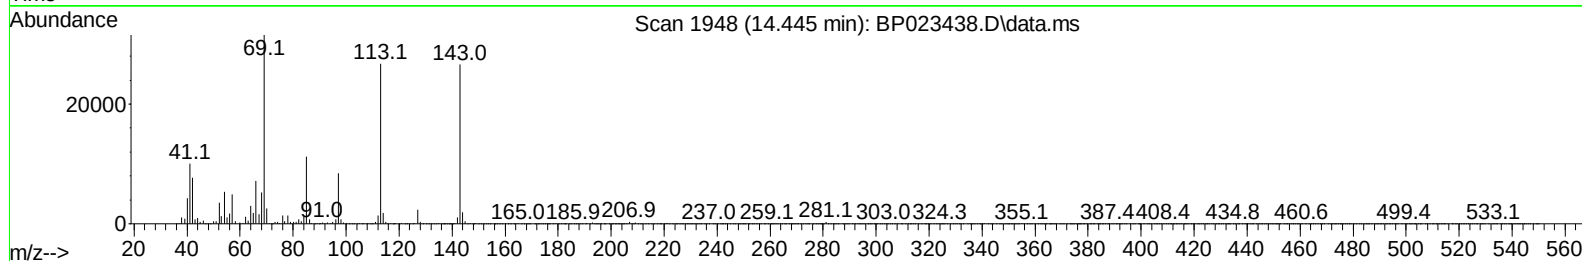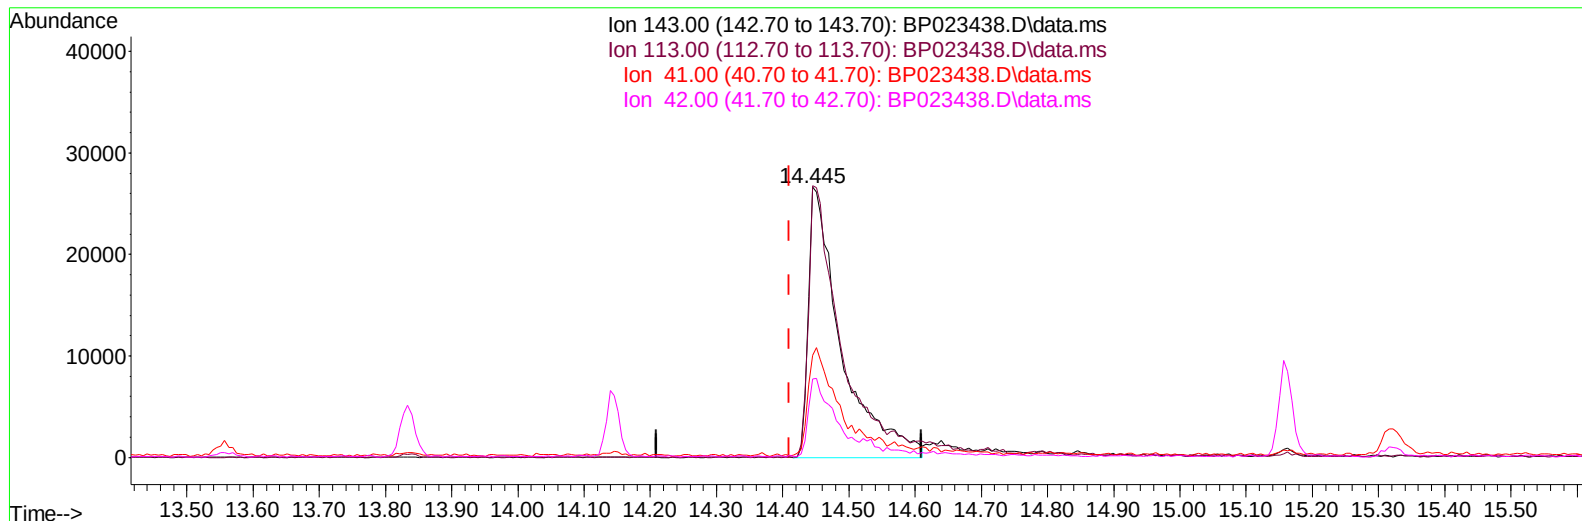

TIC: BP023438.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.445min (+ 0.035) 29.00 ng/ul m

response 91303

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	100.48
41.00	45.60	37.92
42.00	31.70	29.03

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
 Data File : BP023438.D
 Acq On : 16 Dec 2024 17:49
 Operator : RC/JU
 Sample : PB165644BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK644

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/19/2024

Quant Time: Dec 17 00:01:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	110733	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	412844	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.145	164	331009	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.957	188	804921	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	829520	20.000	ng/ul	0.00
88) Perylene-d12	24.545	264	923004	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	12566	4.178	ng/uL	0.00
4) Pyridine-d5	3.516	84	180056	23.280	ng/ul	0.00
7) Phenol-d5	6.757	99	232904	26.806	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.887	67	136449	24.892	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	173875	27.115	ng/ul	0.00
15) 4-Methylphenol-d8	8.257	113	189520	27.027	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	86030	27.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.393	143	99127	27.899	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	196861	26.252	ng/ul	0.01
31) 4-Chloroaniline-d4	10.434	131	217773	25.923	ng/ul	0.00
46) Dimethylphthalate-d6	13.557	166	676585	26.330	ng/ul	0.00
49) Acenaphthylene-d8	13.834	160	693746	25.596	ng/ul	0.00
54) 4-Nitrophenol-d4	14.445	143	91303m	28.995	ng/ul	0.04
60) Fluorene-d10	15.163	176	591277	26.161	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.322	200	83386	17.141	ng/ul	0.01
73) Anthracene-d10	17.057	188	1021352	27.803	ng/ul	0.00
81) Pyrene-d10	19.439	212	1291359	29.797	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.327	264	1243067	25.158	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023438.D
Acq On : 16 Dec 2024 17:49
Operator : RC/JU
Sample : PB165644BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK644

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

Quant Time: Dec 17 00:01:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

