




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023478.D
Acq On : 17 Dec 2024 22:57
Operator : RC/JU
Sample : P5258-15
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E28X8

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:34:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

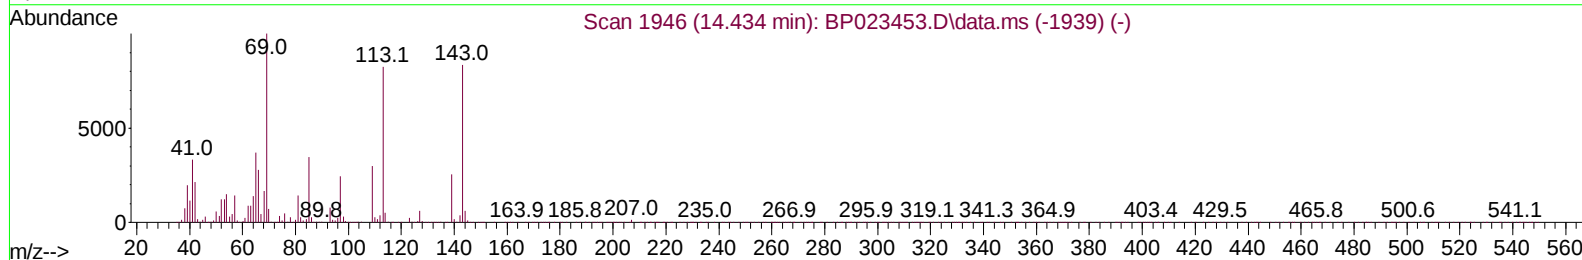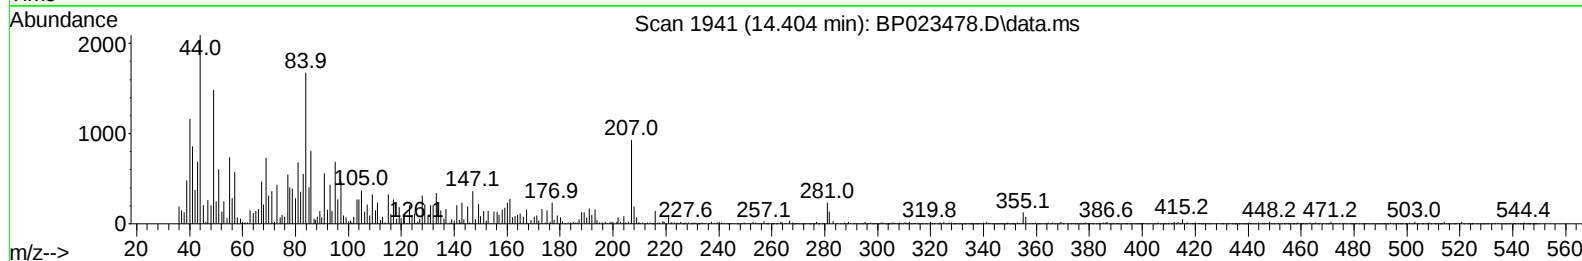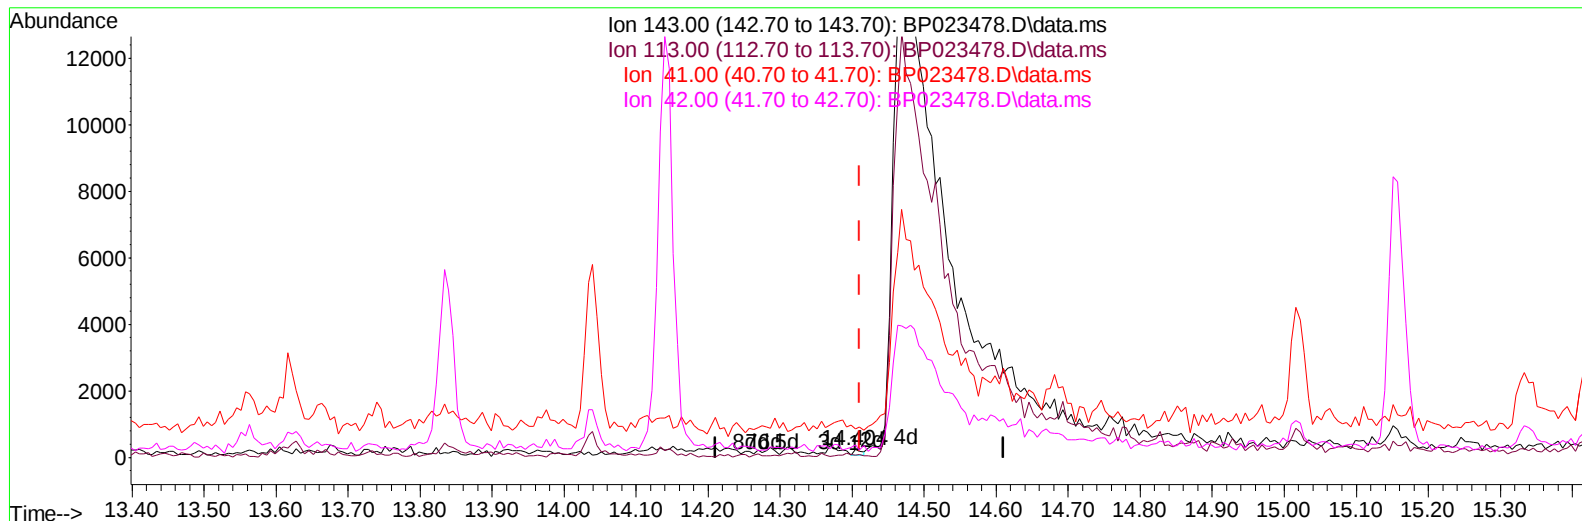

TIC: BP023478.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.404min (-0.006) 0.02 ng/u1

response 128

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	26.92#
41.00	45.60	300.70#
42.00	31.70	130.42#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023478.D
Acq On : 17 Dec 2024 22:57
Operator : RC/JU
Sample : P5258-15
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E28X8

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:34:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

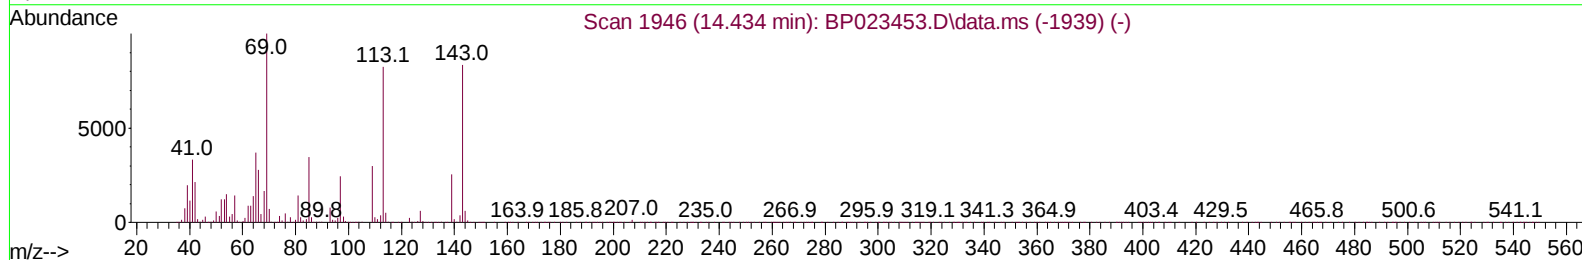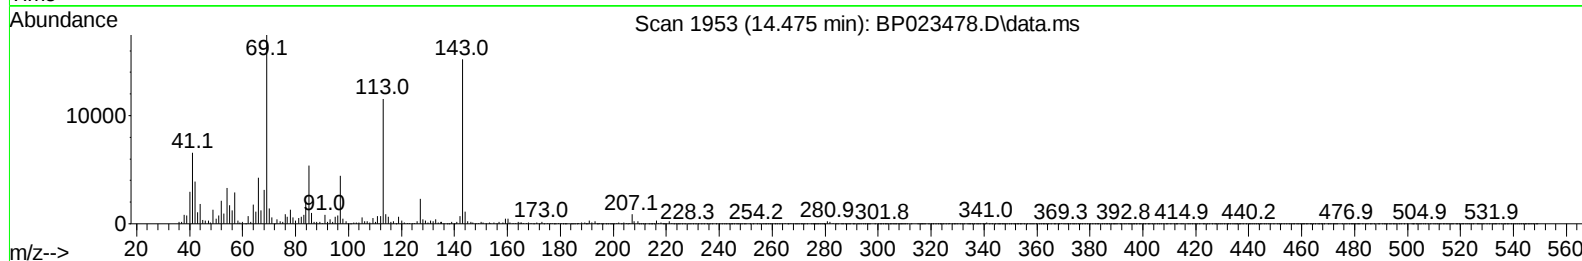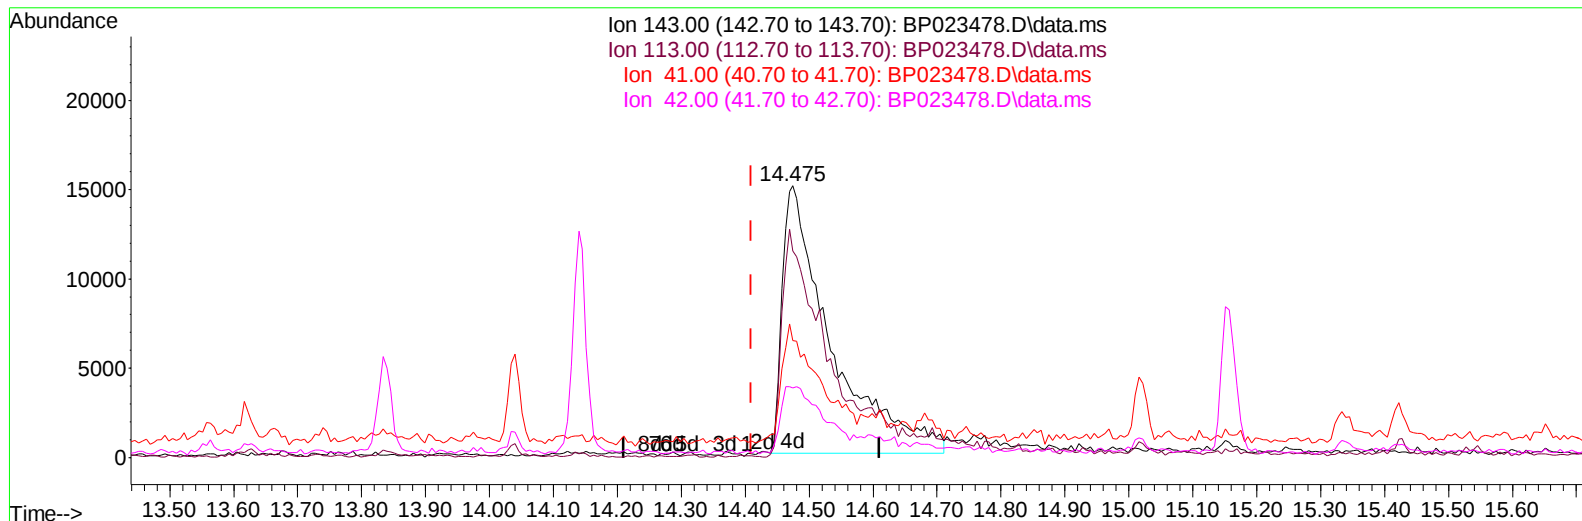

TIC: BP023478.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.475min (+ 0.065) 12.11 ng/ul m

response 79417

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	75.99#
41.00	45.60	43.08
42.00	31.70	25.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
 Data File : BP023478.D
 Acq On : 17 Dec 2024 22:57
 Operator : RC/JU
 Sample : P5258-15
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E28X8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/19/2024

Quant Time: Dec 18 00:35:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	255387	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.269	136	960461	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.145	164	689365	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.951	188	1513186	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	1670879	20.000	ng/ul	# 0.00
88) Perylene-d12	24.563	264	1782676	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	16486	2.377	ng/uL	0.00
4) Pyridine-d5	3.517	84	204408	11.459	ng/ul	0.00
7) Phenol-d5	6.752	99	260794	13.015	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.881	67	178756	14.139	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.081	132	194258	13.135	ng/ul	0.00
15) 4-Methylphenol-d8	8.258	113	207394	12.824	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	86651	12.082	ng/ul	0.00
24) 2-Nitrophenol-d4	9.387	143	107264	12.977	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.940	165	203987	11.693	ng/ul	0.00
31) 4-Chloroaniline-d4	10.446	131	201953	10.333	ng/ul	0.00
46) Dimethylphthalate-d6	13.563	166	681001	12.725	ng/ul	0.00
49) Acenaphthylene-d8	13.840	160	718583	12.730	ng/ul	0.00
54) 4-Nitrophenol-d4	14.475	143	79417m	12.110	ng/ul	0.06
60) Fluorene-d10	15.157	176	574641	12.208	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.334	200	40838	4.466	ng/ul	0.02
73) Anthracene-d10	17.057	188	956000	13.843	ng/ul	0.00
81) Pyrene-d10	19.439	212	1164895	13.344	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.339	264	1147618	12.026	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023478.D
Acq On : 17 Dec 2024 22:57
Operator : RC/JU
Sample : P5258-15
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E28X8

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:35:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/19/2024

