

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
 Data File : BP023430.D
 Acq On : 16 Dec 2024 11:05
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	25	rVB	33394	47137	1.47%	0.148%
2	3.511	85	89	104	rBV	325086	554455	17.34%	1.744%
3	3.816	137	141	146	rVB2	10702	14269	0.45%	0.045%
4	4.205	205	207	215	rVB10	2006	4255	0.13%	0.013%
5	5.452	418	419	425	rBV6	2343	3703	0.12%	0.012%
6	6.669	621	626	630	rBV3	6973	10506	0.33%	0.033%
7	6.746	633	639	657	rVV	394773	780794	24.42%	2.455%
8	6.881	657	662	674	rVB	376385	588660	18.41%	1.851%
9	7.081	688	696	716	rBV	459023	777459	24.32%	2.445%
10	7.528	764	772	782	rBV	402145	666485	20.84%	2.096%
11	8.246	887	894	916	rBV	462327	944121	29.53%	2.969%
12	8.675	960	967	976	rBV	433676	751546	23.50%	2.364%
13	9.057	1026	1032	1034	rBV7	2348	4023	0.13%	0.013%
14	9.381	1080	1087	1107	rBV	355745	683645	21.38%	2.150%
15	9.928	1172	1180	1202	rBV	445342	994944	31.12%	3.129%
16	10.269	1230	1238	1248	rBV	498826	861603	26.95%	2.710%
17	10.428	1255	1265	1287	rBV	404178	887515	27.76%	2.791%
18	10.604	1293	1295	1299	rVB5	3158	4620	0.14%	0.015%
19	11.875	1504	1511	1521	rVB7	6937	19022	0.59%	0.060%
20	13.104	1717	1720	1723	rBV5	2663	4290	0.13%	0.013%
21	13.545	1788	1795	1806	rBV	1110406	1598266	49.99%	5.026%
22	13.828	1836	1843	1860	rBV	1211960	1718653	53.75%	5.405%
23	14.145	1890	1897	1909	rBV	845121	1259817	39.40%	3.962%
24	14.439	1942	1947	1978	rBV	210353	708397	22.16%	2.228%
25	14.751	1995	2000	2006	rVB10	3548	7140	0.22%	0.022%
26	15.157	2062	2069	2085	rBV	1510245	2227413	69.66%	7.005%
27	15.304	2087	2094	2114	rBV2	377021	813448	25.44%	2.558%
28	15.675	2155	2157	2164	rVB7	2406	4360	0.14%	0.014%
29	15.869	2187	2190	2196	rBV8	2439	5086	0.16%	0.016%
30	15.951	2201	2204	2210	rVB7	3912	7285	0.23%	0.023%
31	16.275	2254	2259	2265	rVV10	3034	6314	0.20%	0.020%
32	16.363	2271	2274	2280	rVB8	2322	3526	0.11%	0.011%
33	16.616	2314	2317	2320	rVV5	3357	4173	0.13%	0.013%
34	16.733	2332	2337	2343	rVB5	5941	12569	0.39%	0.040%
35	16.945	2367	2373	2384	rBV2	1099217	1629858	50.97%	5.126%
36	17.051	2384	2391	2403	rVV	1764901	2552460	79.83%	8.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023430.D
Acq On : 16 Dec 2024 11:05
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Title : SVOA CALIBRATION

37	17.263	2423	2427	2431	rBV7	2083	4192	0.13%	0.013%
38	17.651	2488	2493	2496	rBV6	4685	7636	0.24%	0.024%
39	17.886	2528	2533	2541	rBV	53252	91740	2.87%	0.289%
40	18.975	2714	2718	2724	rBV3	21993	34105	1.07%	0.107%
41	19.069	2730	2734	2738	rBV2	18005	31696	0.99%	0.100%
42	19.227	2758	2761	2768	rBV5	27879	35409	1.11%	0.111%
43	19.439	2790	2797	2807	rBV	1800348	3092219	96.71%	9.725%
44	21.369	3119	3125	3134	rBV	1122733	1948739	60.95%	6.129%
45	22.551	3322	3326	3331	rVB3	69716	118202	3.70%	0.372%
46	24.310	3616	3625	3639	rVB	1259727	3197401	100.00%	10.055%
47	24.515	3652	3660	3682	rVB	696394	2074757	64.89%	6.525%




Sum of corrected areas: 31797913

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023430.D
Acq On : 16 Dec 2024 11:05
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

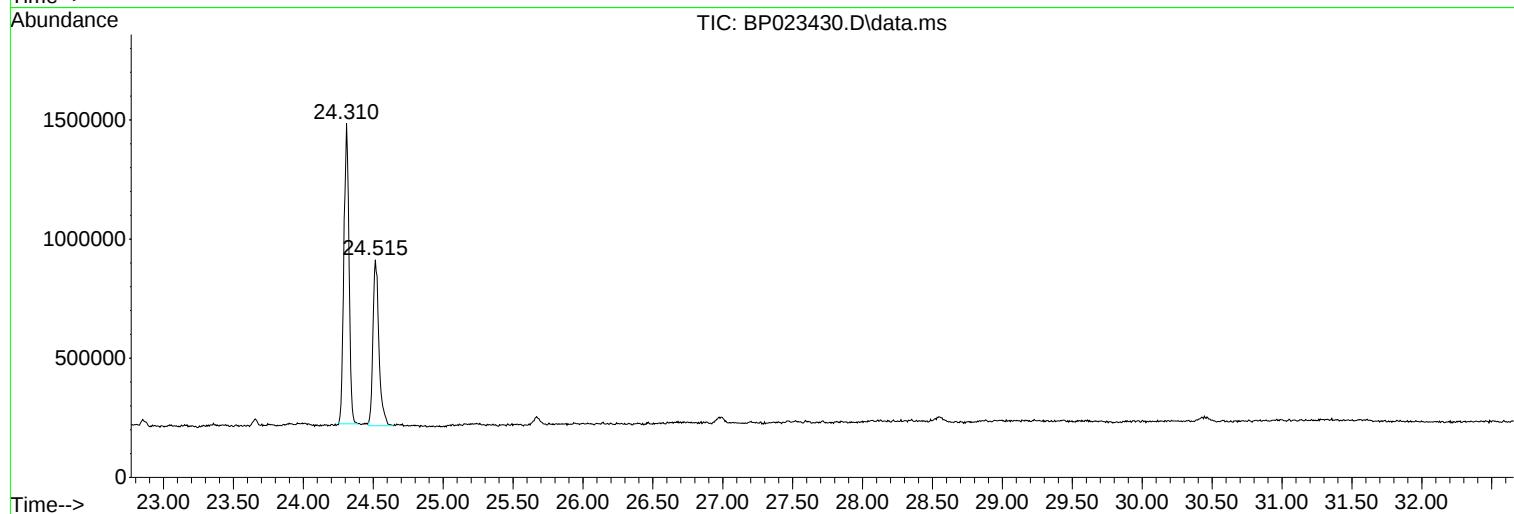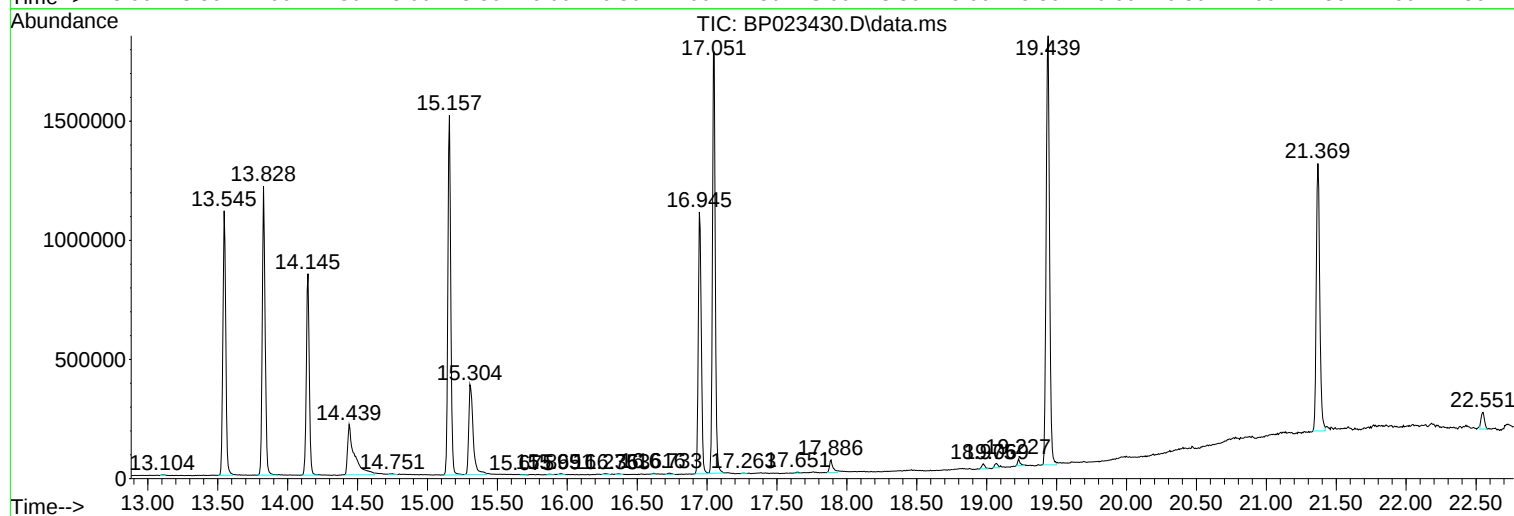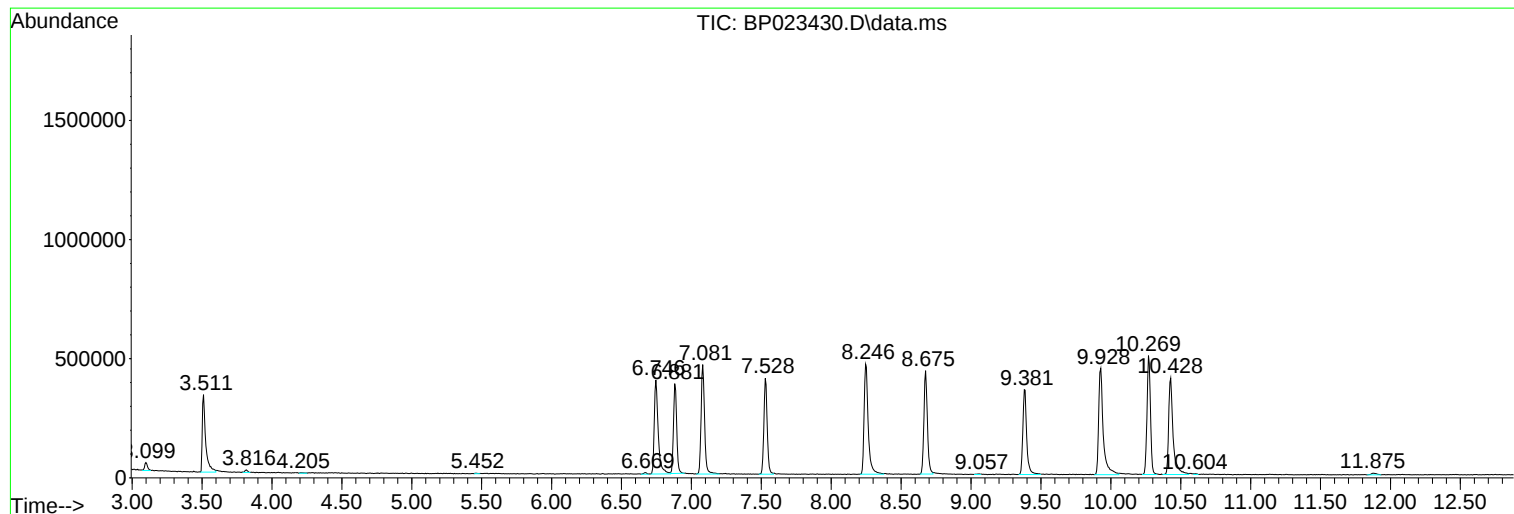

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023430.D
Acq On : 16 Dec 2024 11:05
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023430.D
Acq On : 16 Dec 2024 11:05
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc