

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
 Data File : BP023469.D
 Acq On : 17 Dec 2024 16:53
 Operator : RC/JU
 Sample : PB165621BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	26	rVB	58681	81965	1.49%	0.145%
2	3.511	86	89	103	rBV	627808	1037471	18.85%	1.841%
3	6.752	634	640	656	rBV	672103	1354529	24.61%	2.403%
4	6.881	657	662	678	rVB	666794	1037295	18.84%	1.840%
5	7.081	690	696	718	rVB	798778	1347456	24.48%	2.390%
6	7.528	765	772	788	rBV	804652	1379464	25.06%	2.447%
7	8.252	889	895	920	rBV	782596	1670810	30.35%	2.964%
8	8.675	960	967	986	rBV	719325	1267877	23.03%	2.249%
9	9.381	1081	1087	1106	rBV	541642	1072256	19.48%	1.902%
10	9.934	1174	1181	1206	rBV	711854	1718204	31.21%	3.048%
11	10.275	1231	1239	1249	rBV	1141122	1844204	33.50%	3.272%
12	10.434	1257	1266	1292	rBV	641026	1528636	27.77%	2.712%
13	11.875	1507	1511	1521	rBV4	8864	21480	0.39%	0.038%
14	13.116	1716	1722	1727	rBV10	3320	6408	0.12%	0.011%
15	13.557	1790	1797	1809	rBV	1775975	2499895	45.41%	4.435%
16	13.834	1835	1844	1865	rBV	1881989	3026288	54.97%	5.369%
17	14.145	1889	1897	1909	rBV	1812218	2769294	50.31%	4.913%
18	14.445	1941	1948	1958	rBV2	260621	831809	15.11%	1.476%
19	15.151	2060	2068	2086	rBV	2373002	3947794	71.71%	7.004%
20	15.322	2091	2097	2108	rBV	461670	860902	15.64%	1.527%
21	15.392	2108	2109	2118	rVB5	22154	33573	0.61%	0.060%
22	15.963	2201	2206	2210	rBV8	3755	7194	0.13%	0.013%
23	16.616	2312	2317	2320	rBV7	5900	11155	0.20%	0.020%
24	16.739	2331	2338	2344	rBV3	12590	26646	0.48%	0.047%
25	16.951	2367	2374	2385	rBV	2358761	3637601	66.08%	6.453%
26	17.057	2385	2392	2413	rVV	2818825	4459131	81.00%	7.911%
27	17.633	2487	2490	2496	rBV8	13473	19519	0.35%	0.035%
28	17.892	2531	2534	2540	rVB7	15838	27766	0.50%	0.049%
29	18.975	2715	2718	2723	rVB2	39224	54426	0.99%	0.097%
30	19.063	2730	2733	2738	rVB2	32611	40477	0.74%	0.072%
31	19.433	2790	2796	2807	rBV2	3188569	5505000	100.00%	9.766%
32	21.386	3122	3128	3140	rVB	2489293	4047667	73.53%	7.181%
33	24.345	3623	3631	3644	rVB	2135801	4968862	90.26%	8.815%
34	24.557	3660	3667	3685	rVB	1598020	4224882	76.75%	7.495%

Sum of corrected areas: 56367936




Instrument :
BNA_P
ClientSampleId :
SBLK621

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023469.D
Acq On : 17 Dec 2024 16:53
Operator : RC/JU
Sample : PB165621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

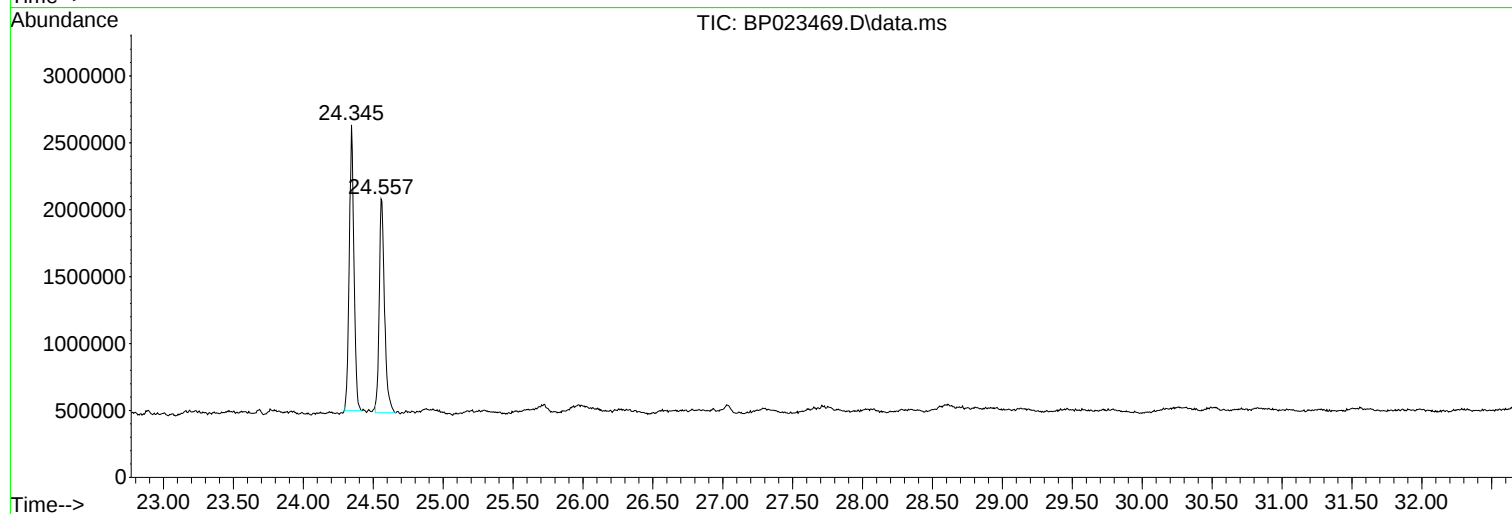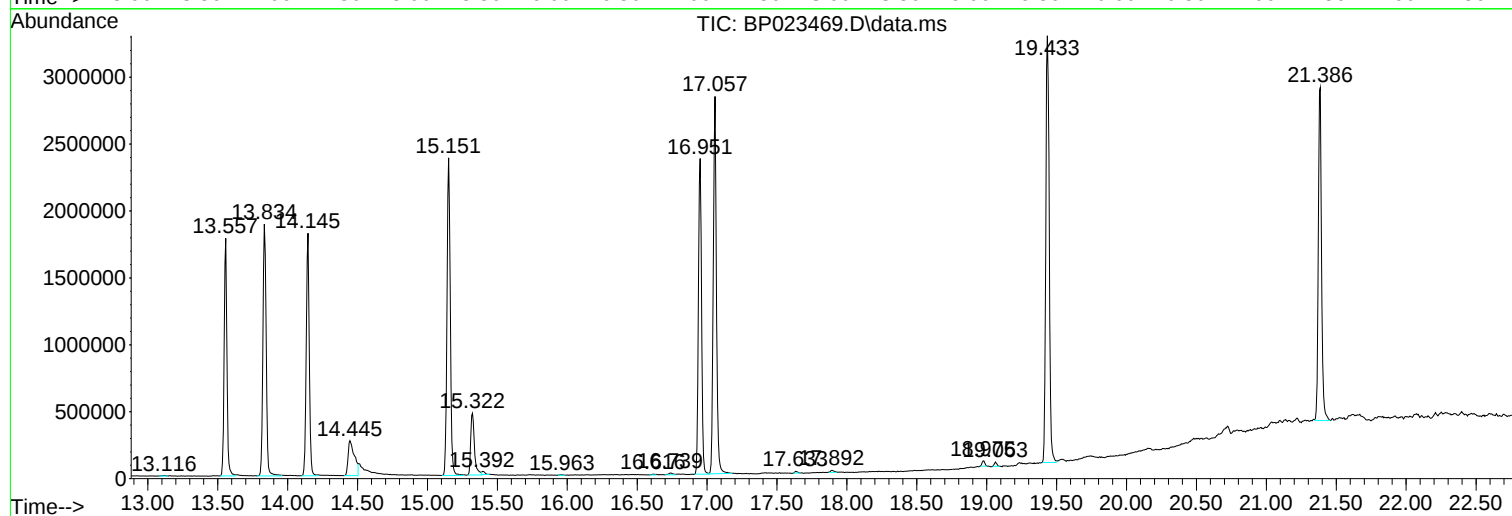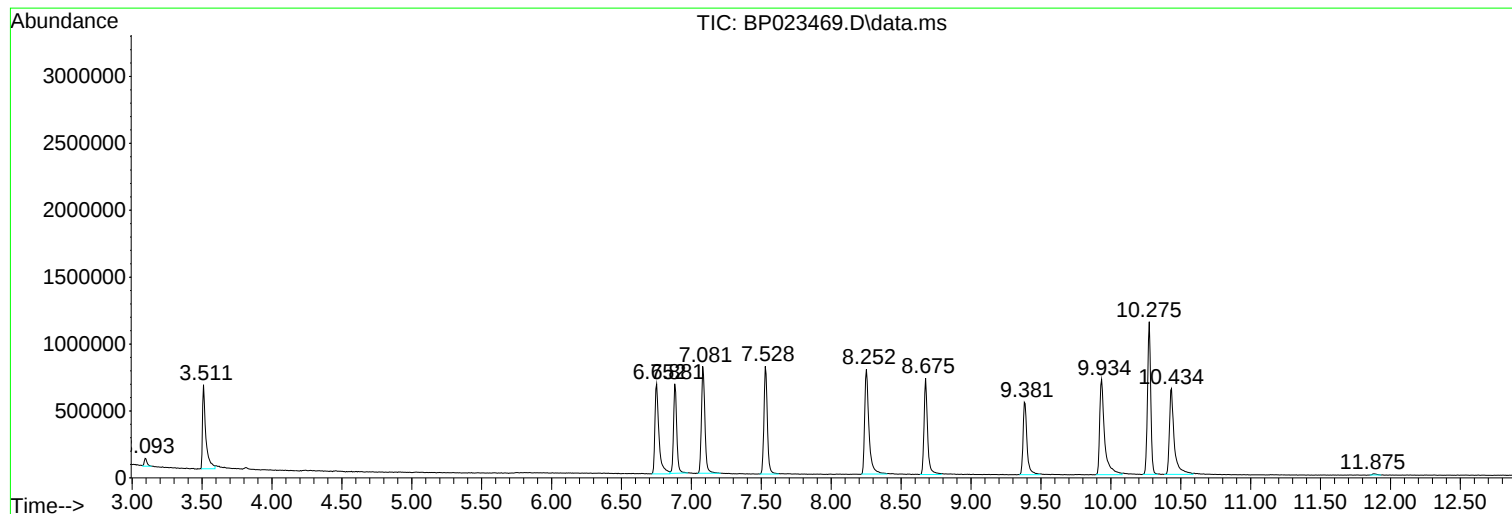

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023469.D
Acq On : 17 Dec 2024 16:53
Operator : RC/JU
Sample : PB165621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121624\
Data File : BP023469.D
Acq On : 17 Dec 2024 16:53
Operator : RC/JU
Sample : PB165621BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc