

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121820\
 Data File : BP004365.D
 Acq On : 18 Dec 2020 19:42
 Operator : CG/JU
 Sample : L5128-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C8

Quant Time: Dec 19 00:51:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 17:12:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	481485	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	2018234	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	1288957	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	2867271	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	3038652	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	3282425	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.32	96	20949	1.81	ng/uL	0.00
5) Phenol-d5	6.99	99	38869	0.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	58537	2.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	80021	2.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	57917	1.74	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	38440	2.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	40321	2.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	84876	2.40	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	112580	2.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	228773	2.22	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	221195	1.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.67	143	11568	0.62	ng/ul	0.00
58) Fluorene-d10	15.47	176	151979	1.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.59	200	24537	1.33	ng/ul	0.00
71) Anthracene-d10	17.33	188	263645	1.86	ng/ul	0.00
79) Pyrene-d10	19.57	212	301240	1.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.53	264	314395	1.74	ng/ul	0.00


Target Compounds					Ovalue	
2) 1,4-Dioxane	3.35	88	62792	5.307	ng/uL#	95
45) Dimethylphthalate	13.92	163	133653	1.293	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121820\
Data File : BP004365.D
Acq On : 18 Dec 2020 19:42
Operator : CG/JU
Sample : L5128-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C8

Quant Time: Dec 19 00:51:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 17:12:07 2020
Response via : Initial Calibration

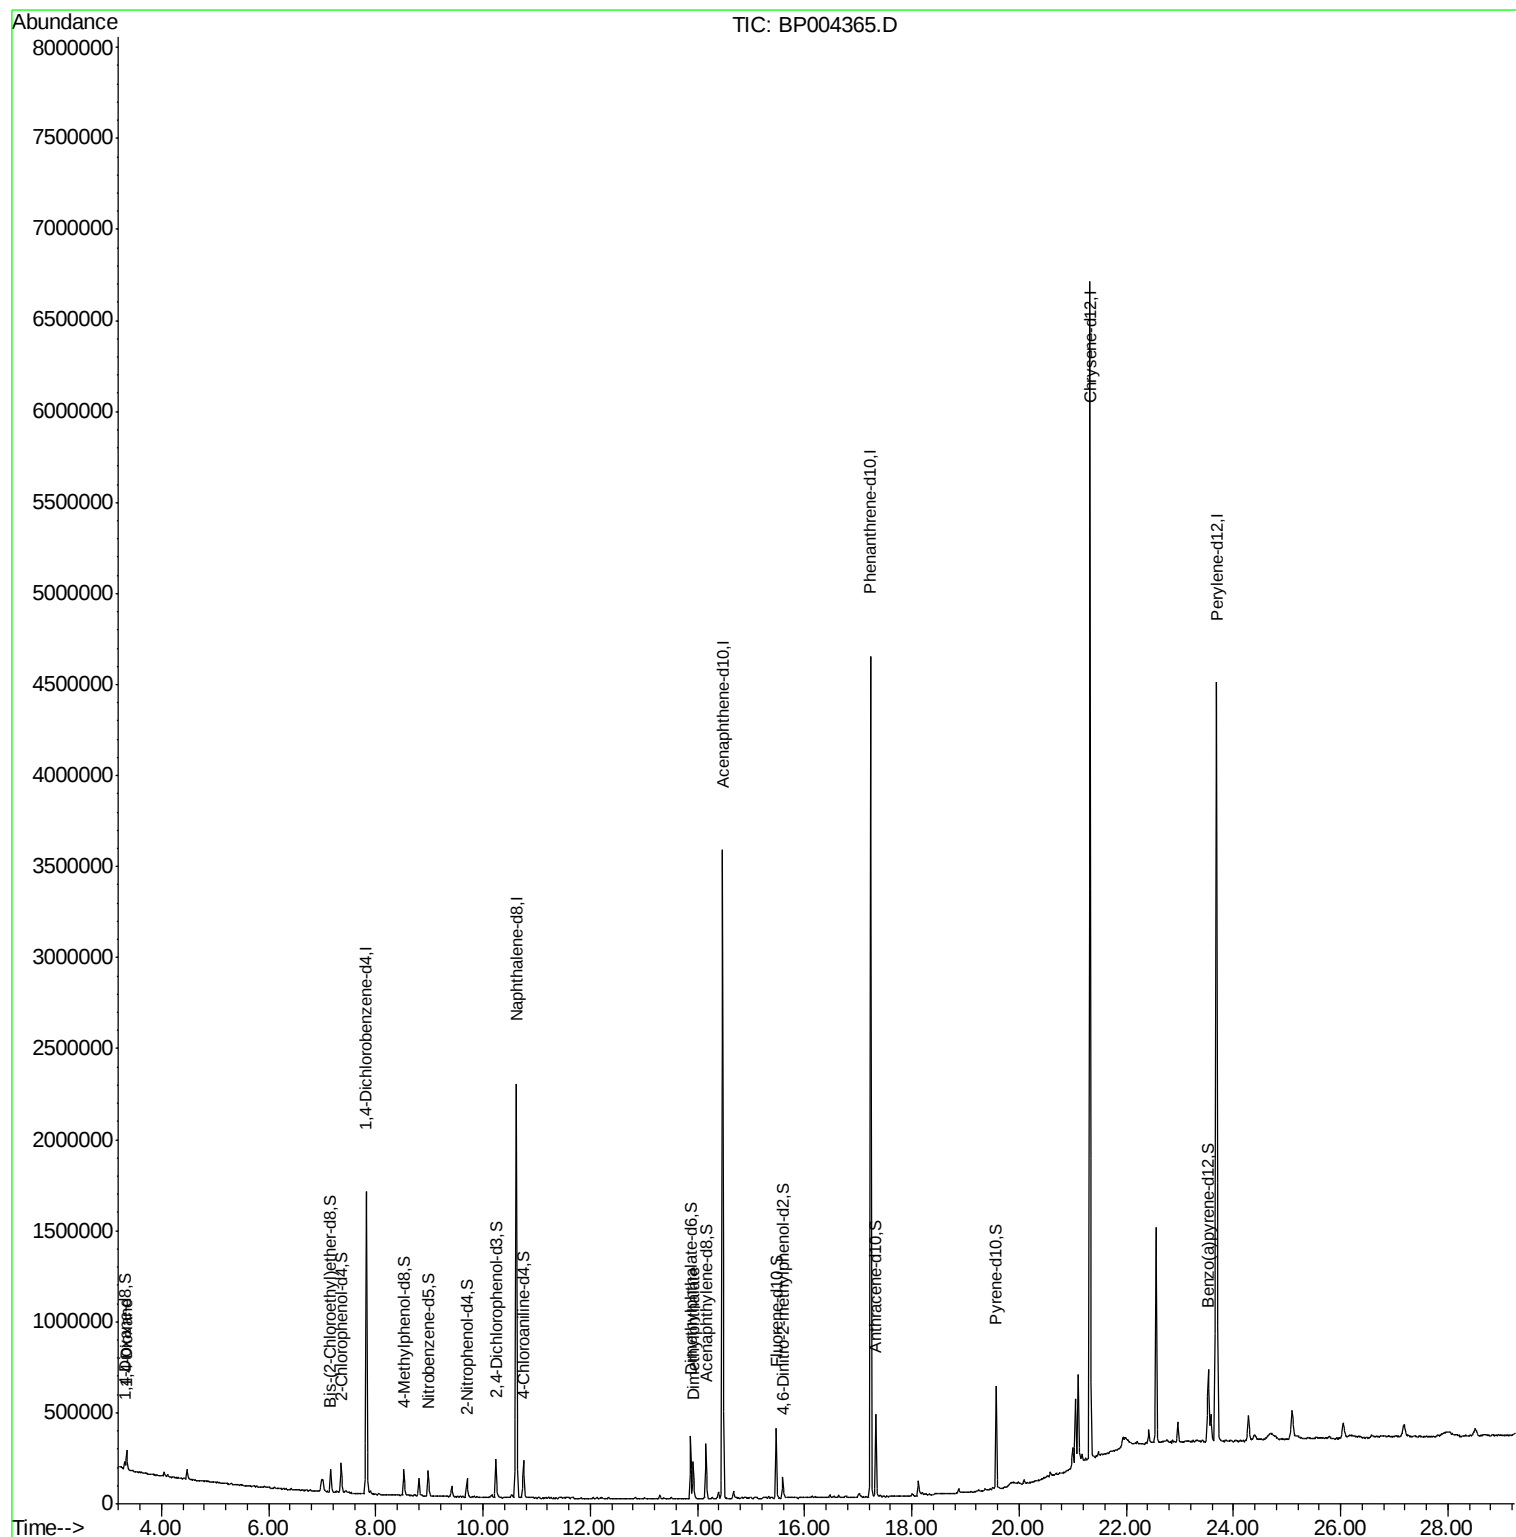

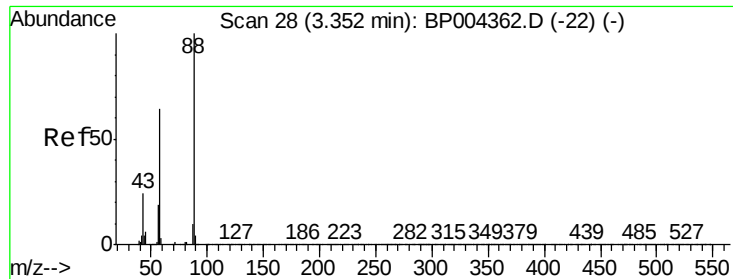

#2

1,4-Dioxane

Concen: 5.307 ng/uL

RT: 3.35 min Scan# 28

Delta R.T. -0.00 min

Lab File: BP004365.D

Acq: 18 Dec 2020 19:42

Instrument :

BNA_P

ClientSampleId :

CB8C8





Tot Ion: 88 Resp: 62792

Ion Ratio Lower Upper

88 100

43 21.9 22.7 34.1#

58 61.5 49.9 74.9

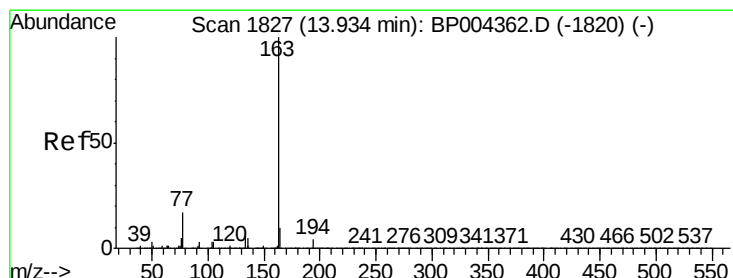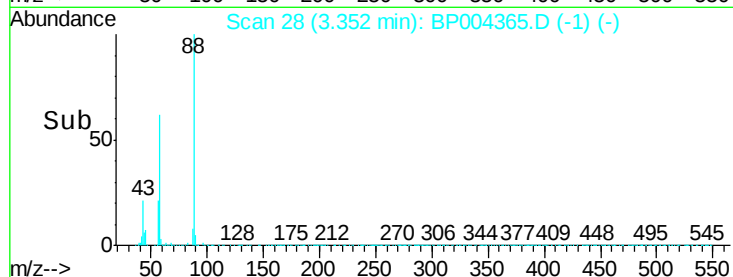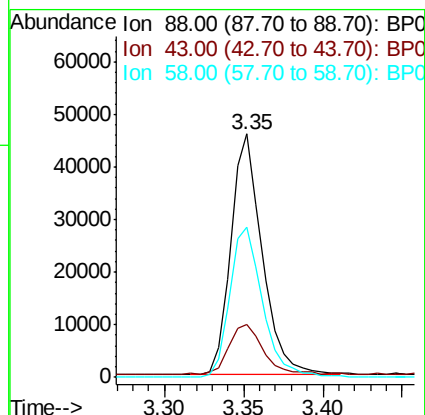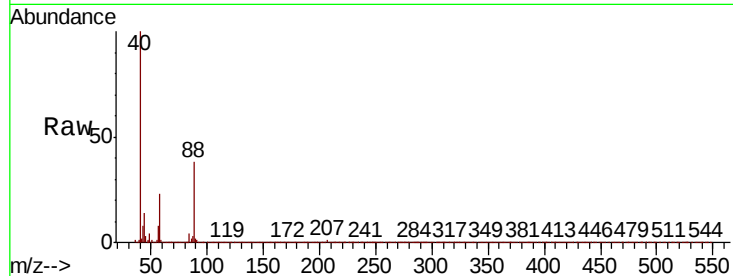

#45

Dimethylphthalate

Concen: 1.293 ng/uL

RT: 13.92 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BP004365.D

Acq: 18 Dec 2020 19:42

Tgt Ion: 163 Resp: 133653

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.5 7.8 11.8

