

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121820\
 Data File : BP004386.D
 Acq On : 19 Dec 2020 10:33
 Operator : CG/JU
 Sample : L5128-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	37	rVB	135916	186819	4.54%	0.378%
2	4.481	217	220	227	rVB2	49315	76384	1.85%	0.155%
3	6.987	640	646	658	rVB	531036	976909	23.72%	1.978%
4	7.152	669	674	686	rVB	525137	859651	20.87%	1.740%
5	7.358	702	709	719	rVB	693448	1115059	27.08%	2.258%
6	7.822	781	788	796	rBV	820661	1301451	31.60%	2.635%
7	7.887	796	799	806	rVB5	12261	23556	0.57%	0.048%
8	8.528	901	908	918	rBV	838600	1362130	33.08%	2.758%
9	8.722	937	941	947	rVB3	9214	17267	0.42%	0.035%
10	8.805	952	955	957	rBV2	6803	8086	0.20%	0.016%
11	8.975	977	984	992	rBV	627483	1053694	25.59%	2.133%
12	9.422	1053	1060	1067	rBV3	64850	125430	3.05%	0.254%
13	9.516	1073	1076	1080	rBV6	4294	6179	0.15%	0.013%
14	9.616	1090	1093	1100	rVB7	6517	12744	0.31%	0.026%
15	9.699	1100	1107	1121	rBV	513198	885946	21.51%	1.794%
16	9.834	1123	1130	1135	rVB6	11330	21114	0.51%	0.043%
17	10.163	1179	1186	1192	rVB5	17667	38974	0.95%	0.079%
18	10.240	1192	1199	1208	rBV	916924	1529712	37.14%	3.097%
19	10.381	1219	1223	1226	rBV6	4795	8206	0.20%	0.017%
20	10.534	1241	1249	1256	rBV3	24368	52839	1.28%	0.107%
21	10.616	1256	1263	1273	rVB	1156601	1957617	47.54%	3.963%
22	10.751	1278	1286	1300	rBV	884833	1517723	36.85%	3.073%
23	10.869	1300	1306	1313	rVB	7688	18287	0.44%	0.037%
24	10.963	1320	1322	1326	rVB5	3422	4565	0.11%	0.009%
25	11.034	1328	1334	1341	rVV5	6983	14993	0.36%	0.030%
26	11.169	1352	1357	1361	rBV8	5242	10611	0.26%	0.021%
27	11.228	1363	1367	1372	rVV8	4444	10655	0.26%	0.022%
28	11.428	1396	1401	1402	rVV4	6620	10623	0.26%	0.022%
29	11.457	1402	1406	1411	rVB5	11832	21894	0.53%	0.044%
30	11.581	1423	1427	1432	rVB8	11777	19665	0.48%	0.040%
31	11.651	1432	1439	1440	rBV7	4881	8359	0.20%	0.017%
32	11.775	1455	1460	1463	rBV7	3838	5679	0.14%	0.011%
33	11.816	1463	1467	1473	rVB5	9199	17217	0.42%	0.035%
34	11.869	1473	1476	1481	rBV7	4483	7932	0.19%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121820\
 Data File : BP004386.D
 Acq On : 19 Dec 2020 10:33
 Operator : CG/JU
 Sample : L5128-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	12.051	1504	1507	1514	rVB8	6036	11547	0.28%	0.023%
36	12.187	1519	1530	1534	rBV9	10536	33605	0.82%	0.068%
37	12.334	1550	1555	1559	rBV6	6138	10773	0.26%	0.022%
38	12.434	1569	1572	1577	rVB7	5573	7792	0.19%	0.016%
39	12.575	1587	1596	1601	rBV7	4807	13216	0.32%	0.027%
40	12.722	1614	1621	1626	rBV7	3110	8019	0.19%	0.016%
41	12.834	1634	1640	1647	rBV7	7888	15705	0.38%	0.032%
42	13.010	1666	1670	1673	rBV6	5628	8551	0.21%	0.017%
43	13.163	1693	1696	1698	rBV4	3269	4495	0.11%	0.009%
44	13.298	1716	1719	1727	rVB3	15581	24609	0.60%	0.050%
45	13.369	1727	1731	1735	rBV6	5226	9315	0.23%	0.019%
46	13.504	1750	1754	1762	rVB6	11810	23216	0.56%	0.047%
47	13.681	1781	1784	1786	rBV4	3895	4685	0.11%	0.009%
48	13.875	1807	1817	1822	rBV	1503963	2070156	50.27%	4.191%
49	13.922	1822	1825	1834	rVB	120298	160949	3.91%	0.326%
50	14.004	1834	1839	1842	rBV7	4062	5516	0.13%	0.011%
51	14.163	1856	1866	1878	rVB	1627703	2521660	61.23%	5.105%
52	14.263	1878	1883	1890	rBV3	17906	35745	0.87%	0.072%
53	14.392	1899	1905	1911	rVB3	45404	71878	1.75%	0.146%
54	14.469	1911	1918	1928	rVB2	1818789	2762819	67.09%	5.594%
55	14.551	1928	1932	1934	rBV4	4208	5017	0.12%	0.010%
56	14.669	1946	1952	1963	rBV	477930	775883	18.84%	1.571%
57	14.828	1975	1979	1982	rBV6	4428	5722	0.14%	0.012%
58	15.004	2003	2009	2012	rVB8	5616	9888	0.24%	0.020%
59	15.063	2016	2019	2022	rBV5	6731	8920	0.22%	0.018%
60	15.222	2042	2046	2049	rBV6	7063	12459	0.30%	0.025%
61	15.269	2052	2054	2061	rVV8	7952	16464	0.40%	0.033%
62	15.334	2061	2065	2068	rVV4	8992	12021	0.29%	0.024%
63	15.375	2070	2072	2077	rVB6	3323	5213	0.13%	0.011%
64	15.469	2077	2088	2095	rBV	2054467	2994125	72.70%	6.062%
65	15.592	2102	2109	2122	rBV	558399	829046	20.13%	1.678%
66	15.710	2124	2129	2140	rVB4	26076	60461	1.47%	0.122%
67	15.934	2162	2167	2170	rBV6	3634	6561	0.16%	0.013%
68	16.134	2196	2201	2209	rBV6	10981	24124	0.59%	0.049%
69	16.198	2209	2212	2215	rBV5	4943	6570	0.16%	0.013%
70	16.469	2252	2258	2261	rBV4	6664	11154	0.27%	0.023%
71	16.539	2267	2270	2276	rVB4	10269	12916	0.31%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121820\
 Data File : BP004386.D
 Acq On : 19 Dec 2020 10:33
 Operator : CG/JU
 Sample : L5128-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

72	16.622	2281	2284	2289	rBV7	3639	5934	0.14%	0.012%
73	16.763	2304	2308	2315	rVB4	10892	18170	0.44%	0.037%
74	17.016	2344	2351	2360	rVB4	13266	34064	0.83%	0.069%
75	17.092	2360	2364	2365	rBV4	4231	6627	0.16%	0.013%
76	17.228	2380	2387	2397	rBV	2343967	3327509	80.80%	6.737%
77	17.328	2398	2404	2416	rVB2	2269802	3264008	79.26%	6.608%
78	17.610	2448	2452	2455	rBV6	3535	6786	0.16%	0.014%
79	17.986	2513	2516	2517	rBV3	5810	5778	0.14%	0.012%
80	18.122	2535	2539	2544	rBV2	35454	57095	1.39%	0.116%
81	18.875	2663	2667	2670	rBV2	27361	34328	0.83%	0.070%
82	19.463	2764	2767	2770	rVB	22013	26255	0.64%	0.053%
83	19.569	2779	2785	2792	rBV	2950886	3969520	96.39%	8.037%
84	21.039	3031	3035	3042	rBV2	203423	367569	8.93%	0.744%
85	21.098	3042	3045	3053	rVB	130568	192076	4.66%	0.389%
86	21.322	3078	3083	3091	rBV	3108839	3885797	94.36%	7.867%
87	22.551	3289	3292	3297	rVB	151775	203335	4.94%	0.412%
88	23.527	3451	3458	3472	rVB2	2110775	4118254	100.00%	8.338%
89	23.680	3476	3484	3496	rVB	1921303	3980696	96.66%	8.059%


Sum of corrected areas: 49392566

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121820\
Data File : BP004386.D
Acq On : 19 Dec 2020 10:33
Operator : CG/JU
Sample : L5128-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

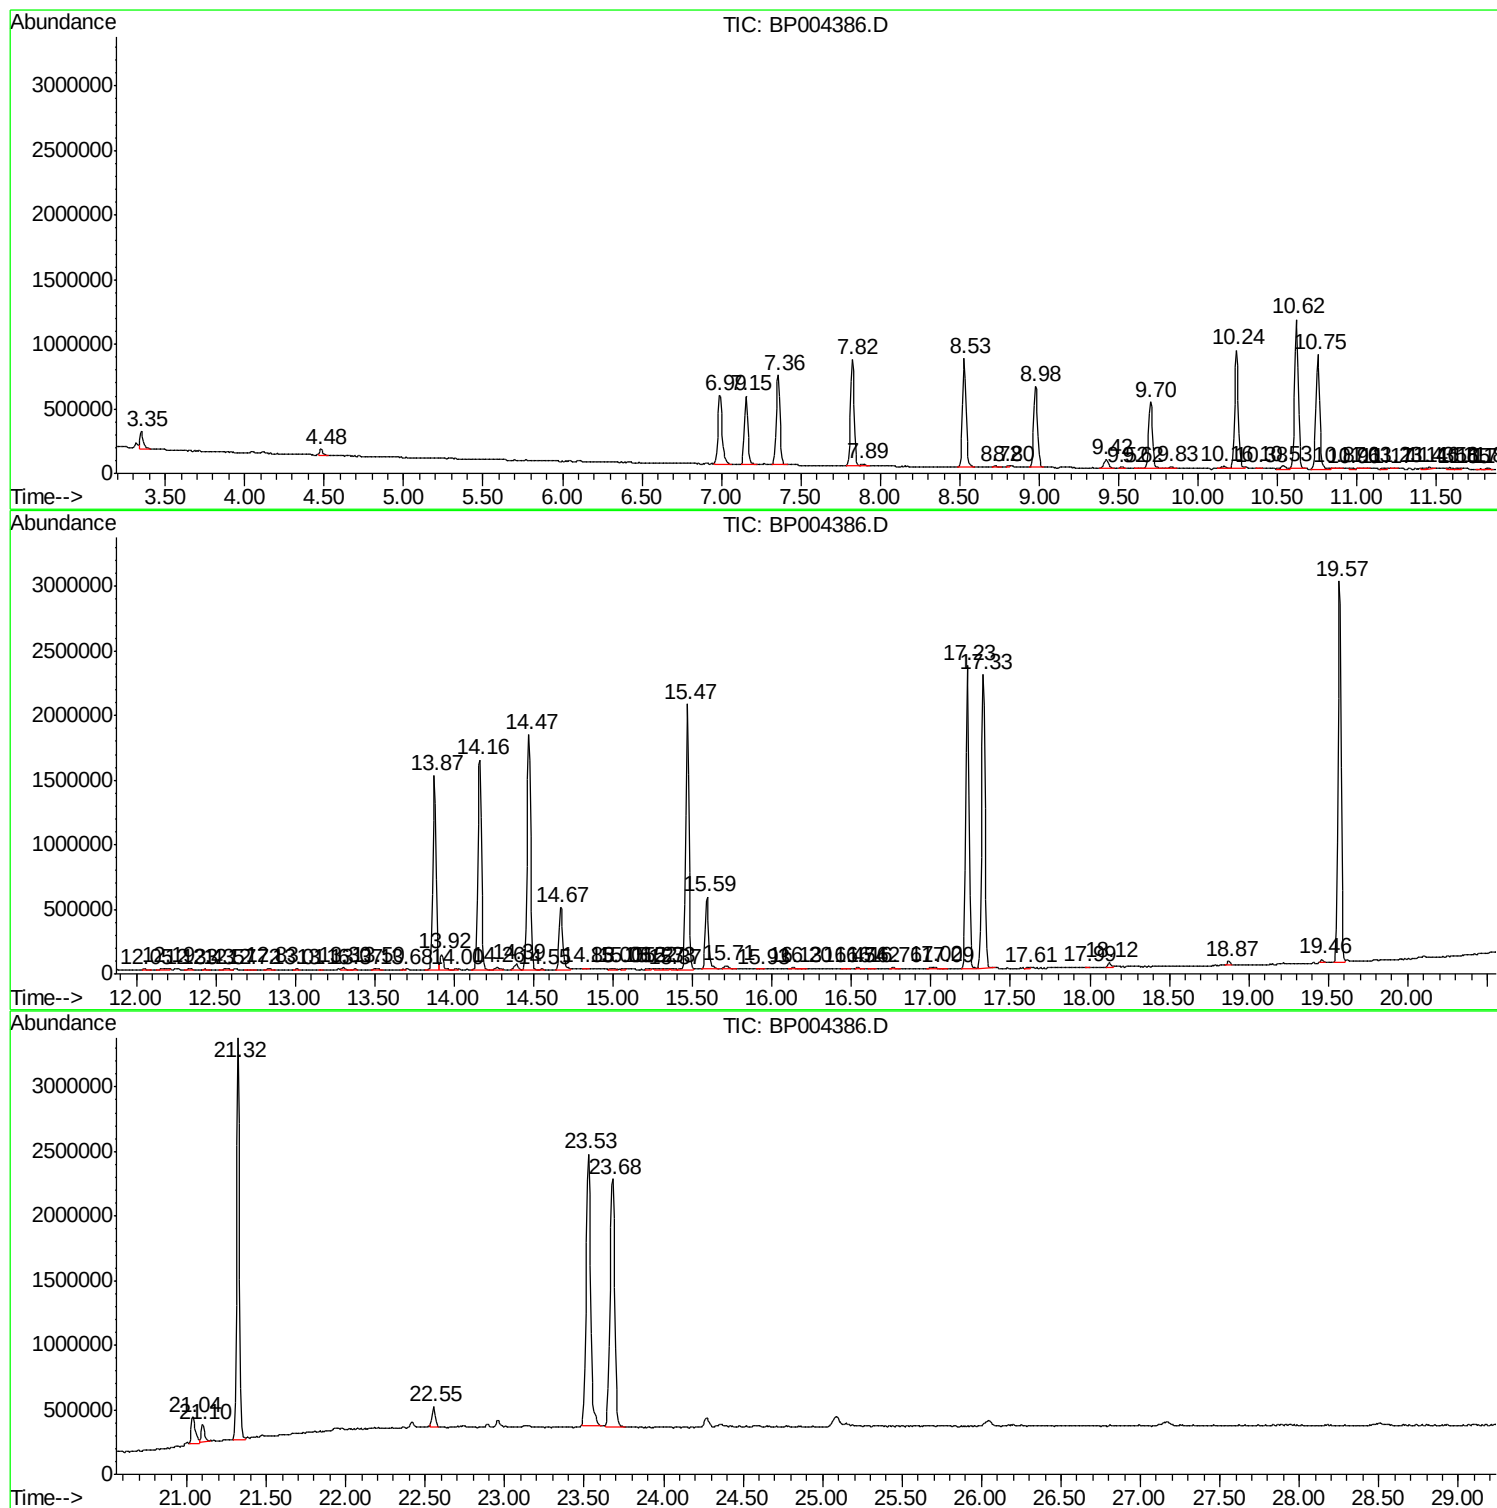

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121820\
Data File : BP004386.D
Acq On : 19 Dec 2020 10:33
Operator : CG/JU
Sample : L5128-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121820\
Data File : BP004386.D
Acq On : 19 Dec 2020 10:33
Operator : CG/JU
Sample : L5128-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc