
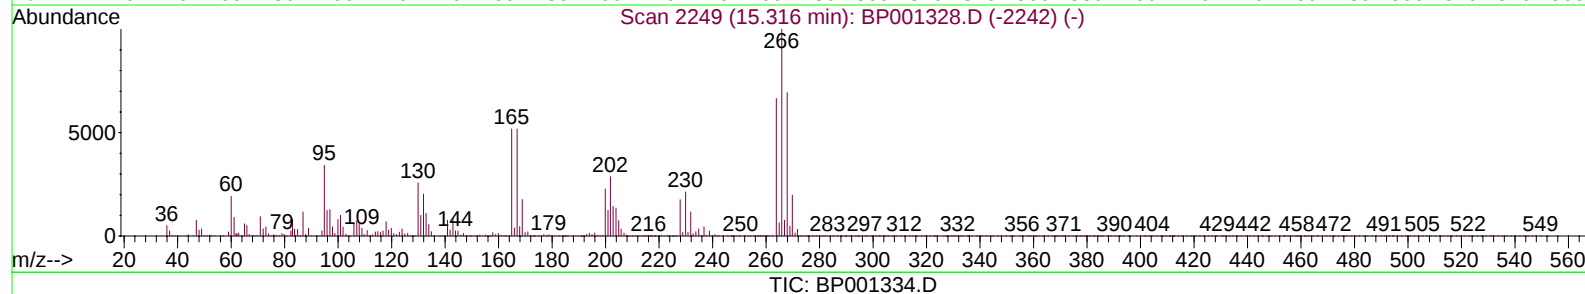
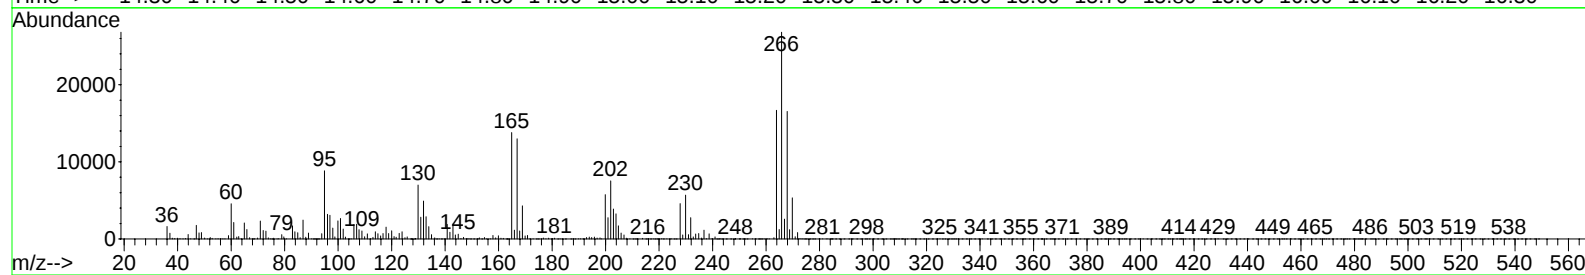


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122019\  
Data File  : BP001334.D  
Acq On     : 20 Dec 2019   09:44  
Operator   : JU  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Dec 20 17:28:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 03:20:39 2019
Response via : Initial Calibration

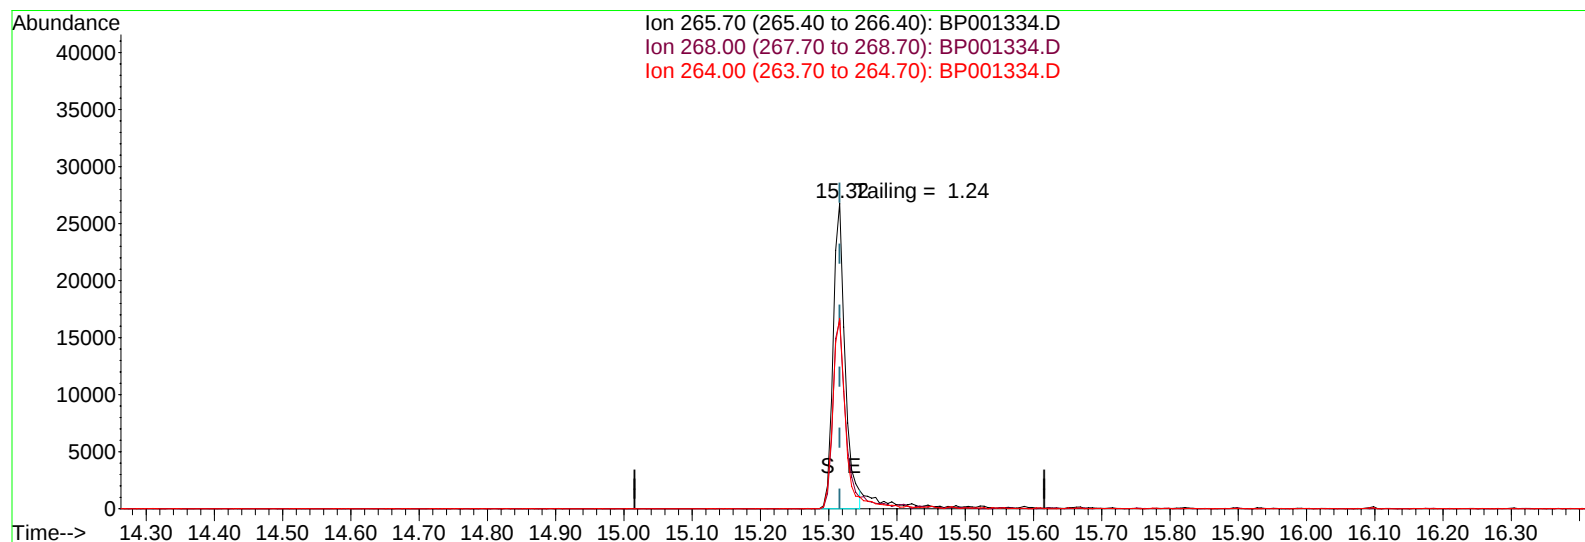

(70) Pentachlorophenol (C)




15.316min (0.000) 47898.12ng

response 35045

Ion	Exp%	Act%
265.70	100	100
268.00	69.30	61.65
264.00	66.50	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122019\
Data File : BP001334.D
Acq On : 20 Dec 2019 09:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 17:28:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 03:20:39 2019
Response via : Initial Calibration

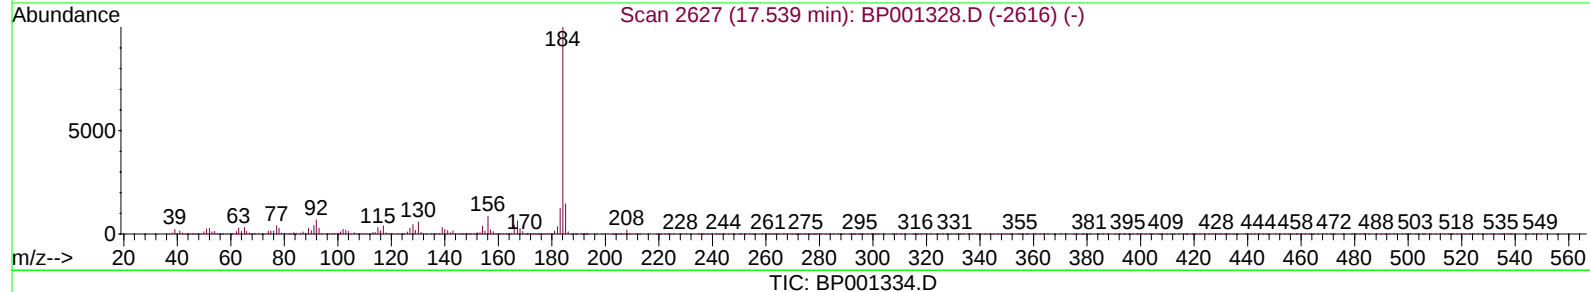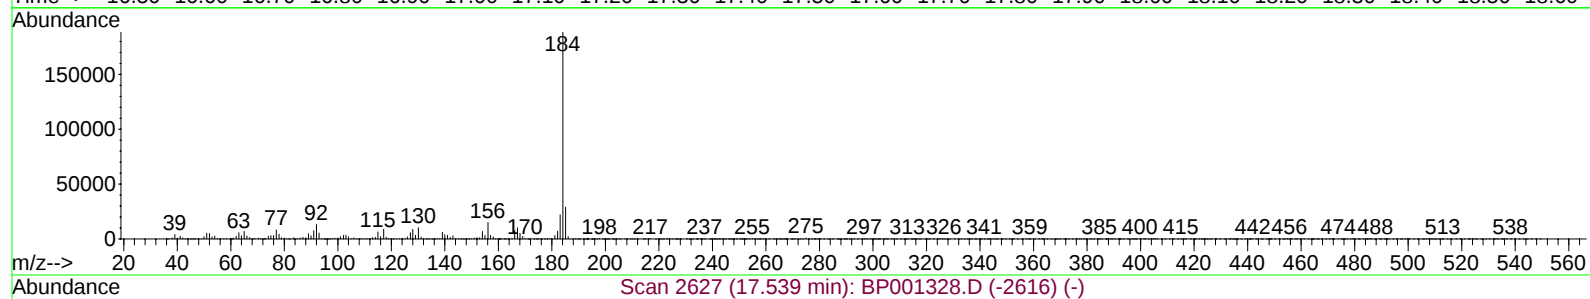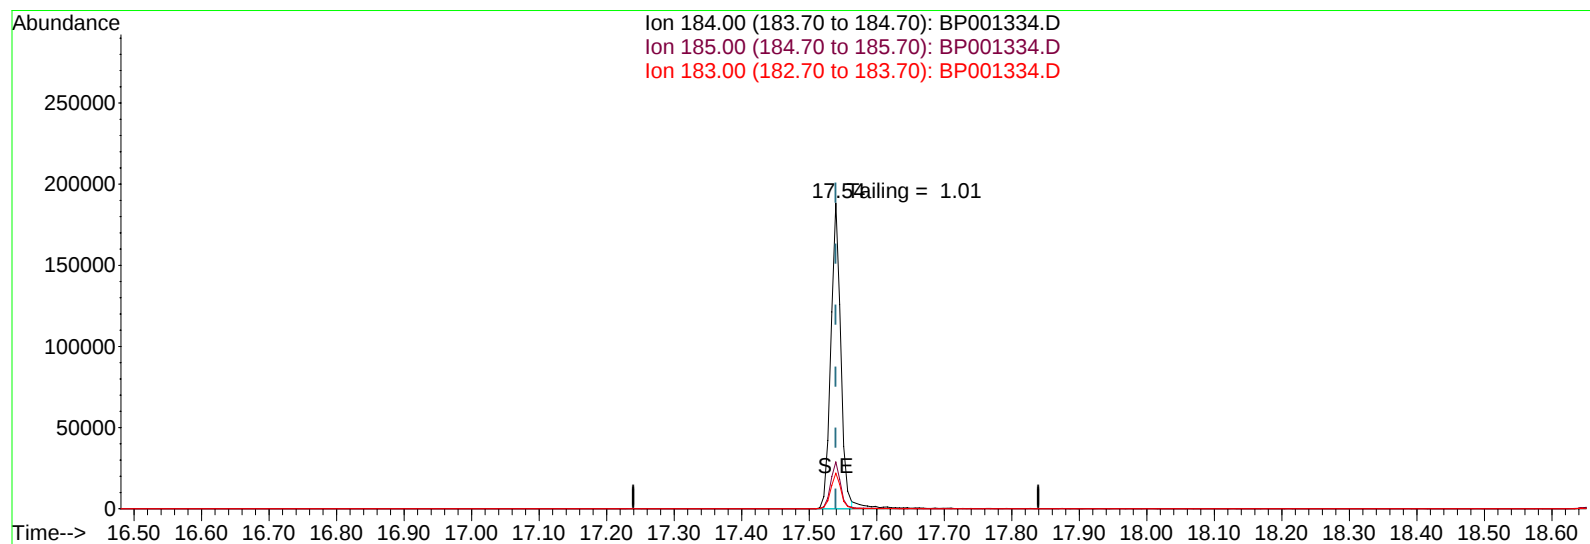

(77) Benzidine

17.539min (0.000) 41990.03ng

response 196830

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	15.32
183.00	12.30	11.68
0.00	0.00	0.00