

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013300.D
 Acq On : 24 Dec 2022 15:15
 Operator : CG/JU
 Sample : N6016-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 00:21:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	728009	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	3045733	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1815639	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	3177621	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2738752	20.000	ng/ul	0.00
88) Perylene-d12	23.915	264	3227254	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	67295	3.952	ng/uL	0.00
4) Pyridine-d5	3.758	84	942187	19.480	ng/ul	0.00
7) Phenol-d5	7.105	99	1443434	24.342	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	888605	24.842	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	1182344	25.329	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	953288	19.620	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	578230	25.839	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	674179	26.760	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	1237832	25.296	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	975892	14.127	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	3531918	25.311	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	3945267	25.730	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	405117	16.140	ng/ul	0.00
60) Fluorene-d10	15.581	176	2868495	24.299	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	294296	14.392	ng/ul	0.00
73) Anthracene-d10	17.445	188	3442303	24.012	ng/ul	0.00
81) Pyrene-d10	19.675	212	3922010	24.949	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	4059226	25.235	ng/ul	0.00
Target Compounds						
6) Benzaldehyde	7.081	77	23987	1.033	ng/ul	94
10) Bis(2-Chloroethyl)ether	7.369	93	78870	1.603	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013300.D
Acq On : 24 Dec 2022 15:15
Operator : CG/JU
Sample : N6016-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 25 00:21:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration




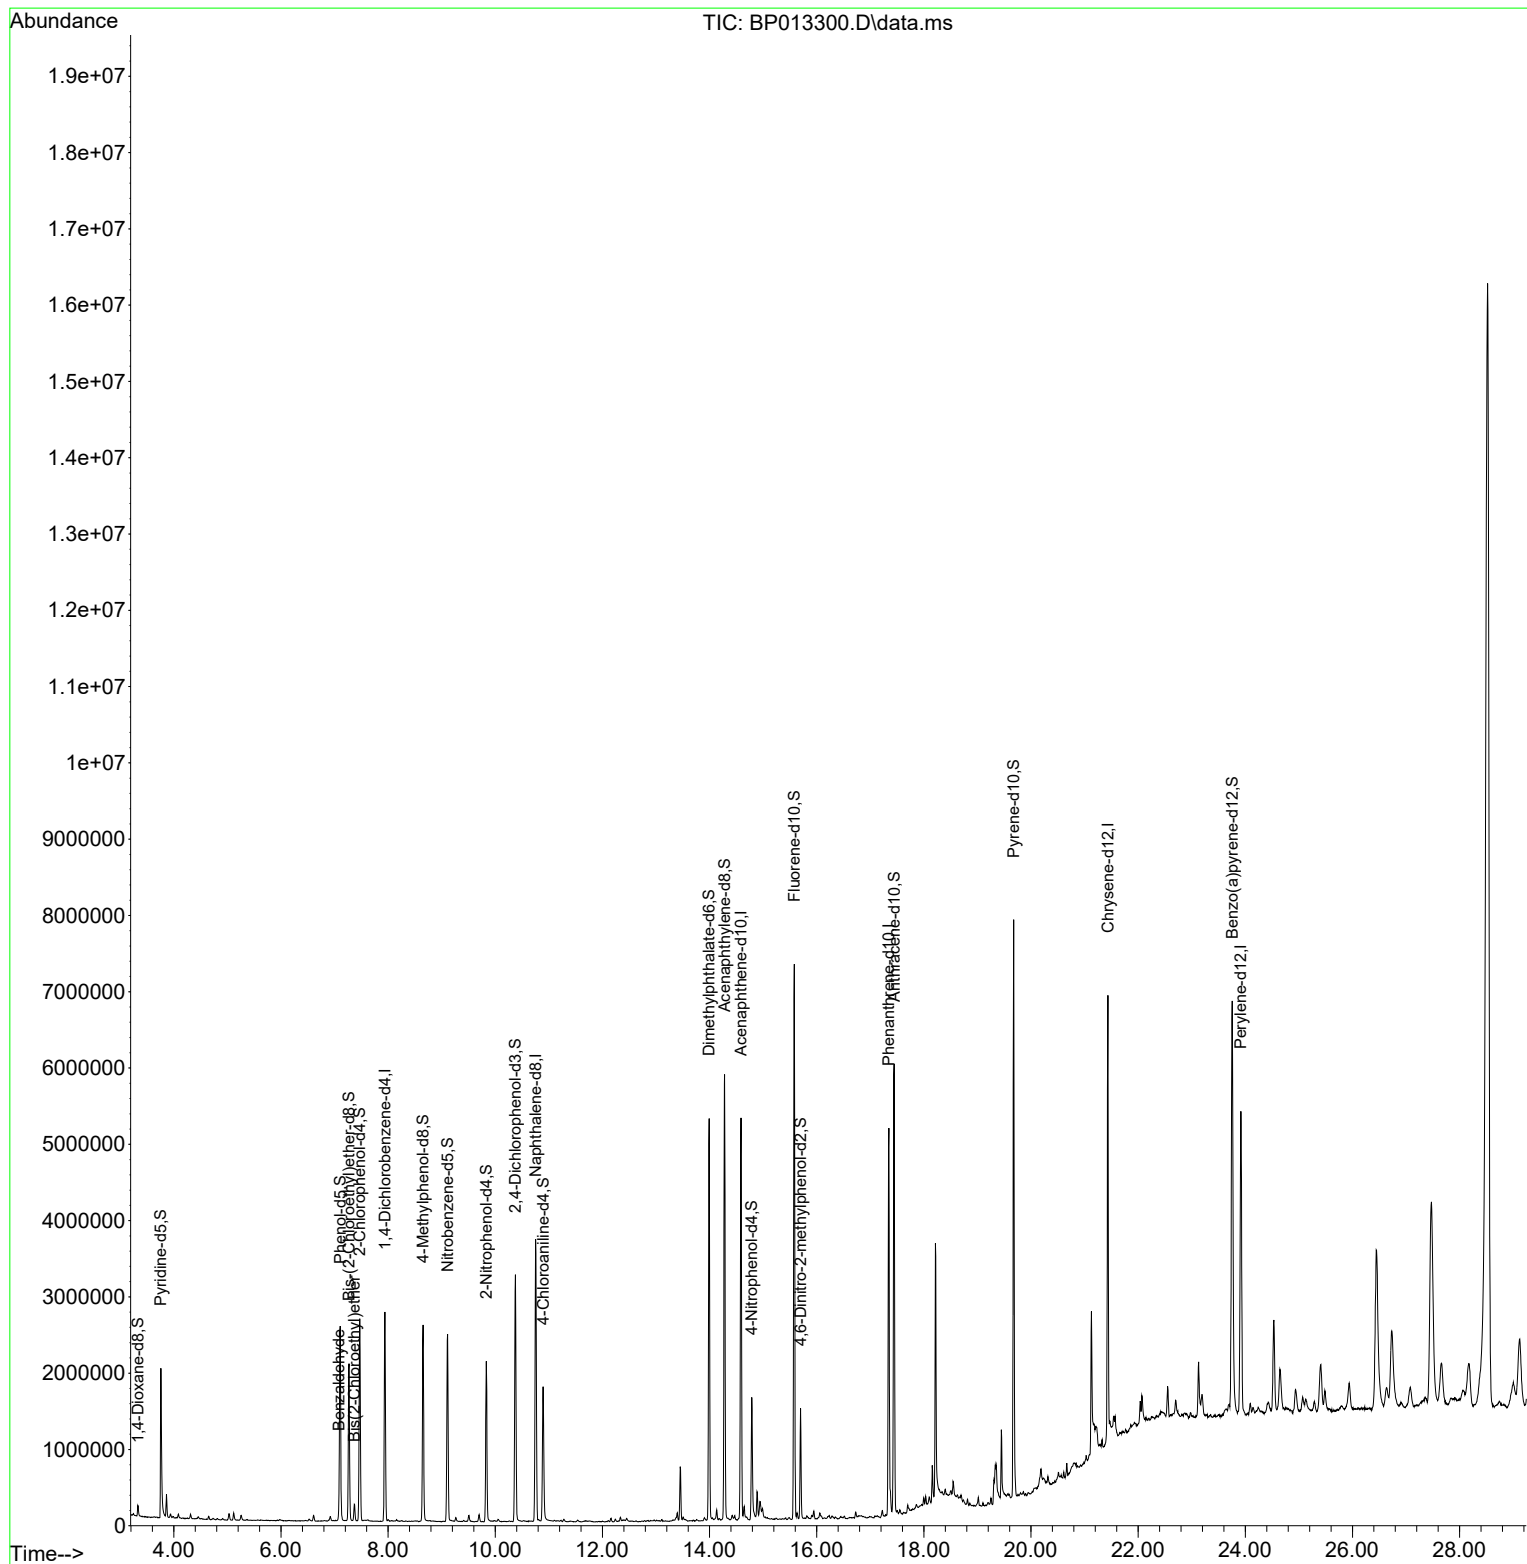


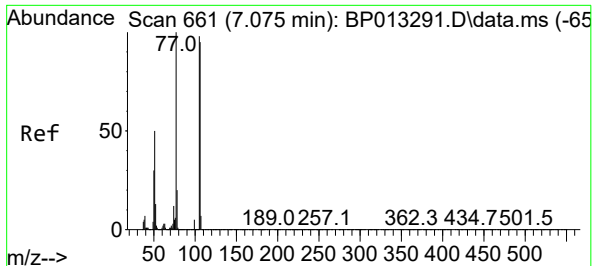

#6
Benzaldehyde
Concen: 1.033 ng/ul
RT: 7.081 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP013300.D
Acq: 24 Dec 2022 15:15

Instrument :
BNA_P
ClientSampleId :

Tgt Ion: 77 Resp: 23987
Ion Ratio Lower Upper
77 100
105 97.8 81.5 122.3
106 88.2 76.9 115.3

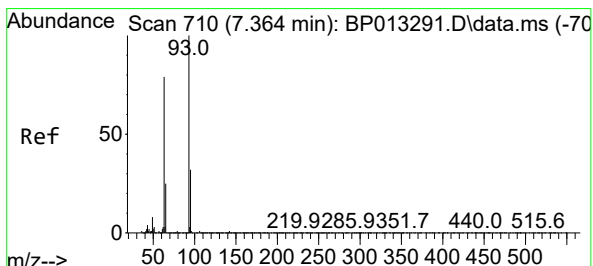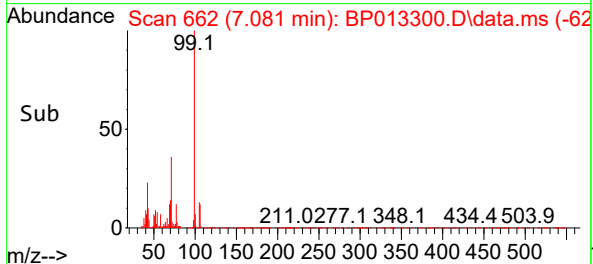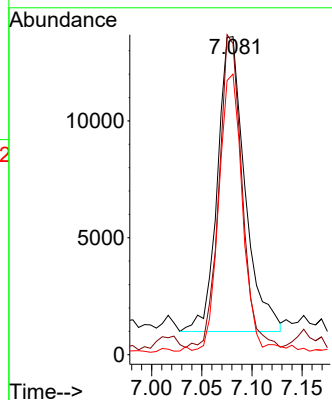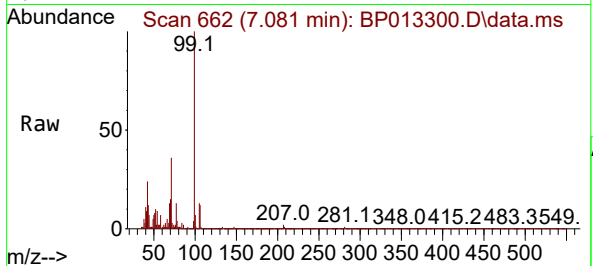

#10
Bis(2-Chloroethyl)ether
Concen: 1.603 ng/ul
RT: 7.369 min Scan# 711
Delta R.T. 0.006 min
Lab File: BP013300.D
Acq: 24 Dec 2022 15:15

Tgt Ion: 93 Resp: 78870
Ion Ratio Lower Upper
93 100
63 3.6 59.8 89.8#
95 3.7 26.4 39.6#

