

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013307.D
 Acq On : 24 Dec 2022 19:12
 Operator : CG/JU
 Sample : PB149810BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 00:23:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	597524	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	2215122	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	1157340	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	2436490	20.000	ng/u1	0.00
79) Chrysene-d12	21.439	240	2730650	20.000	ng/u1	0.00
88) Perylene-d12	23.921	264	3171471	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	80464	5.758	ng/uL	0.00
4) Pyridine-d5	3.758	84	1148837	28.939	ng/u1	0.00
7) Phenol-d5	7.105	99	1440093	29.589	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	883900	30.106	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	1174815	30.663	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	1066316	26.739	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	541901	33.296	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	612827	33.446	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	1081334	30.384	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	1191832	23.722	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	2537047	28.523	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	3032271	31.025	ng/u1	0.00
54) 4-Nitrophenol-d4	14.792	143	477734	29.859	ng/u1	0.00
60) Fluorene-d10	15.581	176	2160488	28.711	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	402850	25.693	ng/u1	0.00
73) Anthracene-d10	17.445	188	3410082	31.023	ng/u1	0.00
81) Pyrene-d10	19.680	212	4507432	28.758	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.763	264	4987517	31.551	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	170297	11.673	ng/uL	95
5) Pyridine	3.775	79	1192784	30.232	ng/u1	96
6) Benzaldehyde	7.075	77	916166	48.074	ng/u1	97
8) Phenol	7.134	94	1486741	30.213	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.363	93	1206014	29.860	ng/u1	98
12) 2-Chlorophenol	7.505	128	1209799	30.792	ng/u1	96
13) 2-Methylphenol	8.387	108	1102360	28.734	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.475	45	1752585	31.622	ng/u1	98
16) Acetophenone	8.769	105	1715124	28.049	ng/u1	95
17) N-Nitroso-di-n-propyla...	8.757	70	868199	28.236	ng/u1	96
18) 4-Methylphenol	8.722	108	1149812	27.058	ng/u1	99
19) Hexachloroethane	9.022	117	482235	30.714	ng/u1	98
22) Nitrobenzene	9.152	77	1292309	33.838	ng/u1	98
23) Isophorone	9.681	82	2307884	29.886	ng/u1	98
25) 2-Nitrophenol	9.869	139	651872	32.835	ng/u1	95
26) 2,4-Dimethylphenol	9.928	107	1145361	29.568	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.163	93	1462664	29.622	ng/u1	99
29) 2,4-Dichlorophenol	10.404	162	1079689	30.970	ng/u1	100
30) Naphthalene	10.804	128	3531550	30.484	ng/u1	100
32) 4-Chloroaniline	10.916	127	1216201	24.462	ng/u1	100
33) Hexachlorobutadiene	11.087	225	800550	33.445	ng/u1	99
34) Caprolactam	11.704	113	276550	23.265	ng/u1	94
35) 4-Chloro-3-methylphenol	12.040	107	972638	27.338	ng/u1	99
36) 2-Methylnaphthalene	12.410	142	2224669	27.992	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013307.D
 Acq On : 24 Dec 2022 19:12
 Operator : CG/JU
 Sample : PB149810BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 00:23:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.628	142	2199474	26.911	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.781	216	1325820	35.577	ng/ul	99
40) Hexachlorocyclopentadiene	12.751	237	404626	16.685	ng/ul	99
41) 2,4,6-Trichlorophenol	13.022	196	811614	33.888	ng/ul	98
42) 2,4,5-Trichlorophenol	13.092	196	856576	33.296	ng/ul	99
43) 1,1'-Biphenyl	13.416	154	2829683	32.555	ng/ul	99
44) 2-Chloronaphthalene	13.463	162	2253436	32.940	ng/ul	99
45) 2-Nitroaniline	13.669	65	598340	36.075	ng/ul	95
47) Dimethylphthalate	14.040	163	2561231	29.053	ng/ul	100
48) 2,6-Dinitrotoluene	14.163	165	524308	32.002	ng/ul	98
50) Acenaphthylene	14.310	152	3299835	31.404	ng/ul	99
51) 3-Nitroaniline	14.492	138	522919	33.802	ng/ul	99
52) Acenaphthene	14.651	153	2248151	30.875	ng/ul	100
53) 2,4-Dinitrophenol	14.704	184	254882	22.759	ng/ul	98
55) 4-Nitrophenol	14.804	109	361706	33.132	ng/ul	93
56) Dibenzofuran	14.986	168	3123002	30.166	ng/ul	99
57) 2,4-Dinitrotoluene	14.951	165	729387	30.649	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.210	232	724888	30.876	ng/ul	97
59) Diethylphthalate	15.404	149	2370877	27.665	ng/ul	100
61) Fluorene	15.634	166	2509820	30.229	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.628	204	1310981	29.858	ng/ul	99
63) 4-Nitroaniline	15.657	138	575183	42.252	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.716	198	401309	26.191	ng/ul	96
67) N-Nitrosodiphenylamine	15.845	169	2077073	30.749	ng/ul	99
68) 4-Bromophenyl-phenylether	16.528	248	786351	29.719	ng/ul	99
69) Hexachlorobenzene	16.645	284	964799	30.708	ng/ul	99
70) Atrazine	16.798	200	756574	28.742	ng/ul	99
71) Pentachlorophenol	16.992	266	618669	32.516	ng/ul	100
72) Phenanthrene	17.386	178	4029563	31.752	ng/ul	100
74) Anthracene	17.480	178	4061165	32.049	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.387	216	1296496	37.296	ng/uL	99
76) Pentachlorobenzene	14.904	250	1133968	31.995	ng/uL	100
77) Carbazole	17.751	167	3788098	35.497	ng/ul	99
78) Di-n-butylphthalate	18.292	149	3934042	30.277	ng/ul	99
80) Fluoranthene	19.351	202	5290750	29.741	ng/ul	100
82) Pyrene	19.704	202	5583436	30.426	ng/ul	100
83) Butylbenzylphthalate	20.569	149	2099380	29.613	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.351	252	1991278	32.280	ng/ul	99
85) Benzo(a)anthracene	21.421	228	5909401	32.599	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.327	149	3005390	30.053	ng/ul	100
87) Chrysene	21.474	228	5501342	32.092	ng/ul	99
89) Di-n-octyl phthalate	22.280	149	5513120	31.029	ng/ul	100
90) Benzo(b)fluoranthene	23.157	252	6221221	30.762	ng/ul	100
91) Benzo(k)fluoranthene	23.210	252	6235179	31.092	ng/ul	100
93) Benzo(a)pyrene	23.810	252	5633684	31.993	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.521	276	7442173	33.929	ng/ul	99
95) Dibenzo(a,h)anthracene	26.539	278	6320155	34.801	ng/ul	99
96) Benzo(g,h,i)perylene	27.315	276	6130042	34.812	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013307.D
Acq On : 24 Dec 2022 19:12
Operator : CG/JU
Sample : PB149810BS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Dec 25 00:23:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

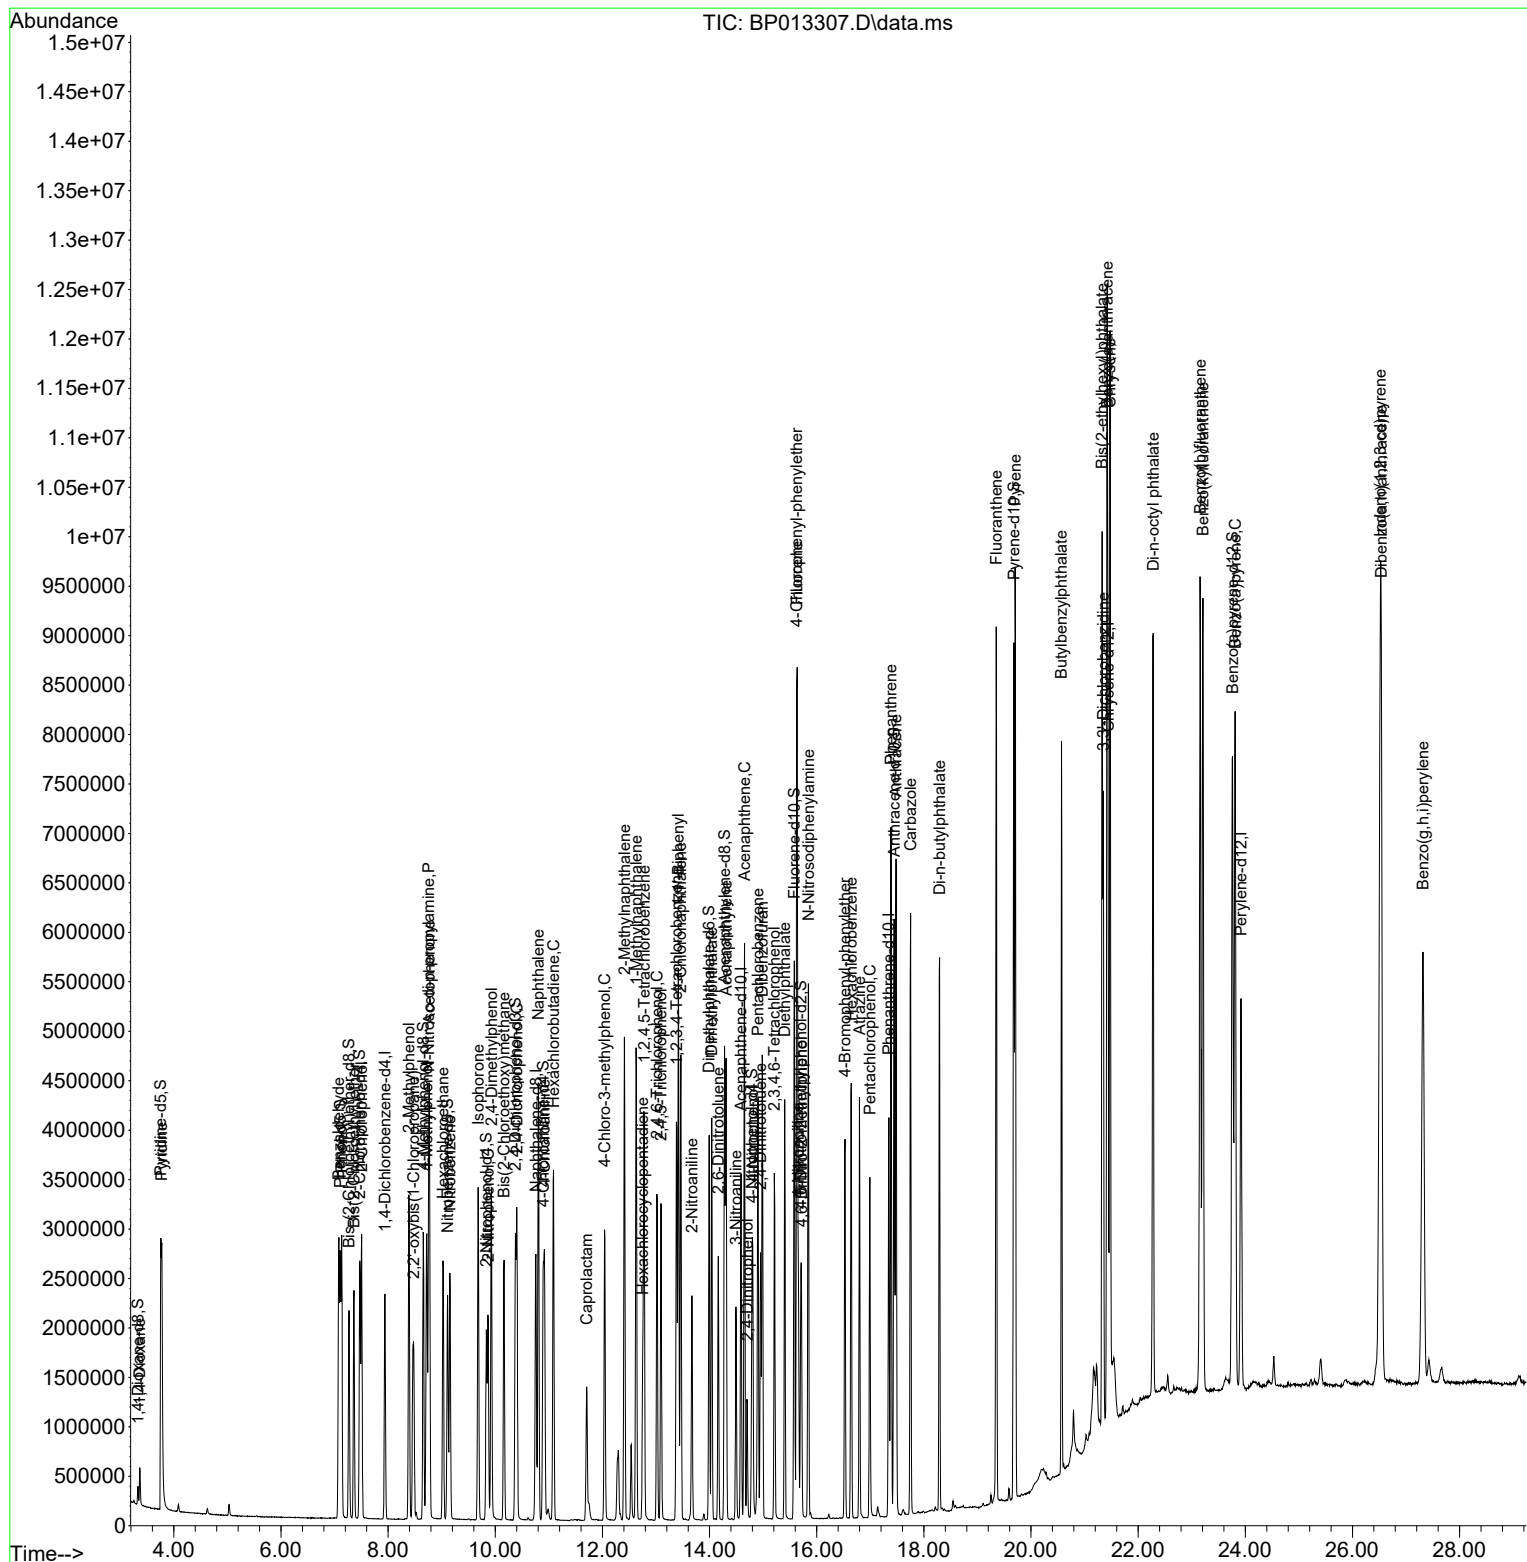

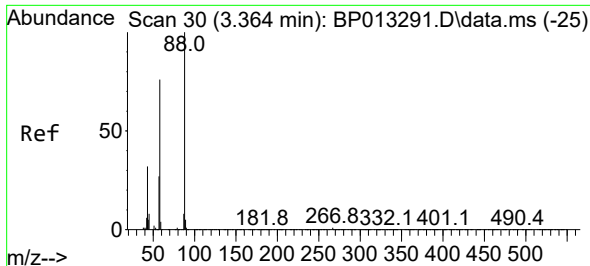




#2
 1,4-Dioxane
 Concen: 11.673 ng/uL
 RT: 3.364 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Instrument :
 BNA_P
 ClientSampleId :

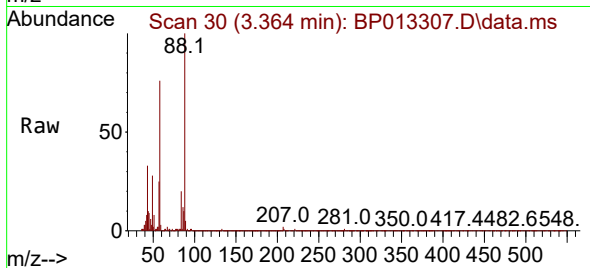

Tgt Ion: 88 Resp: 170297




Ion	Ratio	Lower	Upper
88	100		
43	33.3	22.4	33.6
58	75.8	58.2	87.4

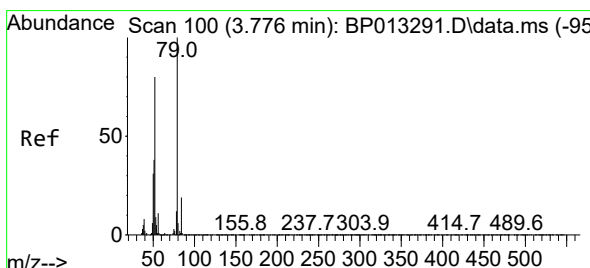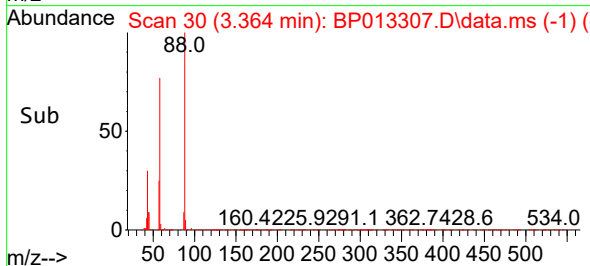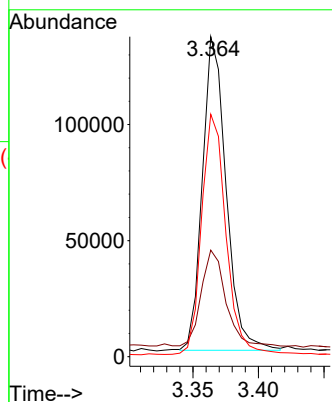


#5
 Pyridine
 Concen: 30.232 ng/uL
 RT: 3.775 min Scan# 100
 Delta R.T. -0.006 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Tgt Ion: 79 Resp: 1192784

Ion	Ratio	Lower	Upper
79	100		
52	79.2	60.7	91.1
51	38.8	28.9	43.3


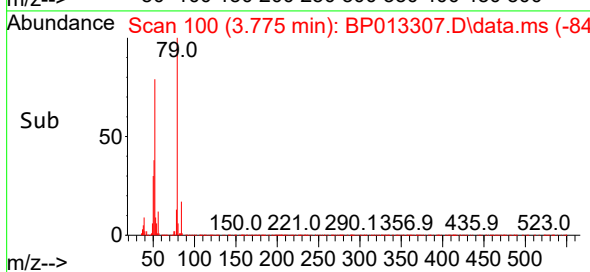
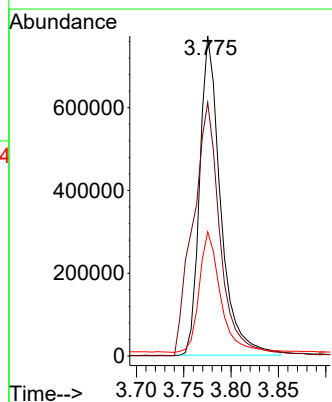
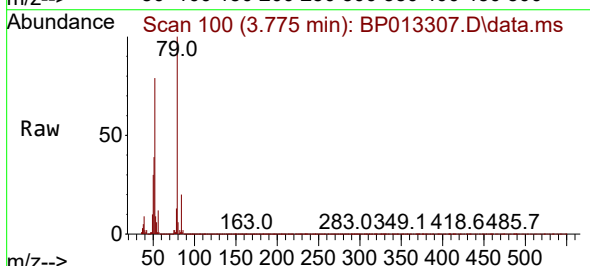




#6
Benzaldehyde
Concen: 48.074 ng/ul
RT: 7.075 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 916166
Ion Ratio Lower Upper
77 100
105 97.4 81.5 122.3
106 94.0 76.9 115.3



#8
Phenol
Concen: 30.213 ng/ul
RT: 7.134 min Scan# 671
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion: 94 Resp: 1486741
Ion Ratio Lower Upper
94 100
65 28.1 21.1 31.7
66 35.5 27.0 40.6

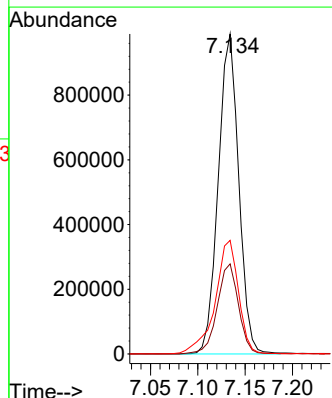







#10
 Bis(2-Chloroethyl)ether
 Concen: 29.860 ng/ul
 RT: 7.363 min Scan# 710
 Delta R.T. 0.000 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Instrument :
 BNA_P
 ClientSampleId :

Tgt Ion: 93 Resp: 1206014




Ion	Ratio	Lower	Upper
93	100		
63	77.4	59.8	89.8
95	32.6	26.4	39.6

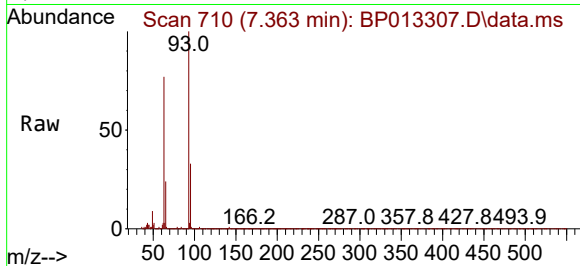


#12
 2-Chlorophenol
 Concen: 30.792 ng/ul
 RT: 7.505 min Scan# 734
 Delta R.T. 0.000 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Tgt Ion: 128 Resp: 1209799

Ion	Ratio	Lower	Upper
128	100		
64	47.3	34.9	52.3
130	32.9	25.8	38.6

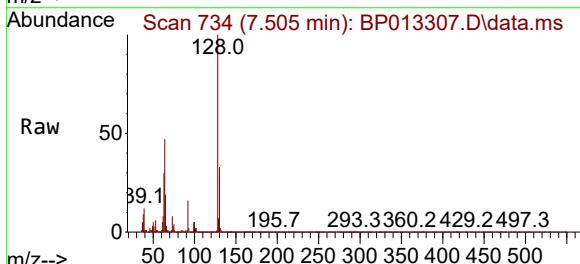



#13

2-Methylphenol

Concen: 28.734 ng/ul

RT: 8.387 min Scan# 884

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 1102360

Ion Ratio Lower Upper

108 100

107 87.8 69.1 103.7

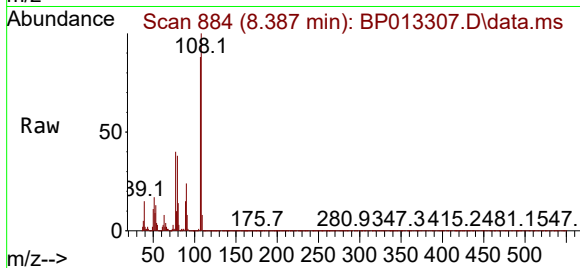

#14

2,2'-oxybis(1-Chloropropane)

Concen: 31.622 ng/ul

RT: 8.475 min Scan# 899

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion: 45 Resp: 1752585


Ion Ratio Lower Upper

45 100

77 13.3 11.0 16.6

79 10.4 9.3 13.9


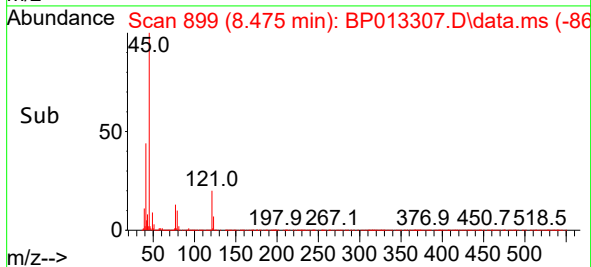

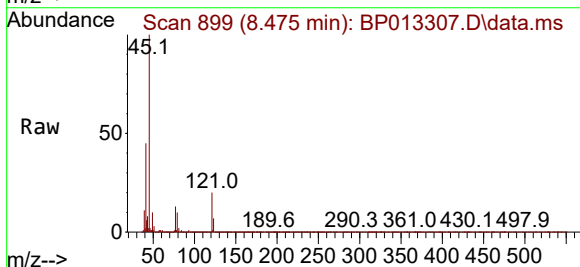




#16
Acetophenone
Concen: 28.049 ng/ul
RT: 8.769 min Scan# 949
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:105 Resp: 1715124
Ion Ratio Lower Upper
105 100
77 77.5 59.3 88.9
51 29.2 19.6 29.4



#17
N-Nitroso-di-n-propylamine
Concen: 28.236 ng/ul
RT: 8.757 min Scan# 947
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion: 70 Resp: 868199
Ion Ratio Lower Upper
70 100
42 61.2 45.5 68.3
101 9.5 7.9 11.9
130 21.7 17.4 26.2



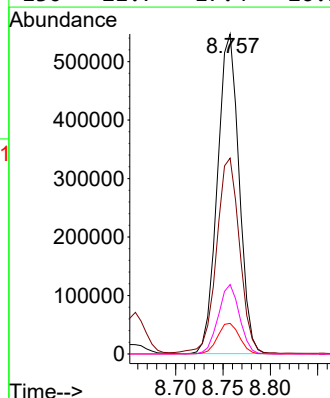





#18
4-Methylphenol
Concen: 27.058 ng/ul
RT: 8.722 min Scan# 940
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 1149812
Ion Ratio Lower Upper
108 100
107 109.8 87.4 131.2



#19
Hexachloroethane
Concen: 30.714 ng/ul
RT: 9.022 min Scan# 992
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:117 Resp: 482235
Ion Ratio Lower Upper
117 100
201 114.7 93.7 140.5
199 71.8 58.6 88.0









#22
Nitrobenzene
Concen: 33.838 ng/ul
RT: 9.152 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 1292309
Ion Ratio Lower Upper
77 100
123 46.6 38.3 57.5
65 13.5 10.3 15.5



#23
Isophorone
Concen: 29.886 ng/ul
RT: 9.681 min Scan# 1104
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion: 82 Resp: 2307884
Ion Ratio Lower Upper
82 100
95 7.0 5.4 8.2
138 17.8 15.3 22.9









#25
2-Nitrophenol
Concen: 32.835 ng/ul
RT: 9.869 min Scan# 1136
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:139 Resp: 651872
Ion Ratio Lower Upper
139 100
65 49.5 36.6 54.8
109 28.5 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 29.568 ng/ul
RT: 9.928 min Scan# 1146
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:107 Resp: 1145361
Ion Ratio Lower Upper
107 100
121 51.1 41.8 62.6
122 87.0 72.6 108.8



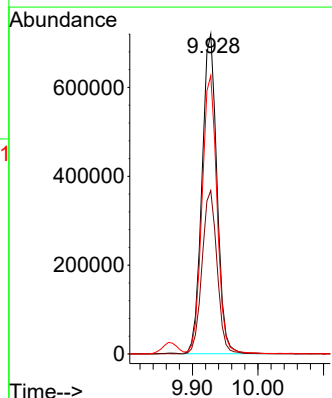





#27
 Bis(2-Chloroethoxy)methane
 Concen: 29.622 ng/ul
 RT: 10.163 min Scan# 1186
 Delta R.T. 0.000 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 1462664
 Ion Ratio Lower Upper
 93 100
 95 32.9 26.0 39.0
 123 11.4 9.2 13.8



#29
 2,4-Dichlorophenol
 Concen: 30.970 ng/ul
 RT: 10.404 min Scan# 1227
 Delta R.T. 0.000 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Tgt Ion:162 Resp: 1079689
 Ion Ratio Lower Upper
 162 100
 164 65.5 52.5 78.7
 98 33.1 26.6 39.8









#30
Naphthalene
Concen: 30.484 ng/ul
RT: 10.804 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 3531550
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 13.1 10.4 15.6



#32
4-Chloroaniline
Concen: 24.462 ng/ul
RT: 10.916 min Scan# 1314
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:127 Resp: 1216201
Ion Ratio Lower Upper
127 100
129 31.8 25.6 38.4





#33

Hexachlorobutadiene

Concen: 33.445 ng/ul

RT: 11.087 min Scan# 11

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:225 Resp: 800550

Ion Ratio Lower Upper

225 100

223 62.1 49.2 73.8

227 63.1 50.2 75.2

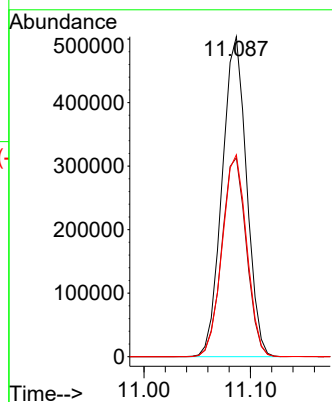

#34

Caprolactam

Concen: 23.265 ng/ul

RT: 11.704 min Scan# 1448

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:113 Resp: 276550


Ion Ratio Lower Upper

113 100

55 182.3 141.9 212.9

56 135.5 99.6 149.4









#35
 4-Chloro-3-methylphenol
 Concen: 27.338 ng/ul
 RT: 12.040 min Scan# 1505
 Delta R.T. -0.006 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion:107 Resp: 972638
 Ion Ratio Lower Upper
 107 100
 144 26.5 21.4 32.2
 142 83.2 65.8 98.6

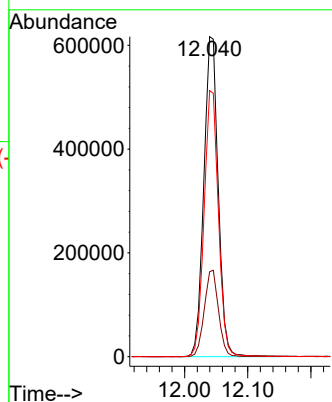

#36
 2-Methylnaphthalene
 Concen: 27.992 ng/ul
 RT: 12.410 min Scan# 1568
 Delta R.T. -0.006 min
 Lab File: BP013307.D
 Acq: 24 Dec 2022 19:12

Tgt Ion:142 Resp: 2224669
 Ion Ratio Lower Upper
 142 100
 141 87.9 70.8 106.2





#37

1-Methylnaphthalene

Concen: 26.911 ng/ul

RT: 12.628 min Scan# 1605

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:142 Resp: 2199474

Ion Ratio Lower Upper

142 100

141 91.3 72.7 109.1

116 3.7 2.7 4.1

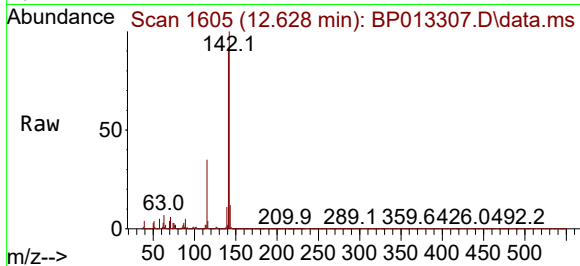

#39

1,2,4,5-Tetrachlorobenzene

Concen: 35.577 ng/ul

RT: 12.781 min Scan# 1631

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Tgt Ion:216 Resp: 1325820




Ion Ratio Lower Upper


216 100

214 78.6 61.9 92.9

179 19.3 15.0 22.6

108 14.2 11.0 16.4

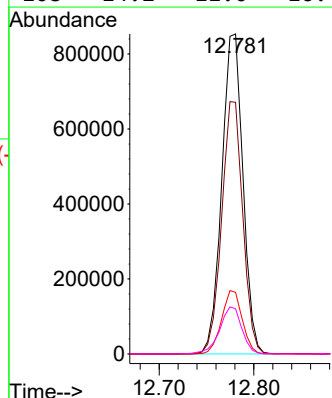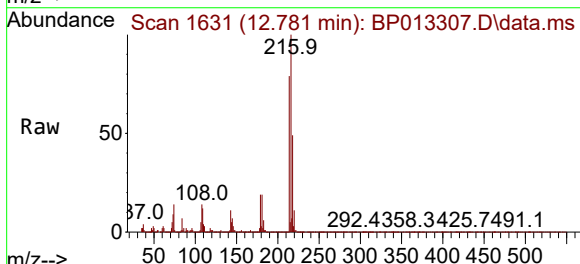



#40

Hexachlorocyclopentadiene

Concen: 16.685 ng/ul

RT: 12.751 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 404626

Ion Ratio Lower Upper

237 100

235 63.2 49.7 74.5

272 13.7 10.8 16.2

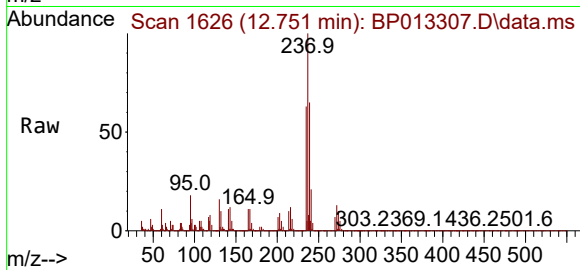

#41

2,4,6-Trichlorophenol

Concen: 33.888 ng/ul

RT: 13.022 min Scan# 1672

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:196 Resp: 811614


Ion Ratio Lower Upper

196 100

198 98.4 77.0 115.6


200 31.4 25.3 37.9

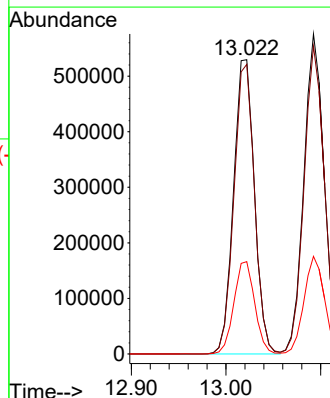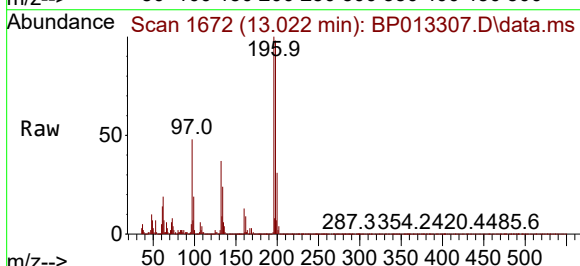






#42
2,4,5-Trichlorophenol
Concen: 33.296 ng/ul
RT: 13.092 min Scan# 1
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:196 Resp: 856576
Ion Ratio Lower Upper
196 100
198 96.2 77.1 115.7
200 30.5 25.4 38.2



#43
1,1'-Biphenyl
Concen: 32.555 ng/ul
RT: 13.416 min Scan# 1739
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:154 Resp: 2829683
Ion Ratio Lower Upper
154 100
153 39.9 31.5 47.3
76 12.9 9.6 14.4

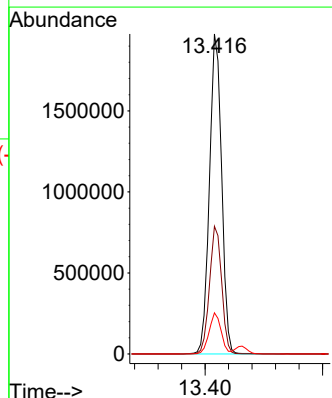



#44

2-Chloronaphthalene

Concen: 32.940 ng/ul

RT: 13.463 min Scan# 1747

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:162 Resp: 2253436

Ion Ratio Lower Upper

162 100

164 33.2 26.3 39.5

127 36.1 29.3 43.9



#45

2-Nitroaniline

Concen: 36.075 ng/ul

RT: 13.669 min Scan# 1782

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion: 65 Resp: 598340


Ion Ratio Lower Upper

65 100

92 67.2 56.4 84.6

138 106.1 90.3 135.5









#47
Dimethylphthalate
Concen: 29.053 ng/ul
RT: 14.040 min Scan# 1845
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:163 Resp: 2561231
Ion Ratio Lower Upper
163 100
194 4.5 3.4 5.0
164 10.4 8.3 12.5

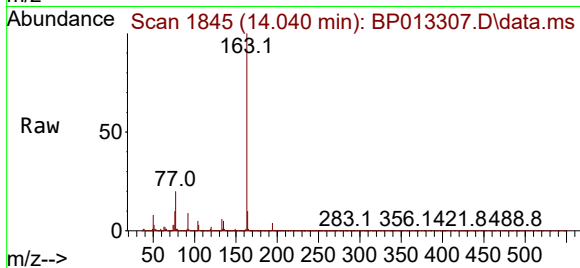

#48
2,6-Dinitrotoluene
Concen: 32.002 ng/ul
RT: 14.163 min Scan# 1866
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:165 Resp: 524308
Ion Ratio Lower Upper
165 100
89 52.4 43.0 64.4
121 19.3 16.1 24.1


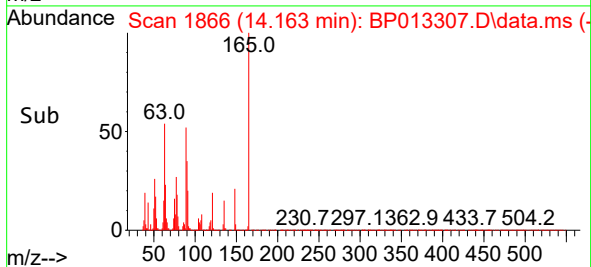

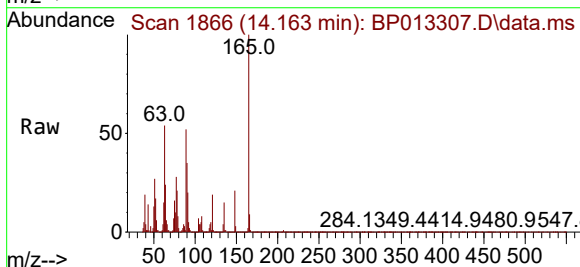




#50
Acenaphthylene
Concen: 31.404 ng/ul
RT: 14.310 min Scan# 1891
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:152 Resp: 3299835
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 12.8 10.6 16.0

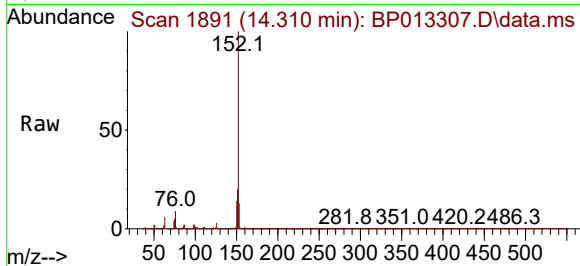

#51
3-Nitroaniline
Concen: 33.802 ng/ul
RT: 14.492 min Scan# 1922
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:138 Resp: 522919
Ion Ratio Lower Upper
138 100
108 9.9 8.6 13.0
92 111.2 88.4 132.6



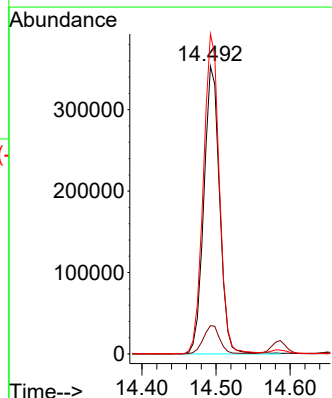
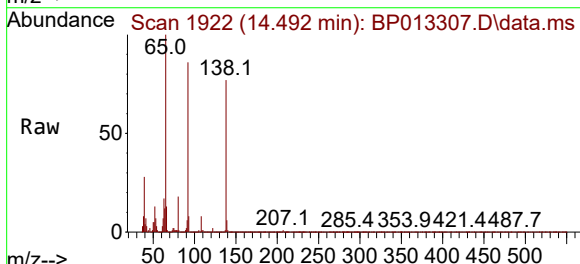




#52
Acenaphthene
Concen: 30.875 ng/ul
RT: 14.651 min Scan# 1949
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:153 Resp: 2248151
Ion Ratio Lower Upper
153 100
152 48.1 38.2 57.4
154 89.0 70.8 106.2

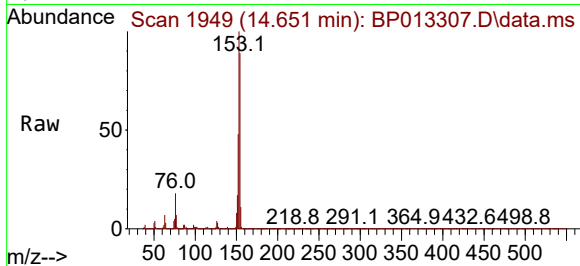

#53
2,4-Dinitrophenol
Concen: 22.759 ng/ul
RT: 14.704 min Scan# 1958
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:184 Resp: 254882
Ion Ratio Lower Upper
184 100
63 58.8 48.4 72.6
154 58.1 45.5 68.3



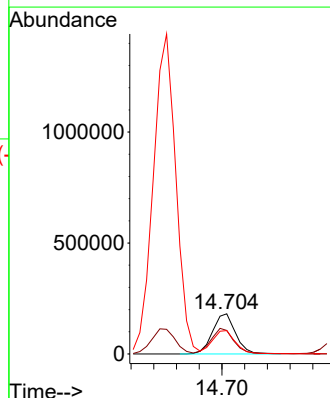
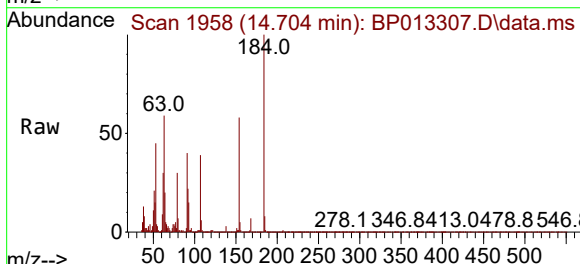


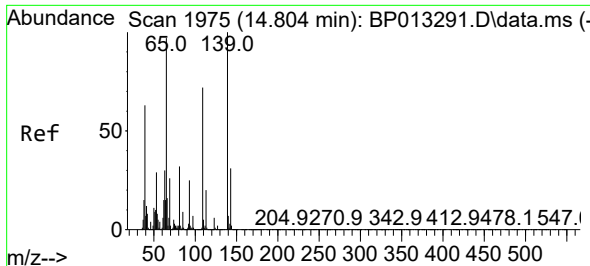

#55
4-Nitrophenol
Concen: 33.132 ng/ul
RT: 14.804 min Scan# 1975
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:109 Resp: 361706
Ion Ratio Lower Upper
109 100
139 136.7 120.8 181.2
65 137.5 107.9 161.9

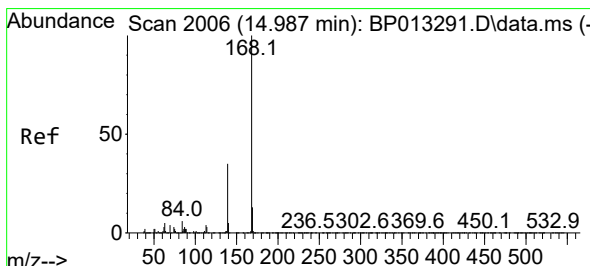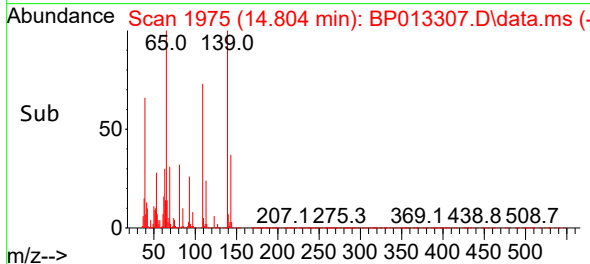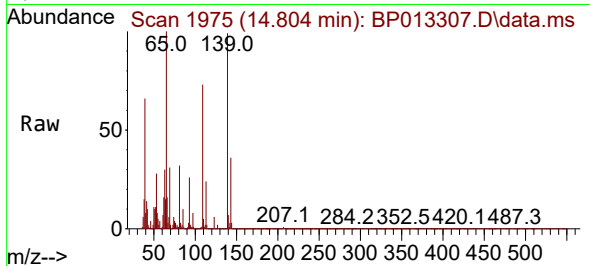

#56
Dibenzofuran
Concen: 30.166 ng/ul
RT: 14.986 min Scan# 2006
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:168 Resp: 3123002
Ion Ratio Lower Upper
168 100
139 34.6 27.9 41.9

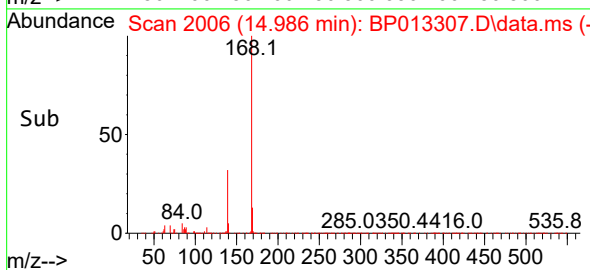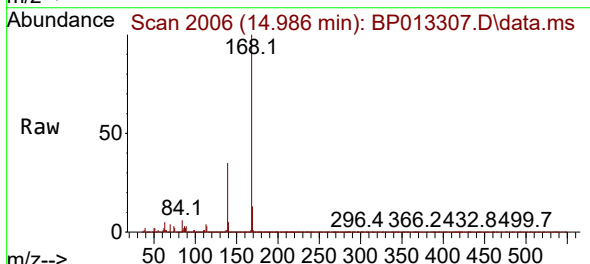



#57

2,4-Dinitrotoluene

Concen: 30.649 ng/ul

RT: 14.951 min Scan# 2000

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:165 Resp: 729387

Ion Ratio Lower Upper

165 100

63 41.6 31.8 47.6

182 2.6 2.1 3.1



#58

2,3,4,6-Tetrachlorophenol

Concen: 30.876 ng/ul

RT: 15.210 min Scan# 2044

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Tgt Ion:232 Resp: 724888




Ion Ratio Lower Upper


232 100

131 38.1 31.8 47.6

130 2.0 1.8 2.6

166 27.1 22.9 34.3



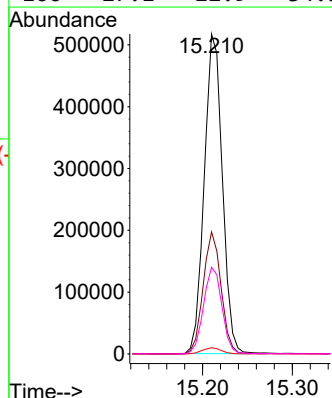





#59
Diethylphthalate
Concen: 27.665 ng/ul
RT: 15.404 min Scan# 2077
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:149 Resp: 2370877
Ion Ratio Lower Upper
149 100
177 23.3 18.4 27.6
150 12.4 9.9 14.9



#61
Fluorene
Concen: 30.229 ng/ul
RT: 15.634 min Scan# 2116
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:166 Resp: 2509820
Ion Ratio Lower Upper
166 100
165 97.7 77.4 116.2
167 13.3 10.6 16.0









#62
4-Chlorophenyl-phenylether
Concen: 29.858 ng/ul
RT: 15.628 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 1310981
Ion Ratio Lower Upper
204 100
206 32.8 26.3 39.5
141 51.5 40.4 60.6



#63
4-Nitroaniline
Concen: 42.252 ng/ul
RT: 15.657 min Scan# 2120
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:138 Resp: 575183
Ion Ratio Lower Upper
138 100
92 49.6 39.0 58.4
108 75.4 55.1 82.7







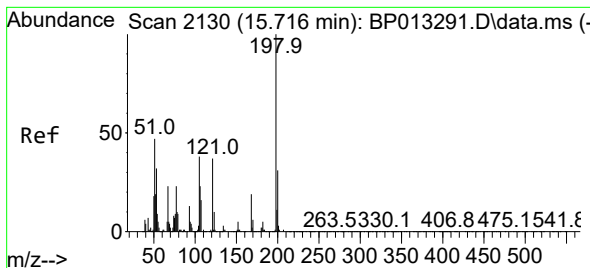

#66
4,6-Dinitro-2-methylphenol
Concen: 26.191 ng/ul
RT: 15.716 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 401309
Ion Ratio Lower Upper
198 100
182 4.3 3.3 4.9
77 23.2 16.6 25.0

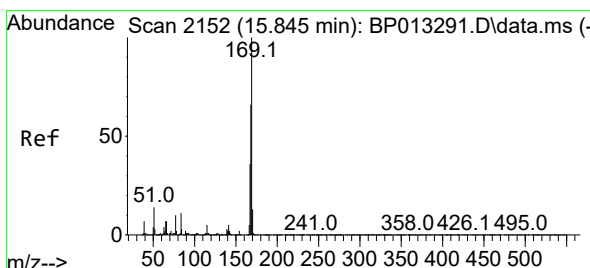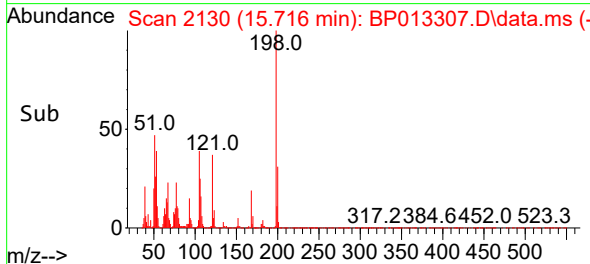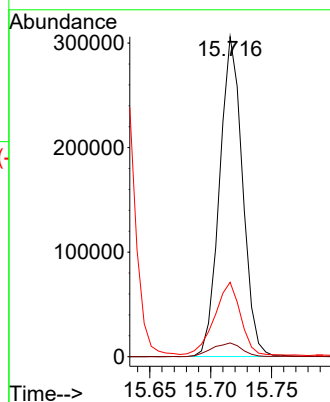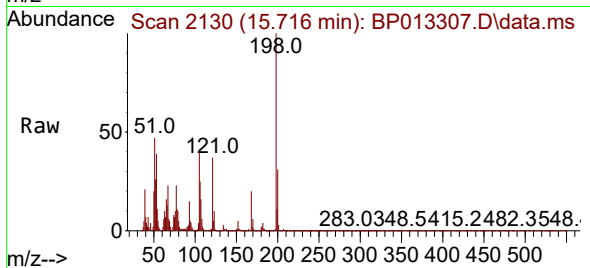

#67
N-Nitrosodiphenylamine
Concen: 30.749 ng/ul
RT: 15.845 min Scan# 2152
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:169 Resp: 2077073
Ion Ratio Lower Upper
169 100
168 64.9 53.0 79.6
167 35.9 29.1 43.7


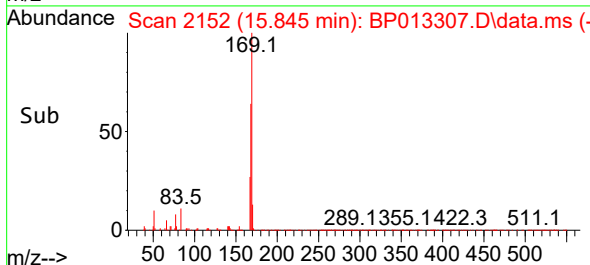

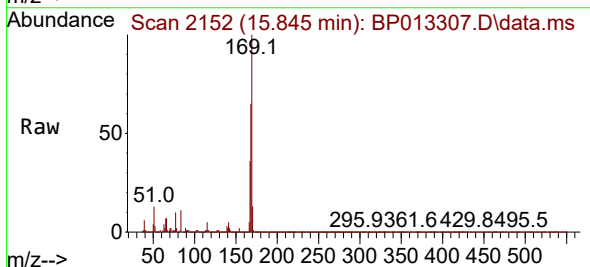




#68
4-Bromophenyl-phenylether
Concen: 29.719 ng/ul
RT: 16.528 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 786351
Ion Ratio Lower Upper
248 100
250 97.7 77.4 116.0
141 58.7 48.3 72.5



#69
Hexachlorobenzene
Concen: 30.708 ng/ul
RT: 16.645 min Scan# 2288
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:284 Resp: 964799
Ion Ratio Lower Upper
284 100
142 27.5 22.6 34.0
249 30.3 24.6 37.0





#70

Atrazine

Concen: 28.742 ng/ul

RT: 16.798 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:200 Resp: 756574

Ion Ratio Lower Upper

200 100

173 25.4 20.5 30.7

215 51.0 39.9 59.9

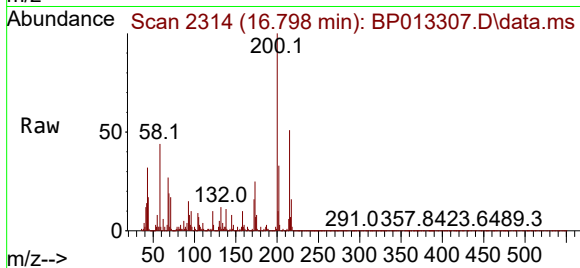

#71

Pentachlorophenol

Concen: 32.516 ng/ul

RT: 16.992 min Scan# 2347

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:266 Resp: 618669


Ion Ratio Lower Upper

266 100

264 63.6 50.9 76.3

268 63.7 51.4 77.2

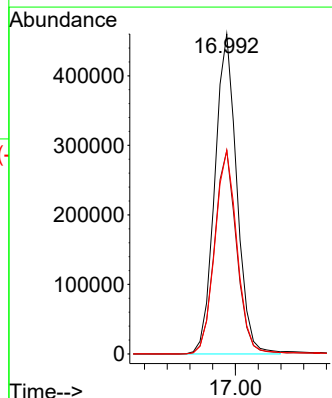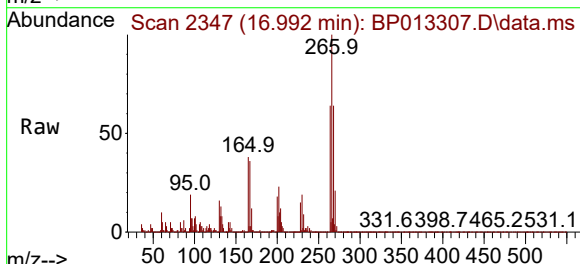



#72

Phenanthrene

Concen: 31.752 ng/ul

RT: 17.386 min Scan# 2414

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 4029563

Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 19.2 15.4 23.0

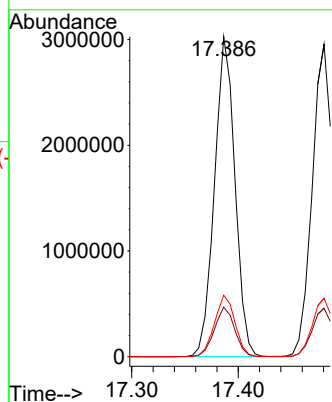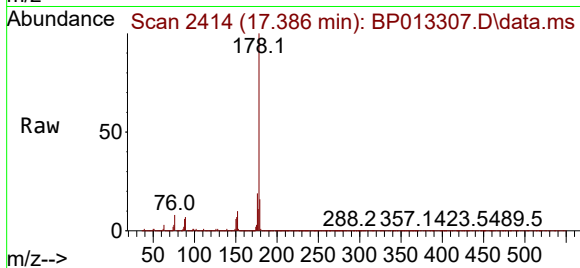

#74

Anthracene

Concen: 32.049 ng/ul

RT: 17.480 min Scan# 2430

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:178 Resp: 4061165


Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 18.7 14.8 22.2




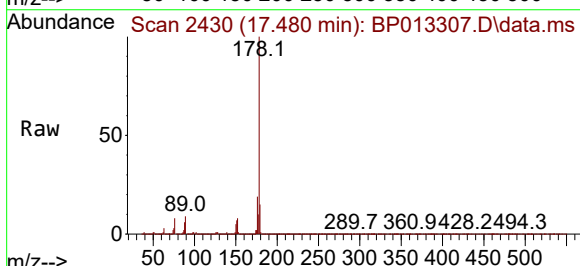




#75
1,2,3,4-Tetrachlorobenzene
Concen: 37.296 ng/uL
RT: 13.387 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:216 Resp: 1296496
Ion Ratio Lower Upper
216 100
214 78.4 62.2 93.2
218 49.2 38.9 58.3

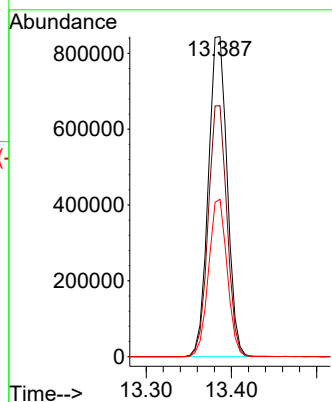

#76
Pentachlorobenzene
Concen: 31.995 ng/uL
RT: 14.904 min Scan# 1992
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:250 Resp: 1133968
Ion Ratio Lower Upper
250 100
248 63.3 50.6 76.0
252 64.0 51.1 76.7





#77

Carbazole

Concen: 35.497 ng/ul

RT: 17.751 min Scan# 2476

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:167 Resp: 3788098

Ion Ratio Lower Upper

167 100

166 21.3 17.2 25.8

139 12.2 9.4 14.2

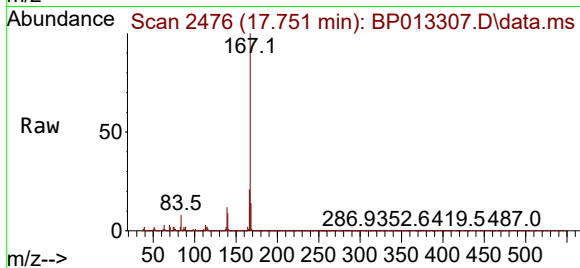

#78

Di-n-butylphthalate

Concen: 30.277 ng/ul

RT: 18.292 min Scan# 2568

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:149 Resp: 3934042


Ion Ratio Lower Upper

149 100

150 9.0 7.5 11.3

104 4.8 3.8 5.6




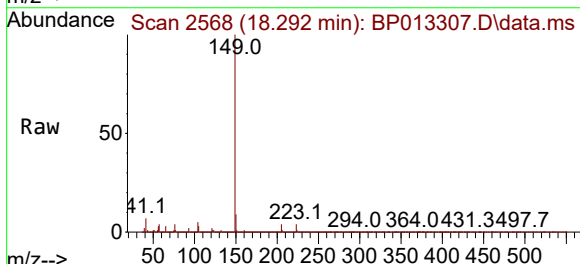




#80
Fluoranthene
Concen: 29.741 ng/ul
RT: 19.351 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:202 Resp: 5290750
Ion Ratio Lower Upper
202 100
101 10.1 8.2 12.2
100 7.5 6.1 9.1



#82
Pyrene
Concen: 30.426 ng/ul
RT: 19.704 min Scan# 2808
Delta R.T. -0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:202 Resp: 5583436
Ion Ratio Lower Upper
202 100
101 11.6 9.4 14.2
100 9.6 7.8 11.8





#83

Butylbenzylphthalate

Concen: 29.613 ng/ul

RT: 20.569 min Scan# 2956

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 2099380

Ion Ratio Lower Upper

149 100

91 70.0 53.4 80.0

206 22.8 17.9 26.9

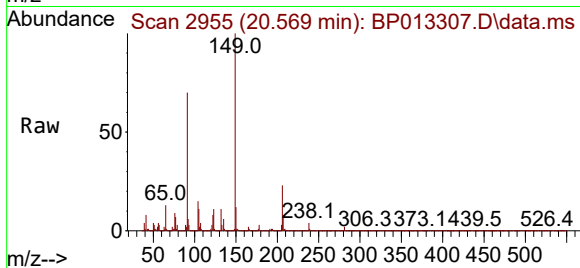

#84

3,3'-Dichlorobenzidine

Concen: 32.280 ng/ul

RT: 21.351 min Scan# 3088

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:252 Resp: 1991278


Ion Ratio Lower Upper

252 100

254 65.4 51.8 77.8

126 8.5 7.4 11.2

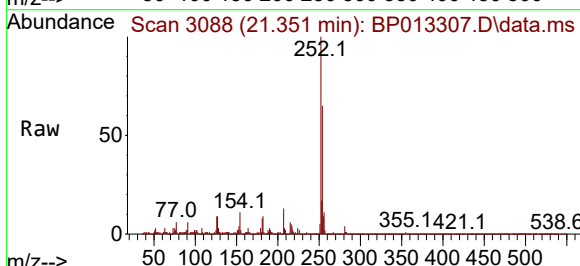



#85

Benzo(a)anthracene

Concen: 32.599 ng/ul

RT: 21.421 min Scan# 3100

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 5909401

Ion Ratio Lower Upper

228 100

229 20.2 16.1 24.1

226 27.8 22.0 33.0

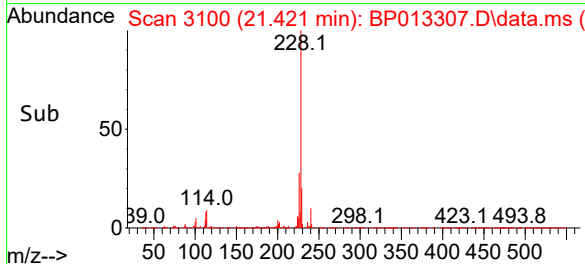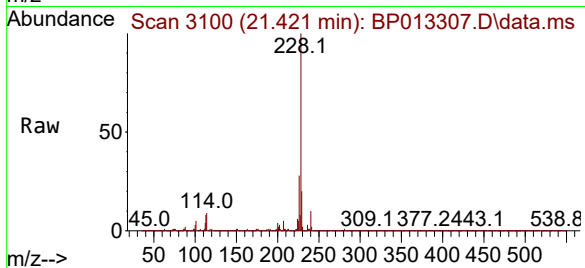

#86

Bis(2-ethylhexyl)phthalate

Concen: 30.053 ng/ul

RT: 21.327 min Scan# 3084

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:149 Resp: 3005390


Ion Ratio Lower Upper

149 100

167 28.1 22.5 33.7

279 5.0 3.8 5.8

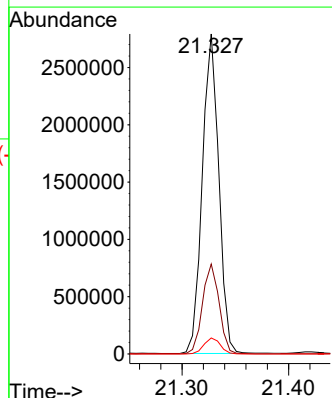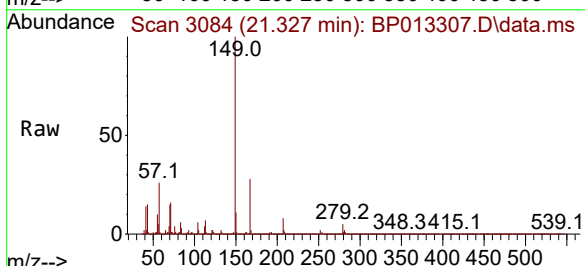



#87

Chrysene

Concen: 32.092 ng/ul

RT: 21.474 min Scan# 3109

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 5501342

Ion Ratio Lower Upper

228 100

226 31.0 24.5 36.7

229 20.3 16.0 24.0



#89

Di-n-octyl phthalate

Concen: 31.029 ng/ul




RT: 22.280 min Scan# 3246


Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Tgt Ion:149 Resp: 5513120


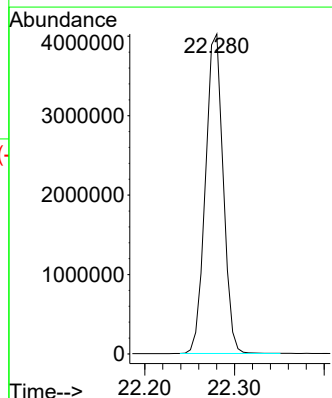
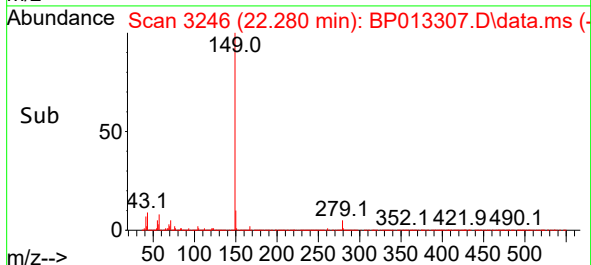
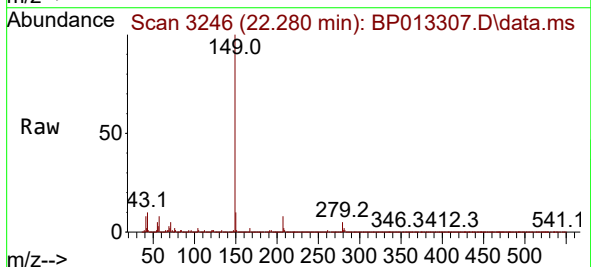




#90
Benzo(b)fluoranthene
Concen: 30.762 ng/ul
RT: 23.157 min Scan# 31
Delta R.T. 0.000 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:252 Resp: 6221221
Ion Ratio Lower Upper
252 100
253 22.3 17.7 26.5
125 8.7 6.8 10.2

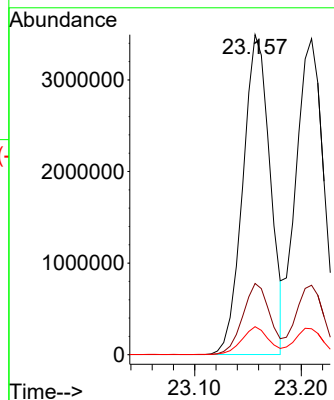

#91
Benzo(k)fluoranthene
Concen: 31.092 ng/ul
RT: 23.210 min Scan# 3404
Delta R.T. 0.006 min
Lab File: BP013307.D
Acq: 24 Dec 2022 19:12

Tgt Ion:252 Resp: 6235179
Ion Ratio Lower Upper
252 100
253 22.0 17.7 26.5
125 8.2 6.8 10.2

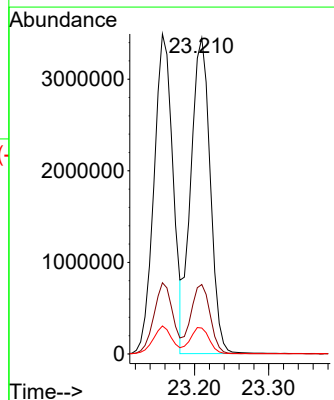



#93

Benzo(a)pyrene

Concen: 31.993 ng/ul

RT: 23.810 min Scan# 3506

Delta R.T. 0.000 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 5633684

Ion Ratio Lower Upper

252 100

253 22.0 17.5 26.3

125 9.1 7.5 11.3

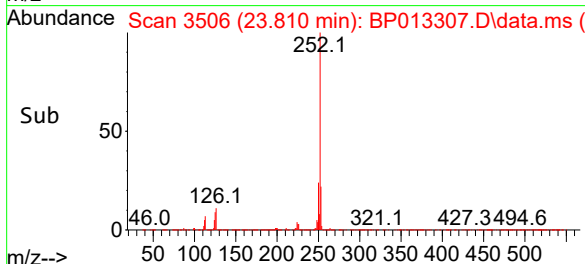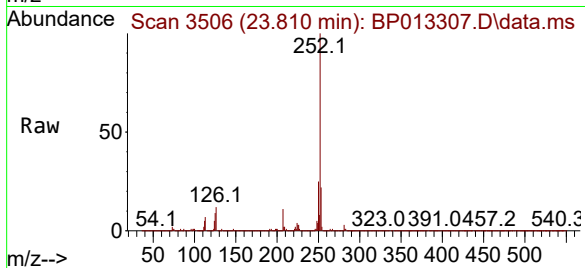

#94

Indeno(1,2,3-cd)pyrene

Concen: 33.929 ng/ul

RT: 26.521 min Scan# 3967

Delta R.T. 0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12




Tgt Ion:276 Resp: 7442173


Ion Ratio Lower Upper

276 100

138 20.6 17.1 25.7

277 25.5 20.0 30.0

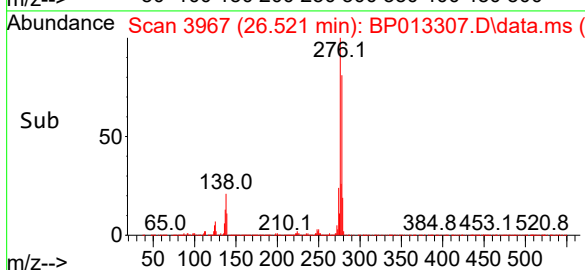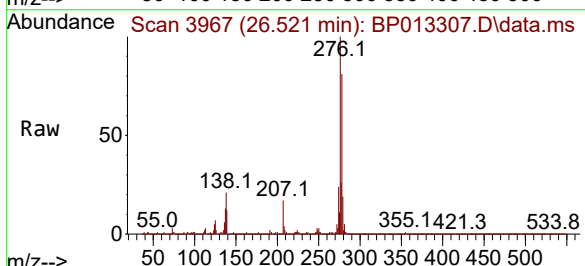



#95

Dibenzo(a,h)anthracene

Concen: 34.801 ng/ul

RT: 26.539 min Scan# 3970

Delta R.T. 0.012 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:278 Resp: 6320155

Ion Ratio Lower Upper

278 100

139 12.8 11.1 16.7

279 23.5 19.0 28.6



#96

Benzo(g,h,i)perylene

Concen: 34.812 ng/ul

RT: 27.315 min Scan# 4102

Delta R.T. 0.006 min

Lab File: BP013307.D

Acq: 24 Dec 2022 19:12

Tgt Ion:276 Resp: 6130042

Ion Ratio Lower Upper

276 100

138 18.1 15.4 23.2

277 23.8 19.1 28.7

