

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013311.D
 Acq On : 24 Dec 2022 22:01
 Operator : CG/JU
 Sample : N6016-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 00:25:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	664635	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	2552570	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1329095	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	2572354	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2846071	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	3258388	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	52236	3.360	ng/uL	0.00
4) Pyridine-d5	3.770	84	94210	2.134	ng/ul	0.01
7) Phenol-d5	7.099	99	957517	17.687	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.264	67	657460	20.132	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	824334	19.343	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	525296	11.842	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	393974	21.007	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	429500	20.342	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	737448	17.982	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	572282	9.885	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1999785	19.578	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2225415	19.827	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	200902	10.934	ng/ul	0.00
60) Fluorene-d10	15.575	176	1632192	18.887	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	149939	9.058	ng/ul	0.00
73) Anthracene-d10	17.439	188	2308226	19.890	ng/ul	0.00
81) Pyrene-d10	19.675	212	3219442	19.707	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	3385448	20.845	ng/ul	0.00


Target Compounds					Qvalue
16) Acetophenone	8.769	105	89655	1.318 ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013311.D
Acq On : 24 Dec 2022 22:01
Operator : CG/JU
Sample : N6016-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Dec 25 00:25:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

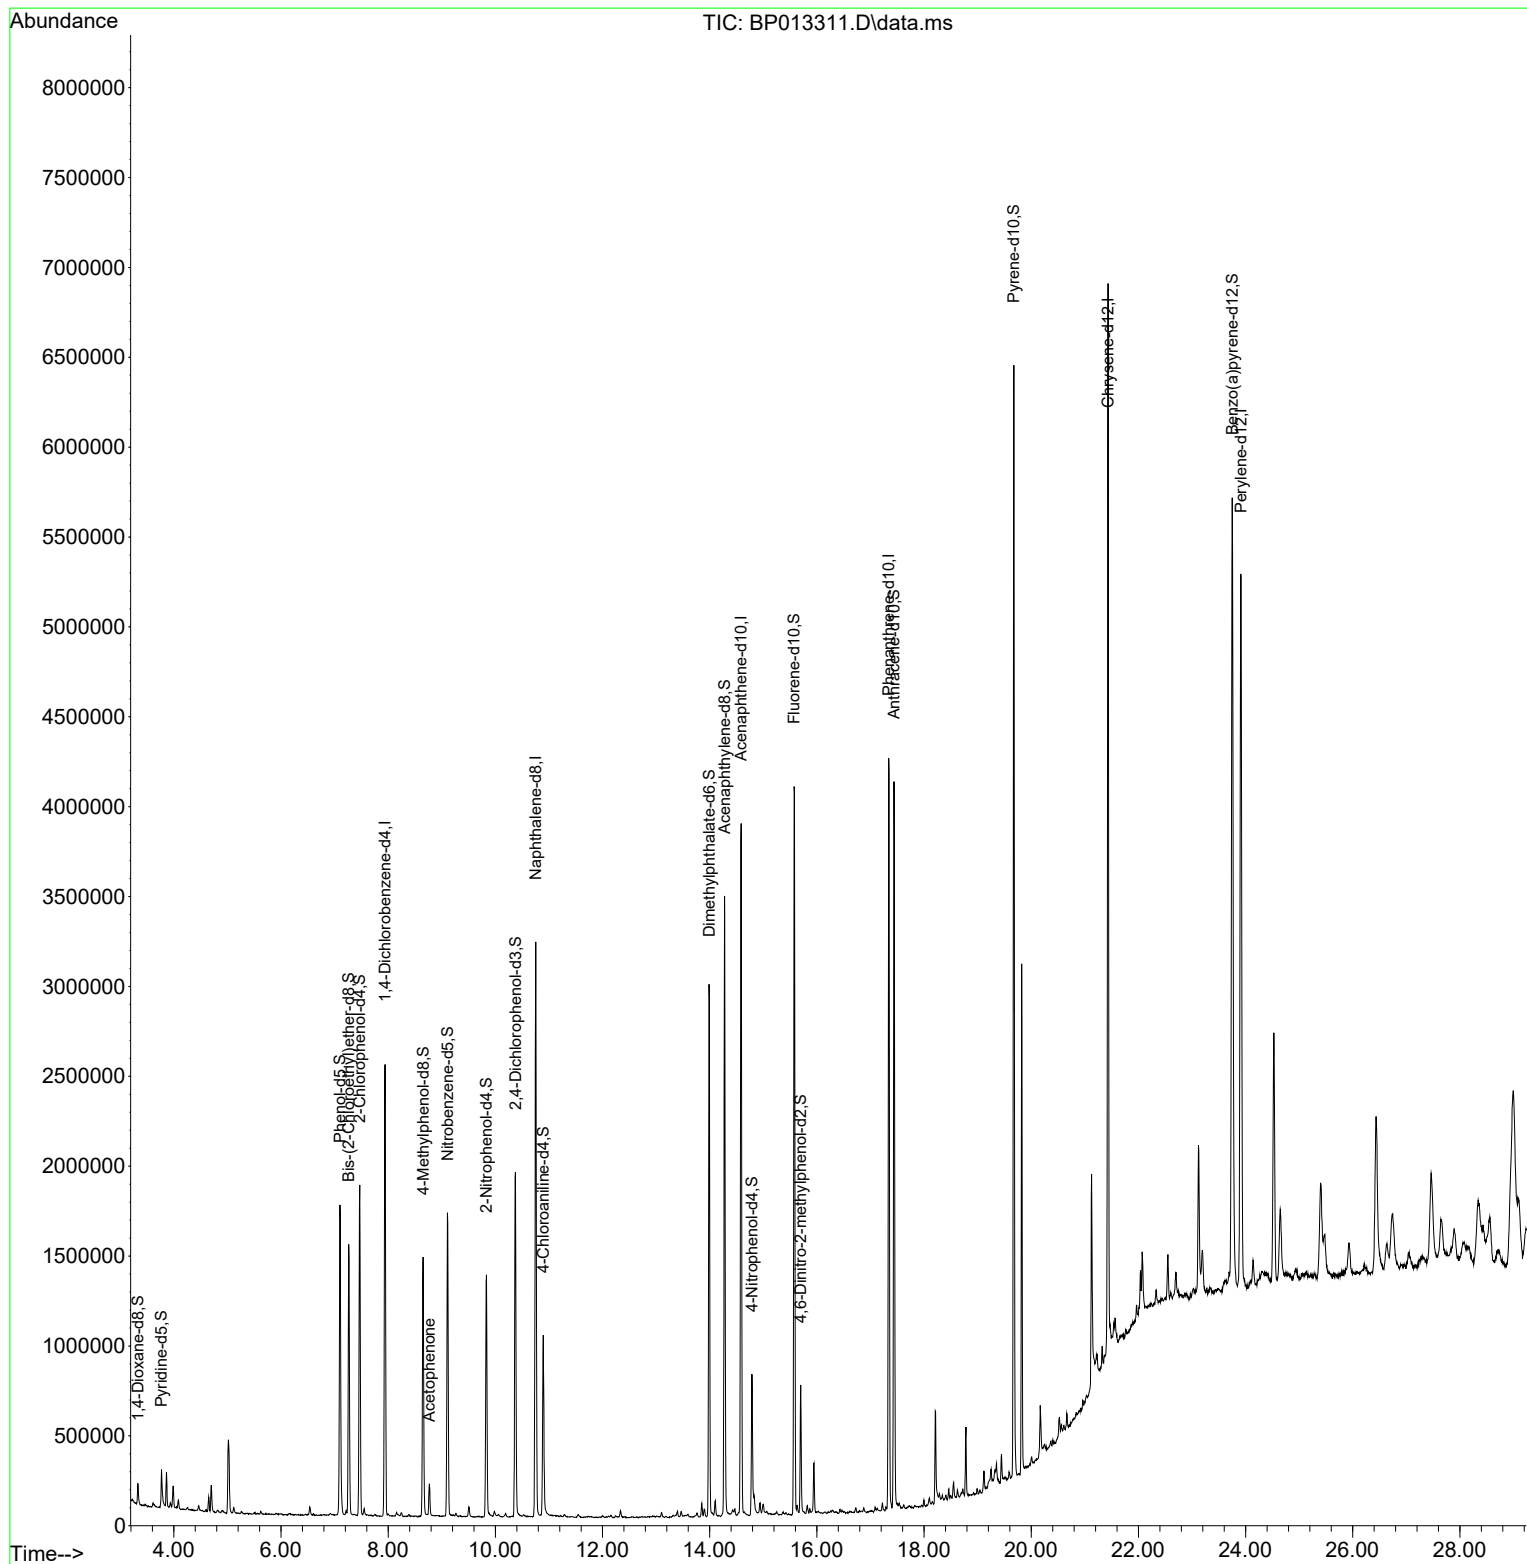

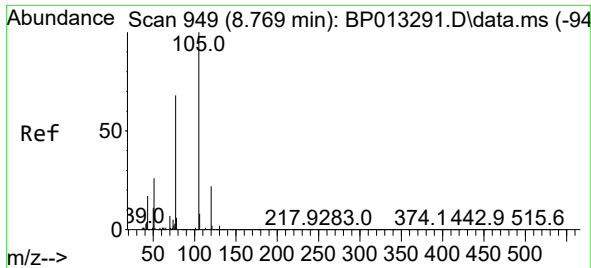

#16
 Acetophenone
 Concen: 1.318 ng/ul
 RT: 8.769 min Scan# 94
 Delta R.T. -0.006 min
 Lab File: BP013311.D
 Acq: 24 Dec 2022 22:01

Instrument :
 BNA_P
 ClientSampleId :

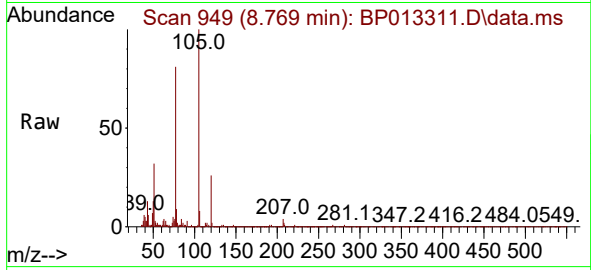

Tgt Ion:	105	Resp:	89655
Ion Ratio	Lower	Upper	
105	100		
77	80.8	59.3	88.9
51	32.4	19.6	29.4#

