

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013325.D
 Acq On : 25 Dec 2022 05:54
 Operator : CG/JU
 Sample : N6018-18
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 21:38:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	605646	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	2351780	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	1262613	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.340	188	2351796	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2458364	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	2862572	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	56115	3.962	ng/uL	0.00
4) Pyridine-d5	3.758	84	460903	11.454	ng/ul	0.00
7) Phenol-d5	7.099	99	1121176	22.727	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.264	67	706270	23.733	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	925155	23.823	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	841217	20.812	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	447538	25.900	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.834	143	497021	25.550	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	902782	23.893	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.893	131	733336	13.748	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	2391231	24.642	ng/ul	-0.01
49) Acenaphthylene-d8	14.275	160	2767864	25.958	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	241565	13.839	ng/ul	0.00
60) Fluorene-d10	15.575	176	1968044	23.973	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	176972	11.693	ng/ul	0.00
73) Anthracene-d10	17.440	188	2802709	26.416	ng/ul	0.00
81) Pyrene-d10	19.675	212	3450282	24.451	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	3684283	25.822	ng/ul	0.00


Target Compounds					Qvalue	
10) Bis(2-Chloroethyl)ether	7.369	93	285706	6.979	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013325.D
Acq On : 25 Dec 2022 05:54
Operator : CG/JU
Sample : N6018-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 25 21:38:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

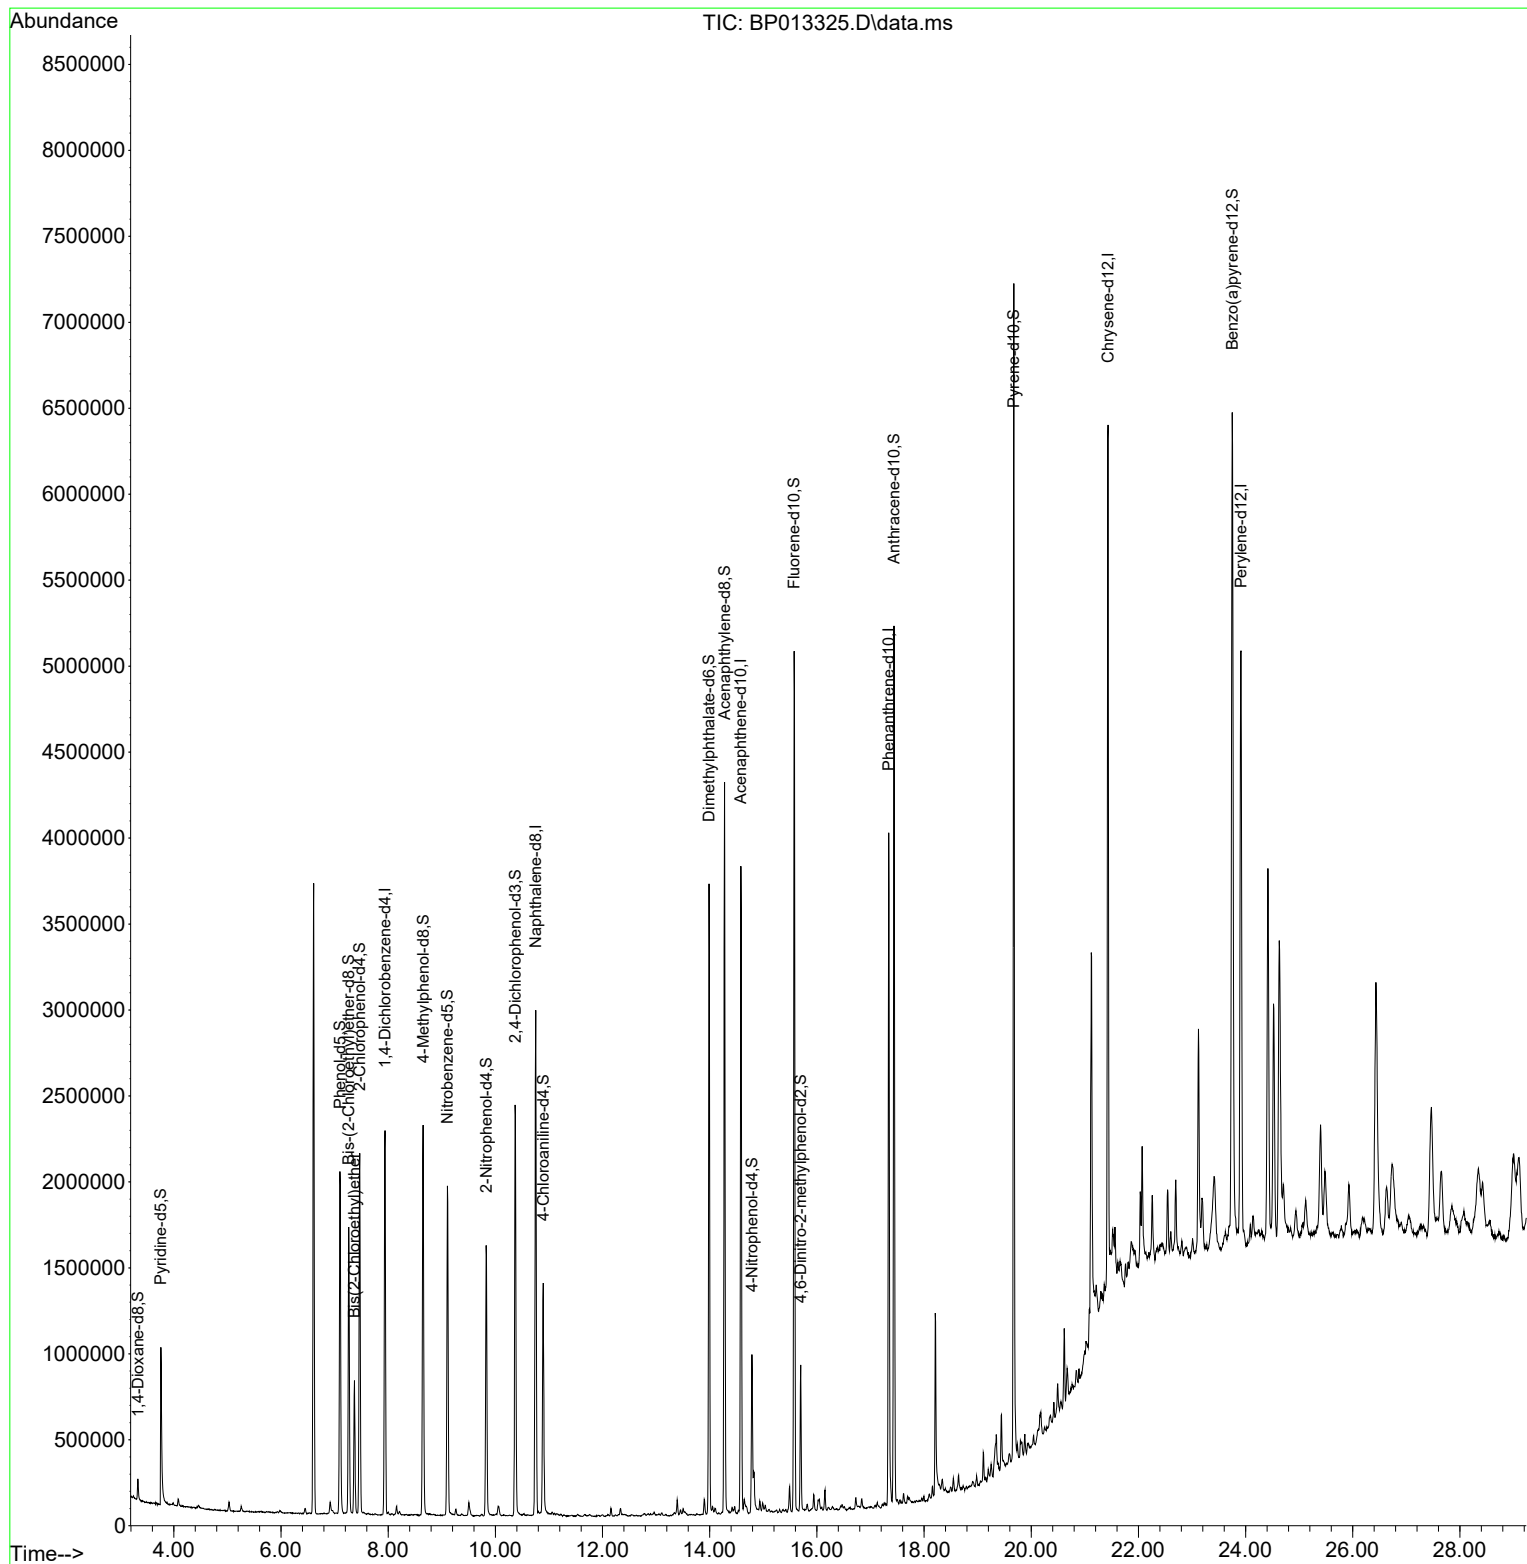

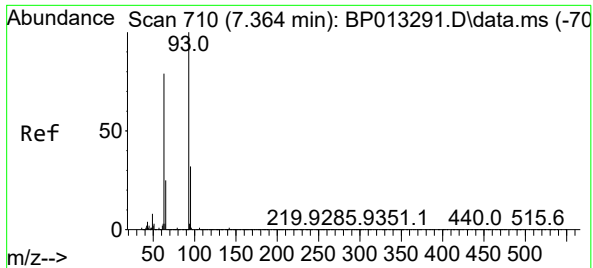

#10
 Bis(2-Chloroethyl)ether
 Concen: 6.979 ng/ul
 RT: 7.369 min Scan# 71
 Delta R.T. 0.006 min
 Lab File: BP013325.D
 Acq: 25 Dec 2022 05:54

Instrument :
 BNA_P
 ClientSampleId :

Tgt Ion: 93 Resp: 285706

Ion	Ratio	Lower	Upper
93	100		
63	2.1	59.8	89.8#
95	2.4	26.4	39.6#

