

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013326.D
 Acq On : 25 Dec 2022 07:02
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 21:38:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	643654	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	2483199	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.586	164	1268641	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	2434787	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	2611060	20.000	ng/u1	0.00
88) Perylene-d12	23.915	264	3048706	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	114396	7.599	ng/uL	0.00
4) Pyridine-d5	3.758	84	849469	19.864	ng/u1	0.00
7) Phenol-d5	7.105	99	1024273	19.537	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	638792	20.198	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	829148	20.090	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	778940	18.133	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	392545	21.516	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	437526	21.301	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	784781	19.671	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	943742	16.756	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	1833945	18.810	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2145788	20.028	ng/u1	0.00
54) 4-Nitrophenol-d4	14.786	143	286832	16.354	ng/u1	0.00
60) Fluorene-d10	15.581	176	1477036	17.906	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	209446	13.367	ng/u1	0.00
73) Anthracene-d10	17.439	188	2170643	19.761	ng/u1	0.00
81) Pyrene-d10	19.674	212	2757014	18.395	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.751	264	2967923	19.531	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	123006	7.827	ng/uL#	92
5) Pyridine	3.775	79	852630	20.062	ng/u1	95
6) Benzaldehyde	7.075	77	404504	19.704	ng/u1	98
8) Phenol	7.128	94	1050759	19.822	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.357	93	844187	19.403	ng/u1	95
12) 2-Chlorophenol	7.499	128	842852	19.915	ng/u1	95
13) 2-Methylphenol	8.387	108	780724	18.892	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.469	45	1248626	20.914	ng/u1	97
16) Acetophenone	8.769	105	1238845	18.808	ng/u1	95
17) N-Nitroso-di-n-propyla...	8.752	70	625290	18.878	ng/u1	94
18) 4-Methylphenol	8.716	108	833048	18.199	ng/u1	98
19) Hexachloroethane	9.022	117	328770	19.439	ng/u1	98
22) Nitrobenzene	9.151	77	930034	21.723	ng/u1	97
23) Isophorone	9.675	82	1663948	19.221	ng/u1	97
25) 2-Nitrophenol	9.863	139	456188	20.498	ng/u1	93
26) 2,4-Dimethylphenol	9.922	107	878014	20.220	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.157	93	1059427	19.139	ng/u1	99
29) 2,4-Dichlorophenol	10.398	162	765936	19.599	ng/u1	99
30) Naphthalene	10.804	128	2541706	19.571	ng/u1	100
32) 4-Chloroaniline	10.916	127	946309	16.979	ng/u1	99
33) Hexachlorobutadiene	11.081	225	573308	21.365	ng/u1	100
34) Caprolactam	11.698	113	189349	14.209	ng/u1	96
35) 4-Chloro-3-methylphenol	12.040	107	683751	17.144	ng/u1	99
36) 2-Methylnaphthalene	12.410	142	1581464	17.751	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013326.D
 Acq On : 25 Dec 2022 07:02
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 21:38:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.628	142	1607793	17.548	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.775	216	949054	23.232	ng/ul	99
40) Hexachlorocyclopentadiene	12.751	237	232207	8.735	ng/ul	100
41) 2,4,6-Trichlorophenol	13.016	196	561542	21.389	ng/ul	100
42) 2,4,5-Trichlorophenol	13.092	196	586826	20.809	ng/ul	98
43) 1,1'-Biphenyl	13.416	154	2034107	21.349	ng/ul	99
44) 2-Chloronaphthalene	13.457	162	1594835	21.268	ng/ul	99
45) 2-Nitroaniline	13.669	65	400683	22.038	ng/ul	97
47) Dimethylphthalate	14.039	163	1827532	18.911	ng/ul	99
48) 2,6-Dinitrotoluene	14.163	165	345690	19.249	ng/ul	99
50) Acenaphthylene	14.304	152	2294442	19.920	ng/ul	99
51) 3-Nitroaniline	14.492	138	315899	18.628	ng/ul	96
52) Acenaphthene	14.645	153	1552437	19.450	ng/ul	99
53) 2,4-Dinitrophenol	14.698	184	120419	9.809	ng/ul	96
55) 4-Nitrophenol	14.804	109	216429	18.086	ng/ul	93
56) Dibenzofuran	14.981	168	2144091	18.893	ng/ul	99
57) 2,4-Dinitrotoluene	14.951	165	460061	17.636	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.210	232	468568	18.207	ng/ul	99
59) Diethylphthalate	15.398	149	1620005	17.245	ng/ul	99
61) Fluorene	15.634	166	1685504	18.519	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.628	204	897550	18.648	ng/ul	100
63) 4-Nitroaniline	15.657	138	275386	18.455	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.716	198	207170	13.530	ng/ul#	97
67) N-Nitrosodiphenylamine	15.839	169	1366449	20.243	ng/ul	99
68) 4-Bromophenyl-phenylether	16.522	248	528473	19.987	ng/ul	98
69) Hexachlorobenzene	16.639	284	617500	19.668	ng/ul	98
70) Atrazine	16.798	200	478313	18.183	ng/ul	99
71) Pentachlorophenol	16.992	266	364878	19.191	ng/ul	99
72) Phenanthrene	17.386	178	2505850	19.759	ng/ul	100
74) Anthracene	17.475	178	2539072	20.051	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.381	216	893793	25.730	ng/uL	99
76) Pentachlorobenzene	14.904	250	788949	22.276	ng/uL	98
77) Carbazole	17.751	167	2244824	21.050	ng/ul	100
78) Di-n-butylphthalate	18.286	149	2339352	18.017	ng/ul	100
80) Fluoranthene	19.351	202	3107526	18.268	ng/ul	98
82) Pyrene	19.704	202	3307274	18.848	ng/ul	98
83) Butylbenzylphthalate	20.569	149	1180465	17.414	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.345	252	1046365	17.739	ng/ul	98
85) Benzo(a)anthracene	21.416	228	3499773	20.191	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.321	149	1701821	17.797	ng/ul	99
87) Chrysene	21.468	228	3262240	19.902	ng/ul	99
89) Di-n-octyl phthalate	22.274	149	3104202	18.175	ng/ul	100
90) Benzo(b)fluoranthene	23.151	252	3776032	19.423	ng/ul	100
91) Benzo(k)fluoranthene	23.204	252	3488286	18.095	ng/ul	100
93) Benzo(a)pyrene	23.804	252	3287619	19.422	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.503	276	4414902	20.938	ng/ul	98
95) Dibenzo(a,h)anthracene	26.521	278	3677292	21.064	ng/ul	99
96) Benzo(g,h,i)perylene	27.303	276	3603538	21.288	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013326.D
 Acq On : 25 Dec 2022 07:02
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 21:38:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration




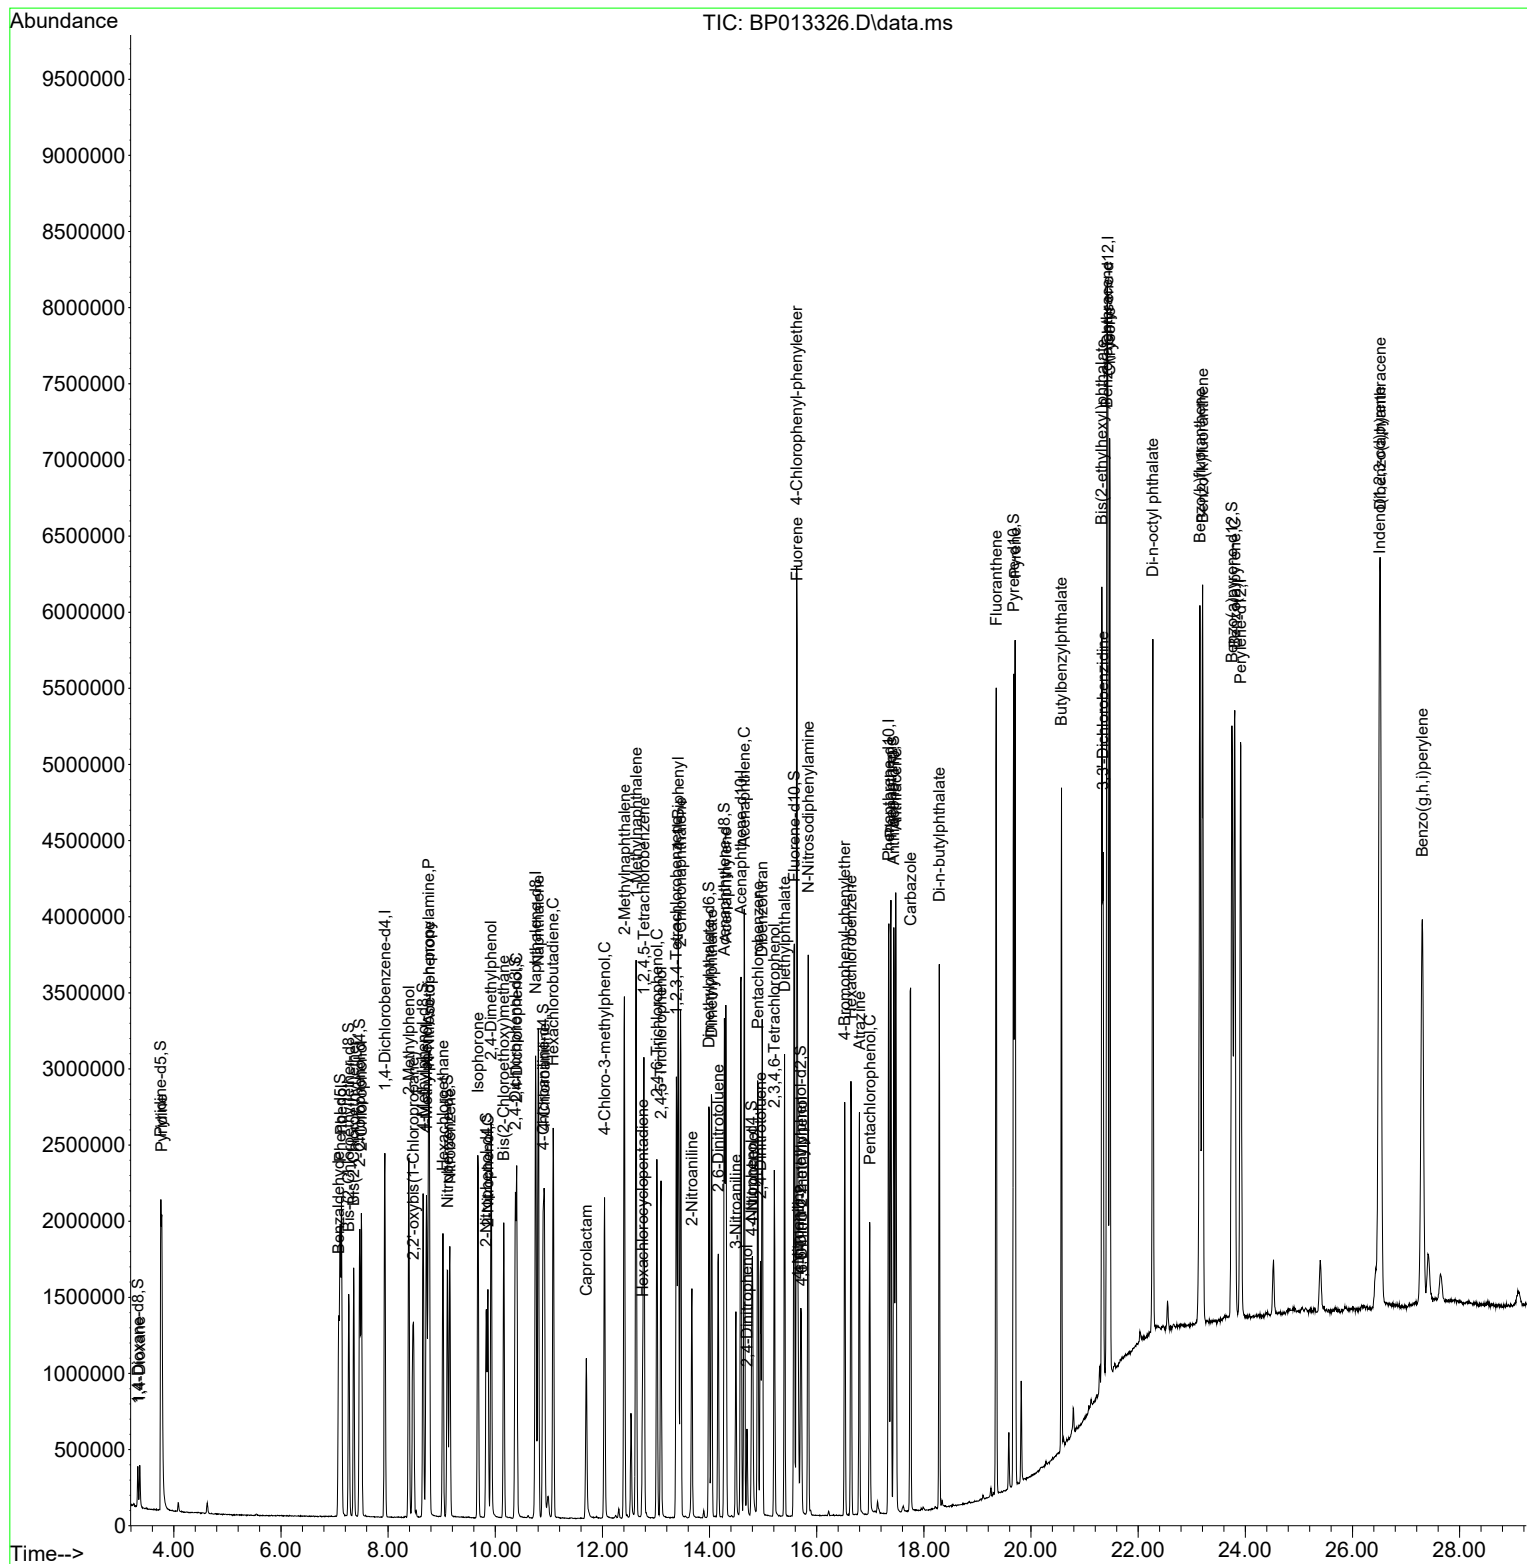


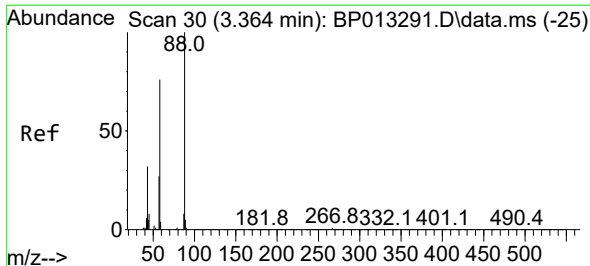

#2
 1,4-Dioxane
 Concen: 7.827 ng/uL
 RT: 3.364 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 88 Resp: 123006
 Ion Ratio Lower Upper
 88 100
 43 34.1 22.4 33.6#
 58 78.8 58.2 87.4

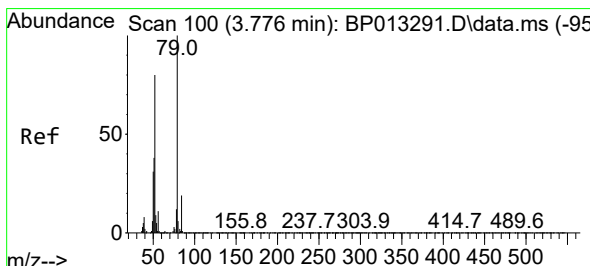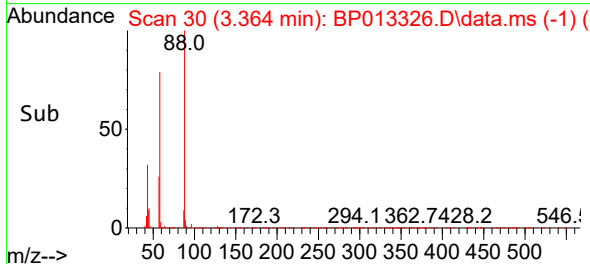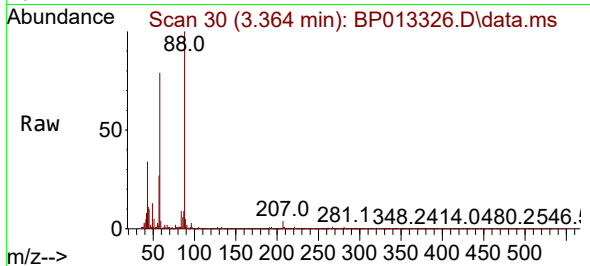

#5
 Pyridine
 Concen: 20.062 ng/uL
 RT: 3.775 min Scan# 100
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02

Tgt Ion: 79 Resp: 852630
 Ion Ratio Lower Upper
 79 100
 52 80.3 60.7 91.1
 51 39.2 28.9 43.3


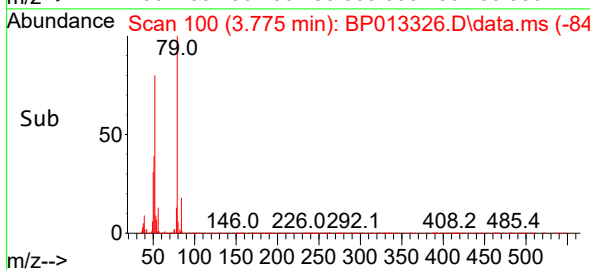

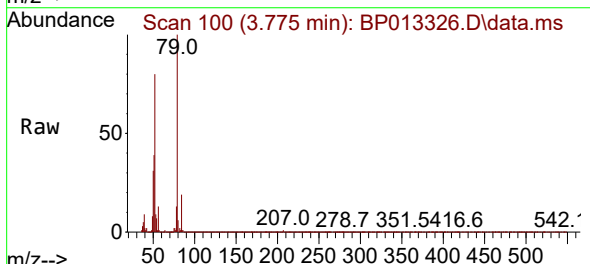




#6
Benzaldehyde
Concen: 19.704 ng/ul
RT: 7.075 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 404504
Ion Ratio Lower Upper
77 100
105 99.8 81.5 122.3
106 94.3 76.9 115.3



#8
Phenol
Concen: 19.822 ng/ul
RT: 7.128 min Scan# 670
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion: 94 Resp: 1050759
Ion Ratio Lower Upper
94 100
65 28.1 21.1 31.7
66 36.2 27.0 40.6



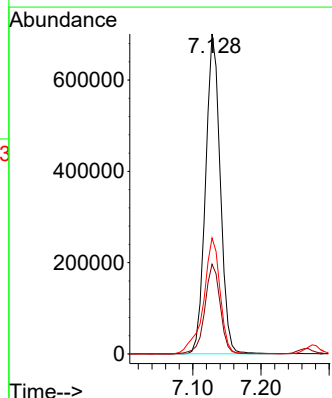





#10
 Bis(2-Chloroethyl)ether
 Concen: 19.403 ng/ul
 RT: 7.357 min Scan# 709
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 844187
 Ion Ratio Lower Upper
 93 100
 63 80.5 59.8 89.8
 95 32.0 26.4 39.6



#12
 2-Chlorophenol
 Concen: 19.915 ng/ul
 RT: 7.499 min Scan# 733
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02

Tgt Ion: 128 Resp: 842852
 Ion Ratio Lower Upper
 128 100
 64 48.4 34.9 52.3
 130 31.9 25.8 38.6

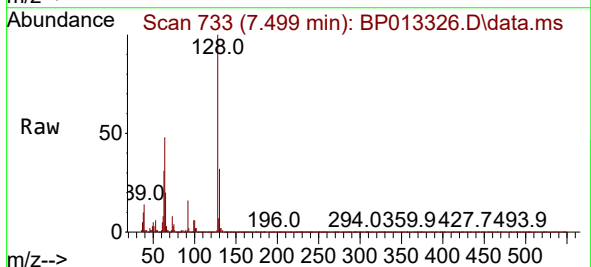



#13

2-Methylphenol

Concen: 18.892 ng/ul

RT: 8.387 min Scan# 884

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 780724

Ion Ratio Lower Upper

108 100

107 87.8 69.1 103.7

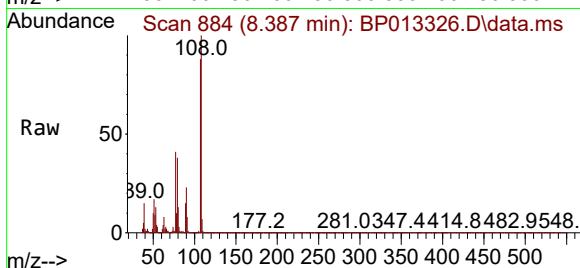

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.914 ng/ul

RT: 8.469 min Scan# 898

Delta R.T. -0.012 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion: 45 Resp: 1248626


Ion Ratio Lower Upper

45 100

77 12.8 11.0 16.6


79 10.1 9.3 13.9








#16
Acetophenone
Concen: 18.808 ng/ul
RT: 8.769 min Scan# 949
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:105 Resp: 1238845
Ion Ratio Lower Upper
105 100
77 77.3 59.3 88.9
51 28.3 19.6 29.4



#17
N-Nitroso-di-n-propylamine
Concen: 18.878 ng/ul
RT: 8.752 min Scan# 946
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion: 70 Resp: 625290
Ion Ratio Lower Upper
70 100
42 63.2 45.5 68.3
101 9.8 7.9 11.9
130 21.7 17.4 26.2



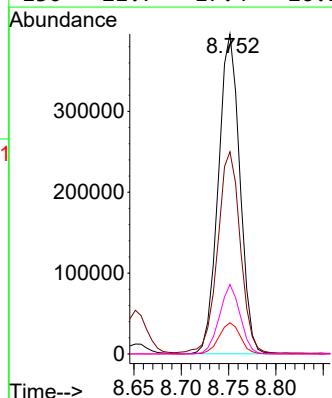





#18
4-Methylphenol
Concen: 18.199 ng/ul
RT: 8.716 min Scan# 940
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 833048
Ion Ratio Lower Upper
108 100
107 111.1 87.4 131.2



#19
Hexachloroethane
Concen: 19.439 ng/ul
RT: 9.022 min Scan# 992
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:117 Resp: 328770
Ion Ratio Lower Upper
117 100
201 116.0 93.7 140.5
199 71.3 58.6 88.0









#22
Nitrobenzene
Concen: 21.723 ng/ul
RT: 9.151 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 930034
Ion Ratio Lower Upper
77 100
123 45.6 38.3 57.5
65 12.8 10.3 15.5



#23
Isophorone
Concen: 19.221 ng/ul
RT: 9.675 min Scan# 1103
Delta R.T. -0.012 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion: 82 Resp: 1663948
Ion Ratio Lower Upper
82 100
95 6.7 5.4 8.2
138 17.6 15.3 22.9









#25
2-Nitrophenol
Concen: 20.498 ng/ul
RT: 9.863 min Scan# 1135
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:139 Resp: 456188
Ion Ratio Lower Upper
139 100
65 52.3 36.6 54.8
109 27.9 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 20.220 ng/ul
RT: 9.922 min Scan# 1145
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:107 Resp: 878014
Ion Ratio Lower Upper
107 100
121 49.1 41.8 62.6
122 87.0 72.6 108.8









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.139 ng/ul
 RT: 10.157 min Scan# 1185
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 1059427
 Ion Ratio Lower Upper
 93 100
 95 32.0 26.0 39.0
 123 11.0 9.2 13.8



#29
 2,4-Dichlorophenol
 Concen: 19.599 ng/ul
 RT: 10.398 min Scan# 1226
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02

Tgt Ion:162 Resp: 765936
 Ion Ratio Lower Upper
 162 100
 164 65.5 52.5 78.7
 98 34.0 26.6 39.8




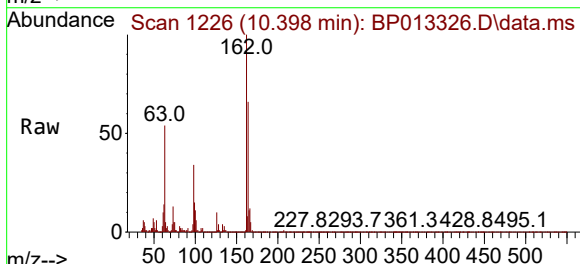




#30
Naphthalene
Concen: 19.571 ng/ul
RT: 10.804 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 2541706
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 13.2 10.4 15.6

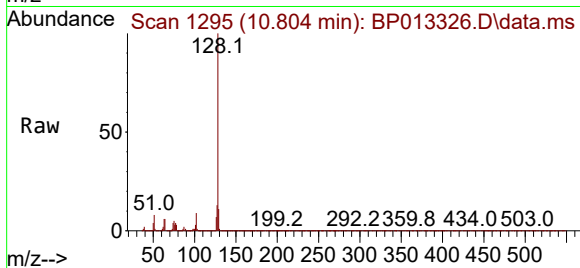

#32
4-Chloroaniline
Concen: 16.979 ng/ul
RT: 10.916 min Scan# 1314
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:127 Resp: 946309
Ion Ratio Lower Upper
127 100
129 31.4 25.6 38.4


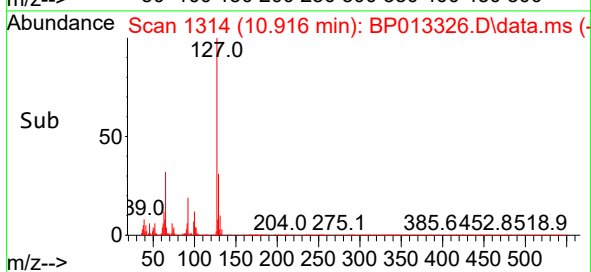






#33
Hexachlorobutadiene
Concen: 21.365 ng/ul
RT: 11.081 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:225 Resp: 573308
Ion Ratio Lower Upper
225 100
223 61.2 49.2 73.8
227 63.1 50.2 75.2



#34
Caprolactam
Concen: 14.209 ng/ul
RT: 11.698 min Scan# 1447
Delta R.T. -0.012 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:113 Resp: 189349
Ion Ratio Lower Upper
113 100
55 179.2 141.9 212.9
56 133.6 99.6 149.4




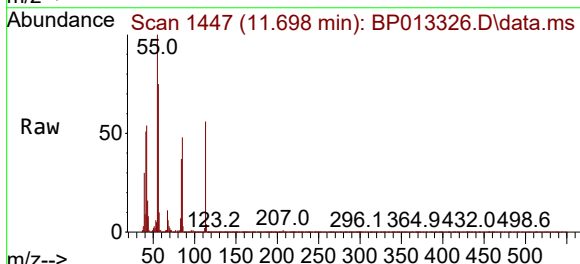




#35
4-Chloro-3-methylphenol
Concen: 17.144 ng/ul
RT: 12.040 min Scan# 1505
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:107 Resp: 683751
Ion Ratio Lower Upper
107 100
144 26.7 21.4 32.2
142 81.2 65.8 98.6



#36
2-Methylnaphthalene
Concen: 17.751 ng/ul
RT: 12.410 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:142 Resp: 1581464
Ion Ratio Lower Upper
142 100
141 88.8 70.8 106.2





#37

1-Methylnaphthalene

Concen: 17.548 ng/ul

RT: 12.628 min Scan# 1605

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:142 Resp: 1607793

Ion Ratio Lower Upper

142 100

141 91.3 72.7 109.1

116 3.7 2.7 4.1

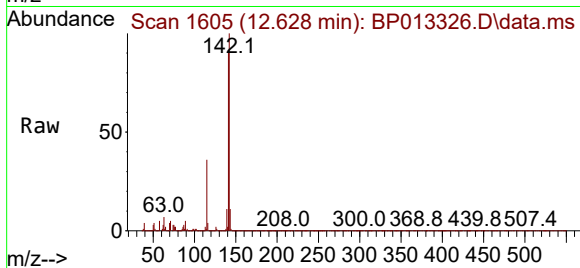

#39

1,2,4,5-Tetrachlorobenzene

Concen: 23.232 ng/ul

RT: 12.775 min Scan# 1630

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Tgt Ion:216 Resp: 949054




Ion Ratio Lower Upper


216 100

214 77.2 61.9 92.9

179 19.4 15.0 22.6

108 14.3 11.0 16.4





#40

Hexachlorocyclopentadiene

Concen: 8.735 ng/ul

RT: 12.751 min Scan# 1626

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 232207

Ion Ratio Lower Upper

237 100

235 61.8 49.7 74.5

272 13.2 10.8 16.2

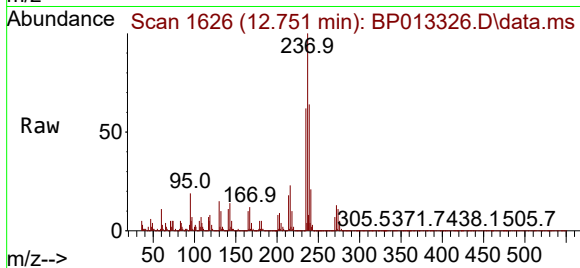

#41

2,4,6-Trichlorophenol

Concen: 21.389 ng/ul

RT: 13.016 min Scan# 1671

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:196 Resp: 561542


Ion Ratio Lower Upper

196 100

198 96.2 77.0 115.6


200 31.0 25.3 37.9








#42
2,4,5-Trichlorophenol
Concen: 20.809 ng/ul
RT: 13.092 min Scan# 1
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:196 Resp: 586826
Ion Ratio Lower Upper
196 100
198 94.2 77.1 115.7
200 30.5 25.4 38.2



#43
1,1'-Biphenyl
Concen: 21.349 ng/ul
RT: 13.416 min Scan# 1739
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:154 Resp: 2034107
Ion Ratio Lower Upper
154 100
153 40.1 31.5 47.3
76 12.3 9.6 14.4





#44

2-Chloronaphthalene

Concen: 21.268 ng/ul

RT: 13.457 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:162 Resp: 1594835

Ion Ratio Lower Upper

162 100

164 32.8 26.3 39.5

127 37.2 29.3 43.9

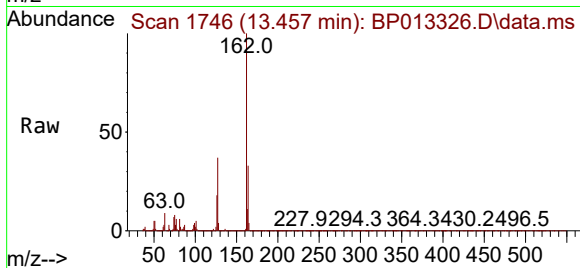

#45

2-Nitroaniline

Concen: 22.038 ng/ul

RT: 13.669 min Scan# 1782

Delta R.T. 0.000 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion: 65 Resp: 400683


Ion Ratio Lower Upper

65 100

92 68.8 56.4 84.6

138 109.5 90.3 135.5









#47
Dimethylphthalate
Concen: 18.911 ng/ul
RT: 14.039 min Scan# 1845
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:163 Resp: 1827532
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 9.7 8.3 12.5

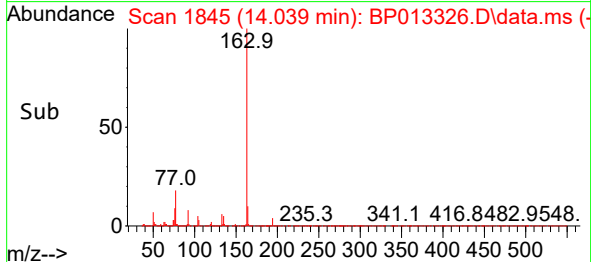

#48
2,6-Dinitrotoluene
Concen: 19.249 ng/ul
RT: 14.163 min Scan# 1866
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:165 Resp: 345690
Ion Ratio Lower Upper
165 100
89 54.0 43.0 64.4
121 19.3 16.1 24.1









#50
Acenaphthylene
Concen: 19.920 ng/ul
RT: 14.304 min Scan# 1891
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:152 Resp: 2294442
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.6
153 13.4 10.6 16.0

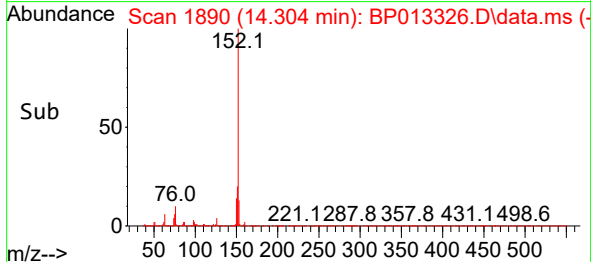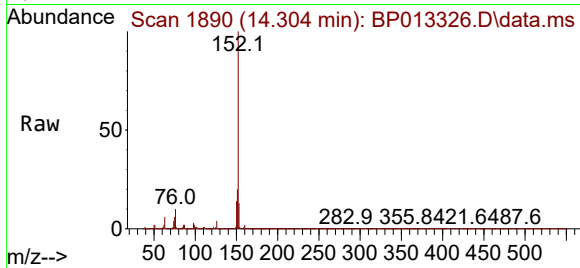

#51
3-Nitroaniline
Concen: 18.628 ng/ul
RT: 14.492 min Scan# 1922
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:138 Resp: 315899
Ion Ratio Lower Upper
138 100
108 10.5 8.6 13.0
92 114.5 88.4 132.6


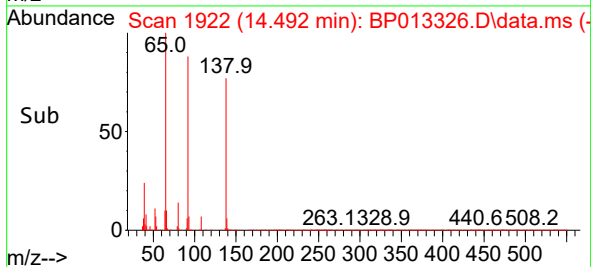

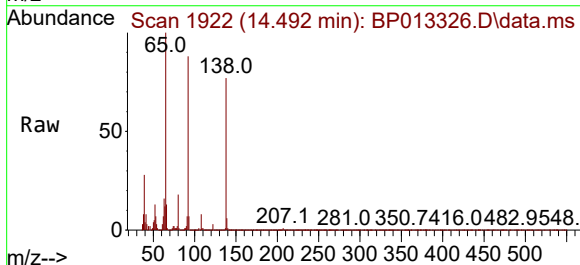




#52
Acenaphthene
Concen: 19.450 ng/ul
RT: 14.645 min Scan# 1948
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:153 Resp: 1552437
Ion Ratio Lower Upper
153 100
152 47.6 38.2 57.4
154 90.2 70.8 106.2



#53
2,4-Dinitrophenol
Concen: 9.809 ng/ul
RT: 14.698 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:184 Resp: 120419
Ion Ratio Lower Upper
184 100
63 64.5 48.4 72.6
154 59.1 45.5 68.3



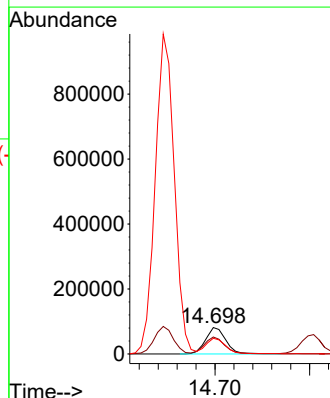
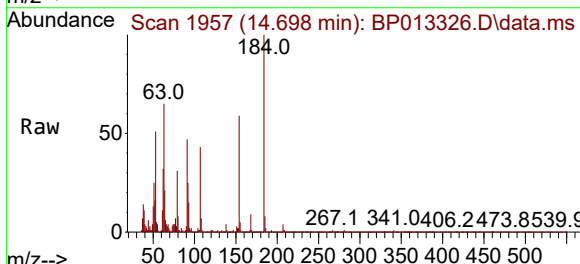




#55
4-Nitrophenol
Concen: 18.086 ng/ul
RT: 14.804 min Scan# 1975
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:109 Resp: 216429
Ion Ratio Lower Upper
109 100
139 139.6 120.8 181.2
65 140.5 107.9 161.9

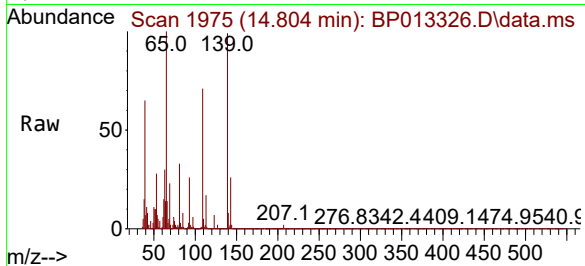

#56
Dibenzofuran
Concen: 18.893 ng/ul
RT: 14.981 min Scan# 2005
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:168 Resp: 2144091
Ion Ratio Lower Upper
168 100
139 35.4 27.9 41.9




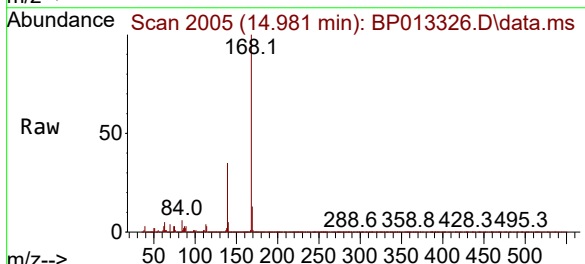




#57
 2,4-Dinitrotoluene
 Concen: 17.636 ng/ul
 RT: 14.951 min Scan# 2000
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion:165 Resp: 460061
 Ion Ratio Lower Upper
 165 100
 63 41.8 31.8 47.6
 182 2.7 2.1 3.1



#58
 2,3,4,6-Tetrachlorophenol
 Concen: 18.207 ng/ul
 RT: 15.210 min Scan# 2044
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02

Tgt Ion:232 Resp: 468568
 Ion Ratio Lower Upper
 232 100
 131 38.6 31.8 47.6
 130 2.1 1.8 2.6
 166 28.1 22.9 34.3




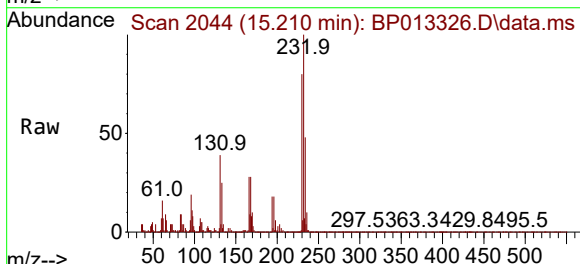




#59
Diethylphthalate
Concen: 17.245 ng/ul
RT: 15.398 min Scan# 2077
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:149 Resp: 1620005
Ion Ratio Lower Upper
149 100
177 23.5 18.4 27.6
150 12.6 9.9 14.9

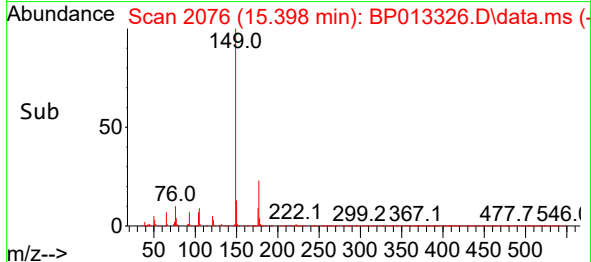

#61
Fluorene
Concen: 18.519 ng/ul
RT: 15.634 min Scan# 2116
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:166 Resp: 1685504
Ion Ratio Lower Upper
166 100
165 97.0 77.4 116.2
167 13.4 10.6 16.0


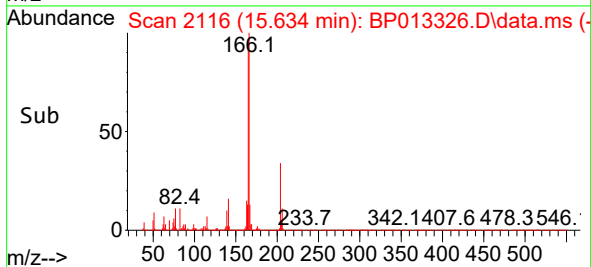

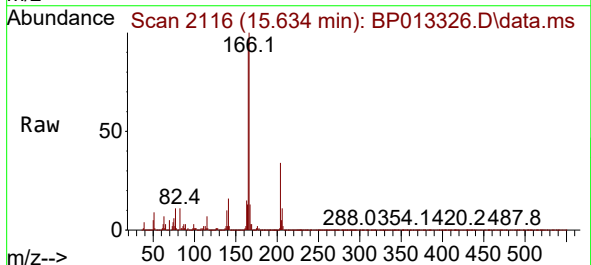




#62
4-Chlorophenyl-phenylether
Concen: 18.648 ng/ul
RT: 15.628 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 897550
Ion Ratio Lower Upper
204 100
206 32.9 26.3 39.5
141 50.0 40.4 60.6



#63
4-Nitroaniline
Concen: 18.455 ng/ul
RT: 15.657 min Scan# 2120
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:138 Resp: 275386
Ion Ratio Lower Upper
138 100
92 51.3 39.0 58.4
108 77.4 55.1 82.7




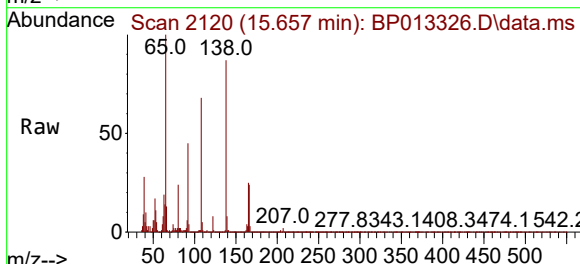


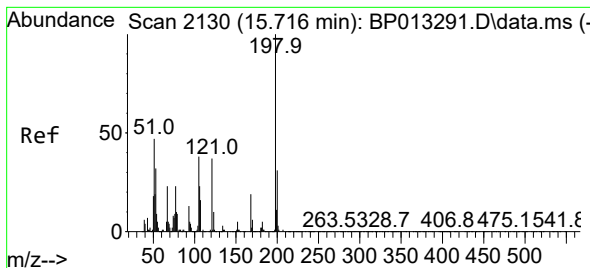

#66
4,6-Dinitro-2-methylphenol
Concen: 13.530 ng/ul
RT: 15.716 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 207170
Ion Ratio Lower Upper
198 100
182 5.0 3.3 4.9#
77 22.3 16.6 25.0

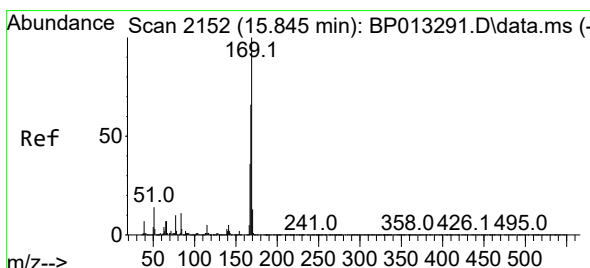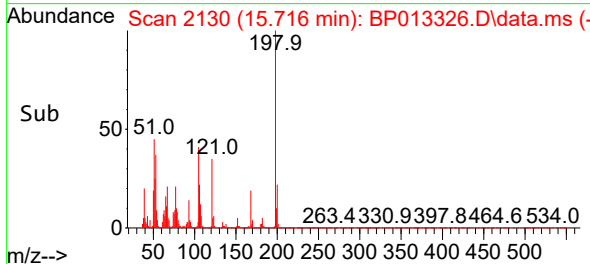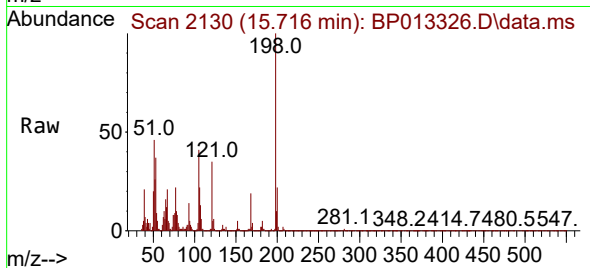

#67
N-Nitrosodiphenylamine
Concen: 20.243 ng/ul
RT: 15.839 min Scan# 2151
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:169 Resp: 1366449
Ion Ratio Lower Upper
169 100
168 65.9 53.0 79.6
167 36.1 29.1 43.7


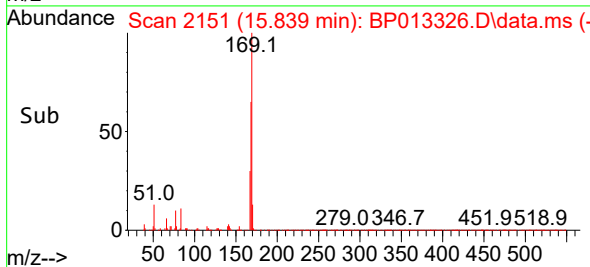

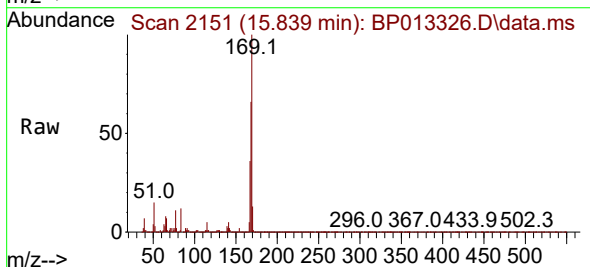




#68
4-Bromophenyl-phenylether
Concen: 19.987 ng/ul
RT: 16.522 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 528473
Ion Ratio Lower Upper
248 100
250 96.2 77.4 116.0
141 63.1 48.3 72.5



#69
Hexachlorobenzene
Concen: 19.668 ng/ul
RT: 16.639 min Scan# 2287
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:284 Resp: 617500
Ion Ratio Lower Upper
284 100
142 30.4 22.6 34.0
249 30.7 24.6 37.0




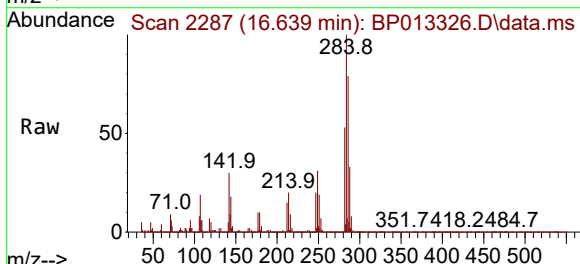




#70
Atrazine
Concen: 18.183 ng/ul
RT: 16.798 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:200 Resp: 478313
Ion Ratio Lower Upper
200 100
173 25.7 20.5 30.7
215 50.6 39.9 59.9

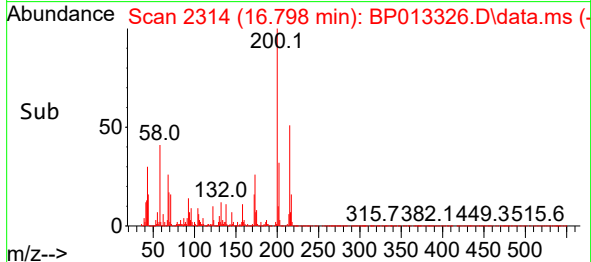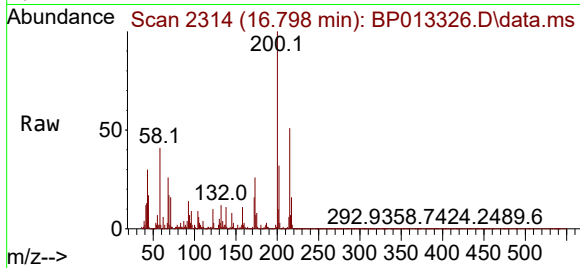

#71
Pentachlorophenol
Concen: 19.191 ng/ul
RT: 16.992 min Scan# 2347
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:266 Resp: 364878
Ion Ratio Lower Upper
266 100
264 63.8 50.9 76.3
268 65.2 51.4 77.2

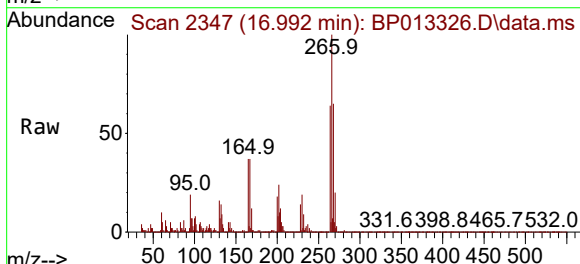



#72

Phenanthrene

Concen: 19.759 ng/ul

RT: 17.386 min Scan# 2414

Delta R.T. 0.000 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 2505850

Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7

176 19.0 15.4 23.0



#74

Anthracene

Concen: 20.051 ng/ul

RT: 17.475 min Scan# 2429

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:178 Resp: 2539072


Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 18.6 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 25.730 ng/uL
RT: 13.381 min Scan# 1733
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:216 Resp: 893793
Ion Ratio Lower Upper
216 100
214 77.5 62.2 93.2
218 47.9 38.9 58.3



#76
Pentachlorobenzene
Concen: 22.276 ng/uL
RT: 14.904 min Scan# 1992
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:250 Resp: 788949
Ion Ratio Lower Upper
250 100
248 61.4 50.6 76.0
252 64.6 51.1 76.7



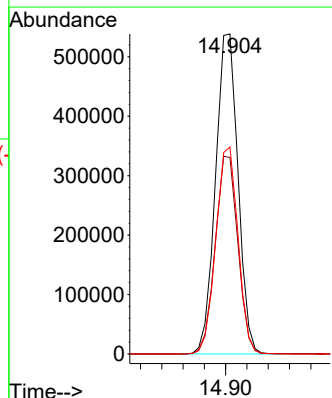
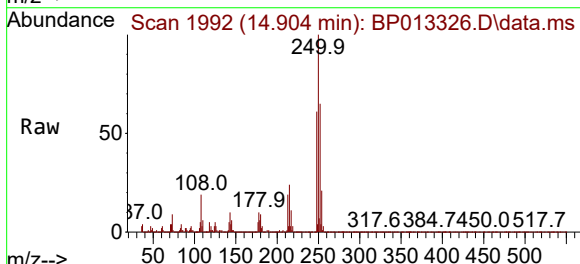




#77
 Carbazole
 Concen: 21.050 ng/ul
 RT: 17.751 min Scan# 2476
 Delta R.T. 0.000 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion:167 Resp: 2244824
 Ion Ratio Lower Upper
 167 100
 166 21.7 17.2 25.8
 139 11.9 9.4 14.2



#78
 Di-n-butylphthalate
 Concen: 18.017 ng/ul
 RT: 18.286 min Scan# 2567
 Delta R.T. -0.006 min
 Lab File: BP013326.D
 Acq: 25 Dec 2022 07:02

Tgt Ion:149 Resp: 2339352
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.5 11.3
 104 4.8 3.8 5.6





#80

Fluoranthene

Concen: 18.268 ng/ul

RT: 19.351 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:202 Resp: 3107526

Ion Ratio Lower Upper

202 100

101 9.2 8.2 12.2

100 7.3 6.1 9.1

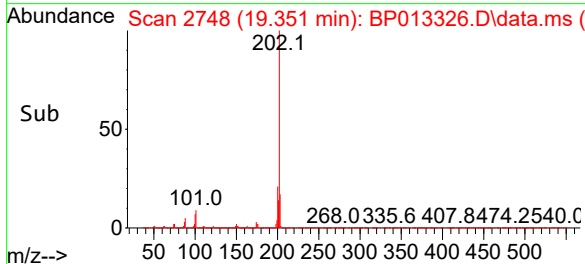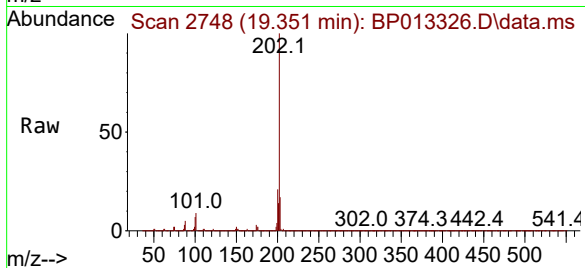

#82

Pyrene

Concen: 18.848 ng/ul

RT: 19.704 min Scan# 2808

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:202 Resp: 3307274


Ion Ratio Lower Upper

202 100

101 11.2 9.4 14.2

100 9.1 7.8 11.8

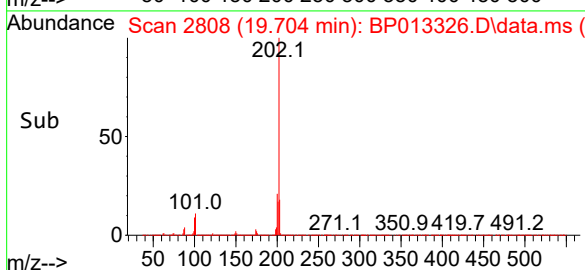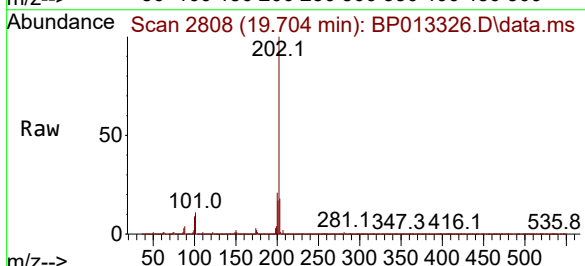



#83

Butylbenzylphthalate

Concen: 17.414 ng/ul

RT: 20.569 min Scan# 2956

Delta R.T. 0.000 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 1180465

Ion Ratio Lower Upper

149 100

91 67.9 53.4 80.0

206 22.6 17.9 26.9



#84

3,3'-Dichlorobenzidine

Concen: 17.739 ng/ul

RT: 21.345 min Scan# 3087

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:252 Resp: 1046365


Ion Ratio Lower Upper

252 100

254 63.3 51.8 77.8

126 9.2 7.4 11.2





#85

Benzo(a)anthracene

Concen: 20.191 ng/ul

RT: 21.416 min Scan# 3099

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 3499773

Ion Ratio Lower Upper

228 100

229 19.8 16.1 24.1

226 27.3 22.0 33.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 17.797 ng/ul

RT: 21.321 min Scan# 3083

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:149 Resp: 1701821


Ion Ratio Lower Upper

149 100

167 27.8 22.5 33.7

279 4.6 3.8 5.8





#87

Chrysene

Concen: 19.902 ng/ul

RT: 21.468 min Scan# 3109

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:228 Resp: 3262240

Ion Ratio Lower Upper

228 100

226 30.1 24.5 36.7

229 19.9 16.0 24.0

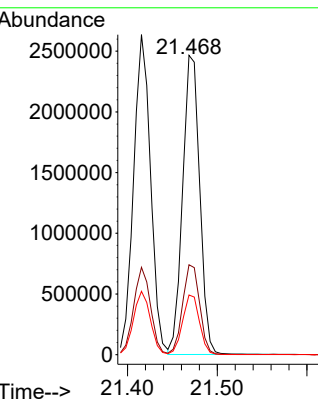

#89

Di-n-octyl phthalate

Concen: 18.175 ng/ul




RT: 22.274 min Scan# 3245


Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Tgt Ion:149 Resp: 3104202



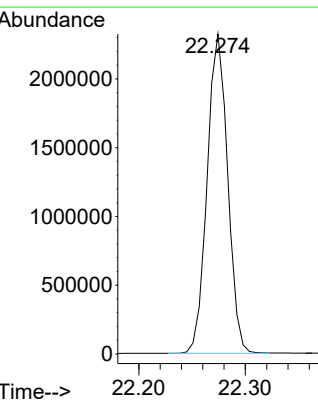
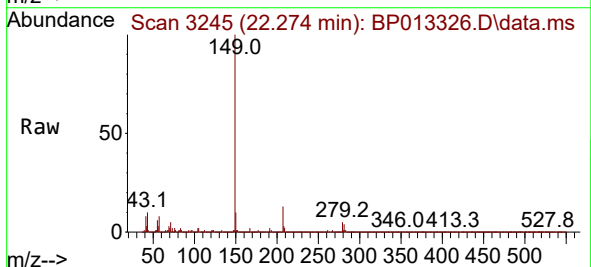




#90
Benzo(b)fluoranthene
Concen: 19.423 ng/ul
RT: 23.151 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:252 Resp: 3776032
Ion Ratio Lower Upper
252 100
253 22.1 17.7 26.5
125 8.9 6.8 10.2

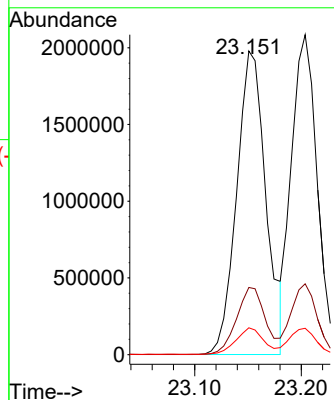

#91
Benzo(k)fluoranthene
Concen: 18.095 ng/ul
RT: 23.204 min Scan# 3403
Delta R.T. 0.000 min
Lab File: BP013326.D
Acq: 25 Dec 2022 07:02

Tgt Ion:252 Resp: 3488286
Ion Ratio Lower Upper
252 100
253 22.2 17.7 26.5
125 8.2 6.8 10.2

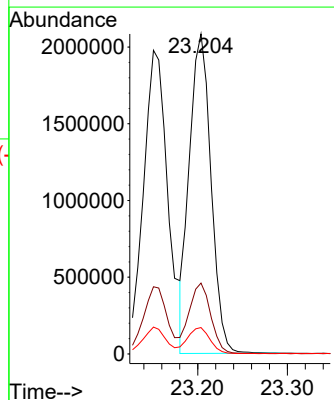



#93

Benzo(a)pyrene

Concen: 19.422 ng/ul

RT: 23.804 min Scan# 3

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 3287619

Ion Ratio Lower Upper

252 100

253 21.8 17.5 26.3

125 9.3 7.5 11.3

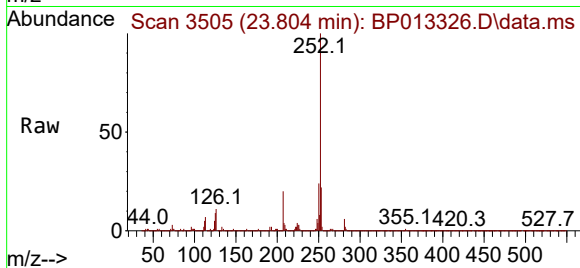

#94

Indeno(1,2,3-cd)pyrene

Concen: 20.938 ng/ul

RT: 26.503 min Scan# 3964

Delta R.T. -0.012 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02




Tgt Ion:276 Resp: 4414902


Ion Ratio Lower Upper

276 100

138 19.7 17.1 25.7

277 25.3 20.0 30.0

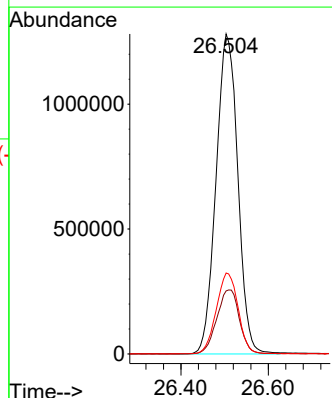



#95

Dibenzo(a,h)anthracene

Concen: 21.064 ng/ul

RT: 26.521 min Scan# 3970

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:278 Resp: 3677292

Ion Ratio Lower Upper

278 100

139 13.2 11.1 16.7

279 23.8 19.0 28.6



#96

Benzo(g,h,i)perylene

Concen: 21.288 ng/ul

RT: 27.303 min Scan# 4100

Delta R.T. -0.006 min

Lab File: BP013326.D

Acq: 25 Dec 2022 07:02

Tgt Ion:276 Resp: 3603538

Ion Ratio Lower Upper

276 100

138 17.7 15.4 23.2

277 23.8 19.1 28.7

