

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013333.D
 Acq On : 25 Dec 2022 10:58
 Operator : CG/JU
 Sample : N6187-08
 Misc : GCMS CONFIRMATION
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 25 21:40:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	568391	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.752	136	2237123	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	1204691	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2116077	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	1876049	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	2265872	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	256	0.019	ng/uL	-0.01
4) Pyridine-d5	3.752	84	801	0.021	ng/ul	0.00
7) Phenol-d5	7.099	99	62	0.001	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.275	67	245	0.009	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	122	0.003	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	15	0.000	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	48	0.003	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	121	0.007	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.387	165	204	0.006	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	287	0.006	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	106	0.001	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	338	0.003	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	207	0.012	ng/ul	0.00
60) Fluorene-d10	15.575	176	1415	0.018	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	8	0.001	ng/ul	0.00
73) Anthracene-d10	17.345	188	2116361	22.169	ng/ul	-0.10
81) Pyrene-d10	19.680	212	1681	0.016	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	3025	0.027	ng/ul	-0.02


Target Compounds					Qvalue	
52) Acenaphthene	14.698	153	122589	1.617	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013333.D
Acq On : 25 Dec 2022 10:58
Operator : CG/JU
Sample : N6187-08
Misc : GCMS CONFIRMATION
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 25 21:40:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

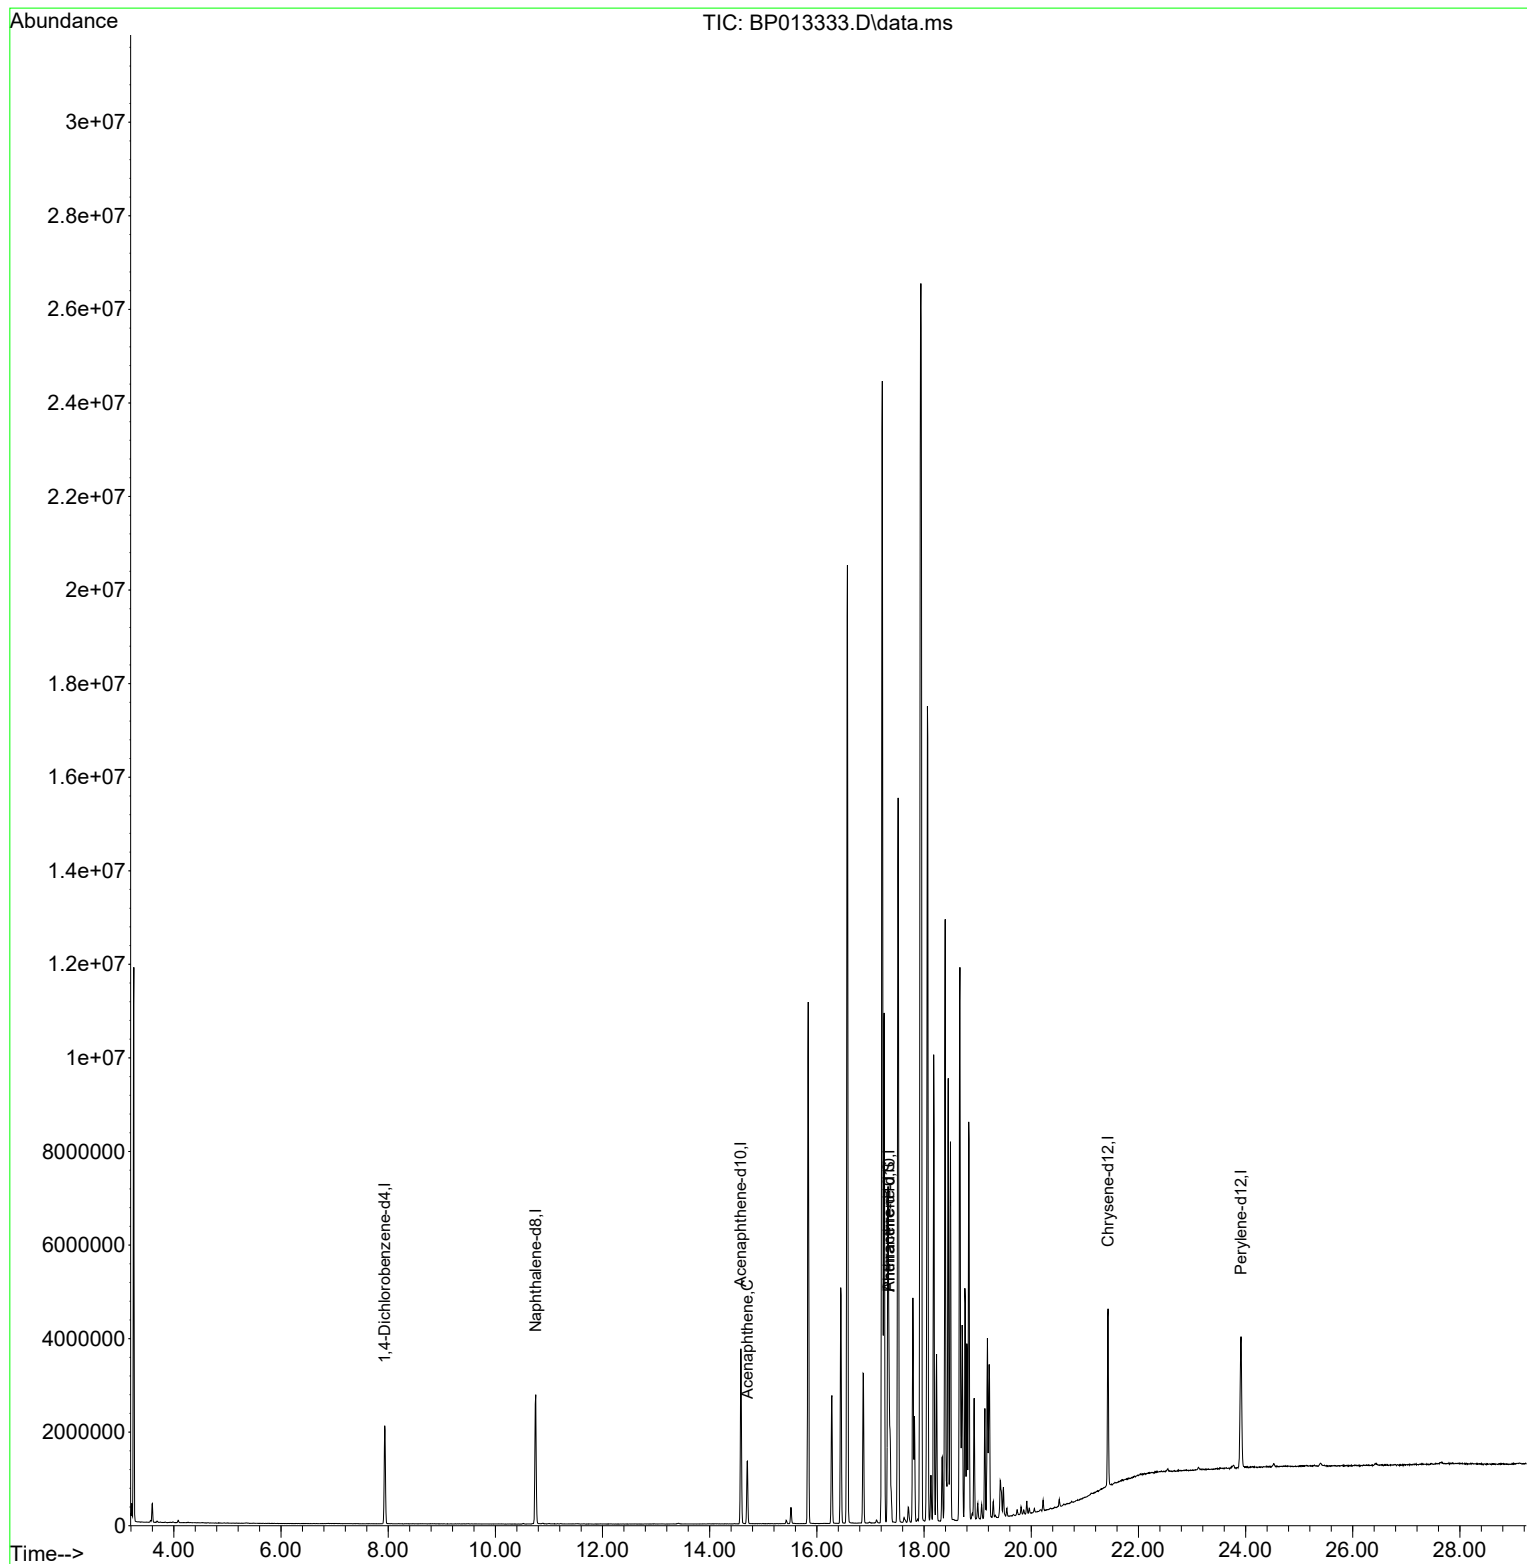

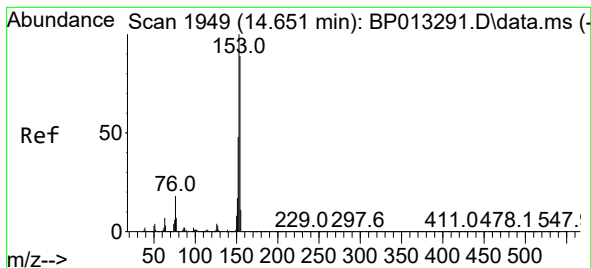

#52

Acenaphthene

Concen: 1.617 ng/ul

RT: 14.698 min Scan# 1957

Delta R.T. 0.047 min


Lab File: BP013333.D

Acq: 25 Dec 2022 10:58

Instrument :

BNA_P

ClientSampleId :

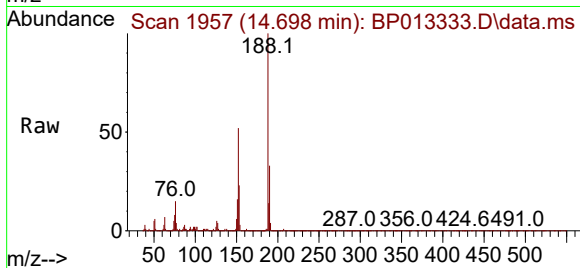

Tgt Ion:153 Resp: 122589

Ion Ratio Lower Upper

153 100

152 225.9 38.2 57.4#

154 11.6 70.8 106.2#

